

Data File : BG035286.D
Acq On : 21 Jun 2018 5:17
Operator : SJ/JU
Sample : J3247-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-01-061918

Quant Time: Jun 21 07:00:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	60484	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	205009	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	143162	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	391280	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	430402	20.00	ng	-0.03
86) Perylene-d12	24.91	264	411661	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	475142	132.57	ng	0.00
7) Phenol-d6	7.22	99	610315	115.38	ng	0.00
23) Nitrobenzene-d5	9.22	82	476663	110.52	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	324643	177.14	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	1054352	95.74	ng	-0.02
78) Terphenyl-d14	20.03	244	1947556	94.78	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG035286.D
Acq On : 21 Jun 2018 5:17
Operator : SJ/JU
Sample : J3247-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-01-061918

Quant Time: Jun 21 07:00:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

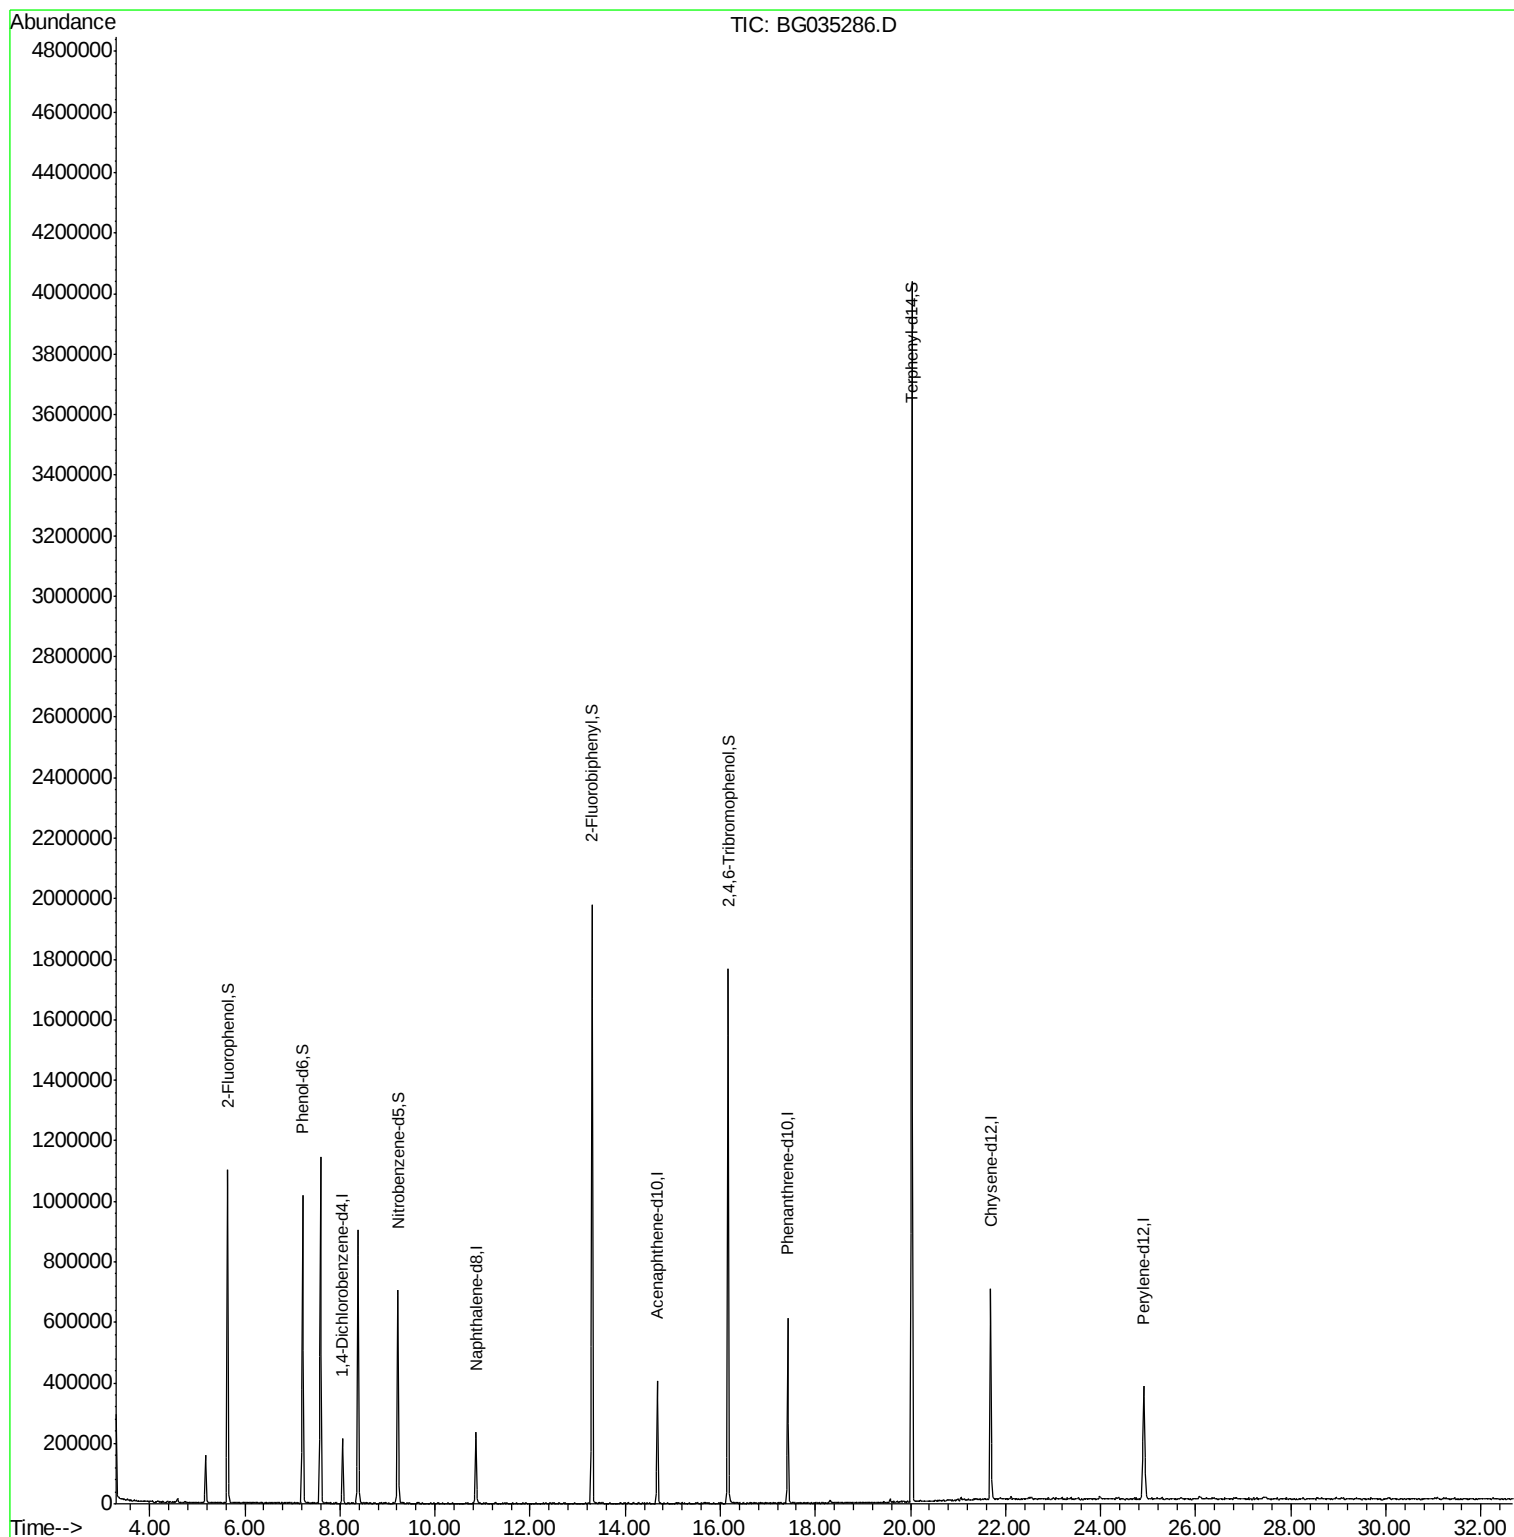

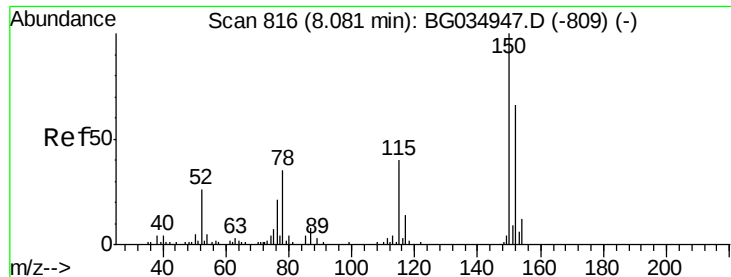


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 812
Delta R.T. -0.02 min
Lab File: BG035286.D
Acq: 21 Jun 2018 5:17

Instrument :
BNA_G
ClientSampleId :
OR-01-061918

Tgt Ion:152 Resp: 60484
Ion Ratio Lower Upper
152 100
150 157.6 126.6 189.8
115 61.6 53.0 79.4

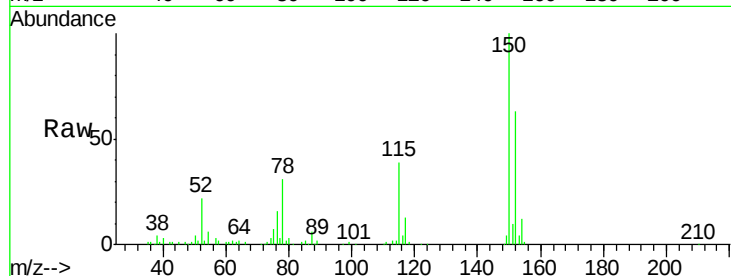


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

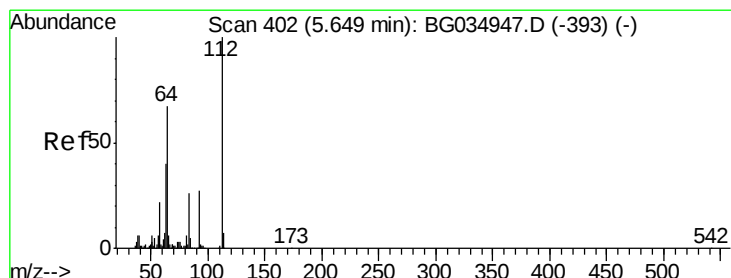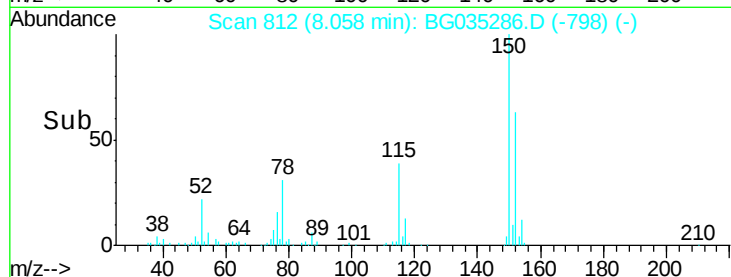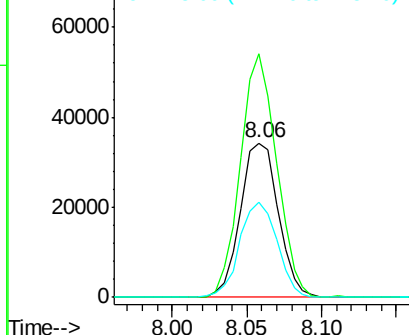



#5


2-Fluorophenol
Concen: 132.573 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG035286.D
Acq: 21 Jun 2018 5:17

Tgt Ion:112 Resp: 475142
Ion Ratio Lower Upper
112 100
64 62.8 56.3 84.5
63 35.3 30.1 45.1

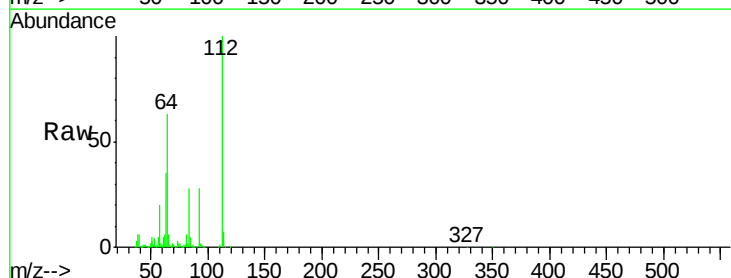

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

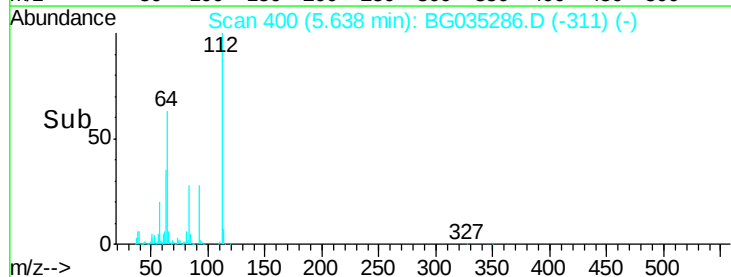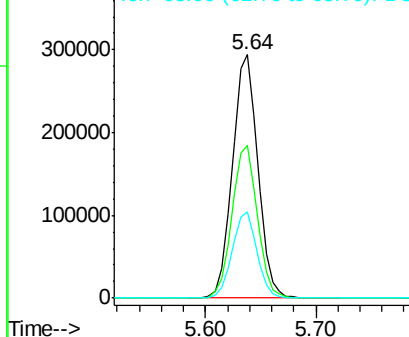

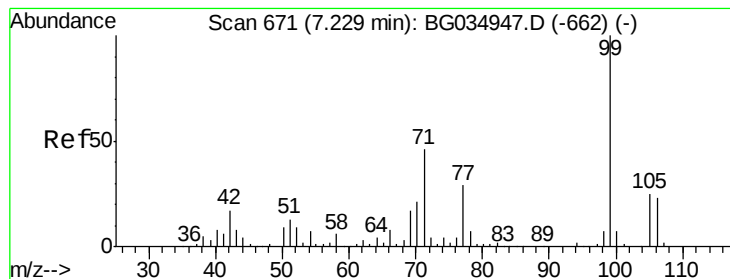

#7

Phenol-d6

Concen: 115.376 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG035286.D

Acq: 21 Jun 2018 5:17

Instrument :

BNA_G

ClientSampleId :

OR-01-061918


Tgt Ion: 99 Resp: 610315

Ion Ratio Lower Upper




99 100

42 15.2 14.1 21.1

71 40.5 26.1 39.1#

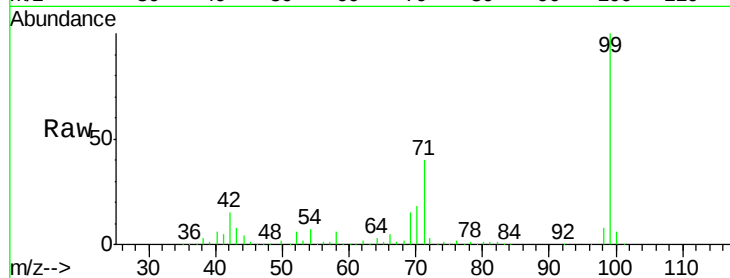

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

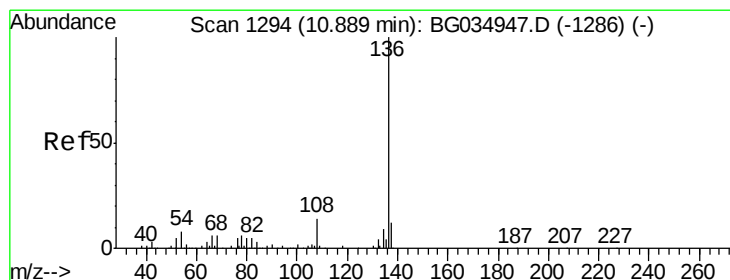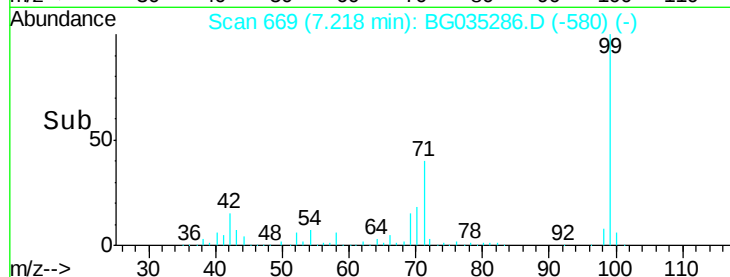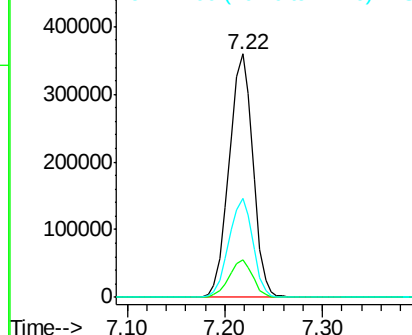

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.02 min

Lab File: BG035286.D

Acq: 21 Jun 2018 5:17

Tgt Ion: 136 Resp: 205009


Ion Ratio Lower Upper

136 100



137 9.9 9.2 13.8


54 6.9 10.3 15.5#

68 5.2 4.5 6.7

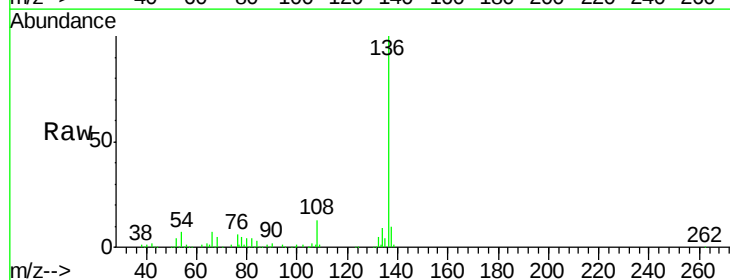

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



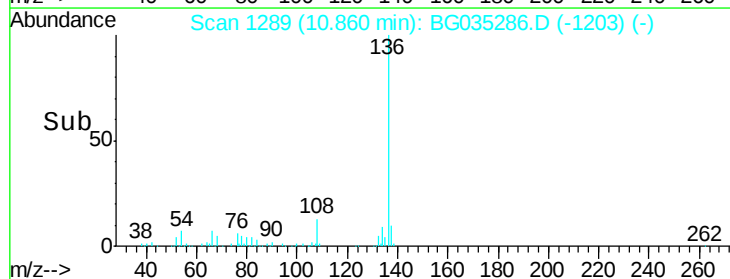
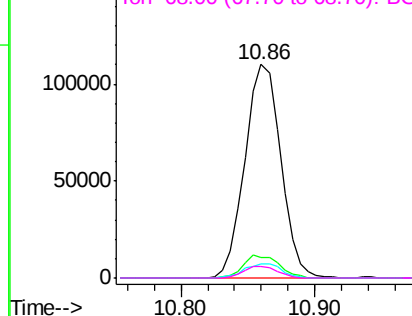


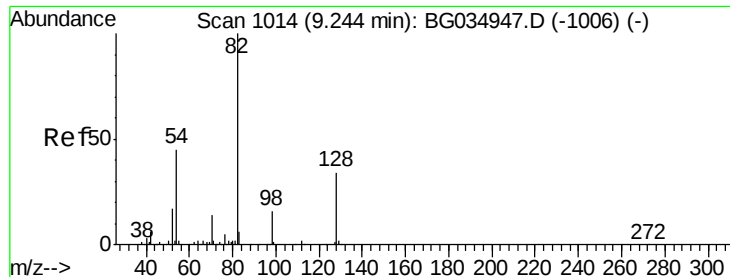

#23
 Nitrobenzene-d5
 Concen: 110.521 ng
 RT: 9.22 min Scan# 1010
 Delta R.T. -0.02 min
 Lab File: BG035286.D
 Acq: 21 Jun 2018 5:17




Instrument :
 BNA_G
 ClientSampleId :
 OR-01-061918


Tgt Ion: 82 Resp: 476663
 Ion Ratio Lower Upper
 82 100
 128 37.6 29.7 44.5
 54 42.1 43.1 64.7#

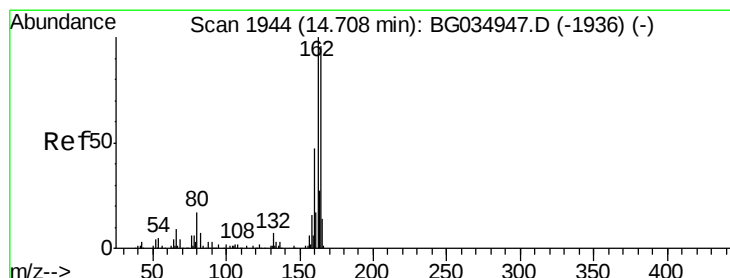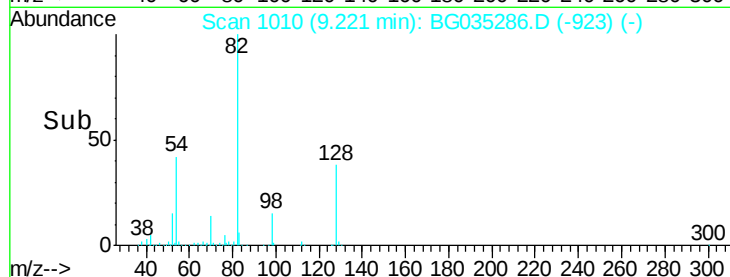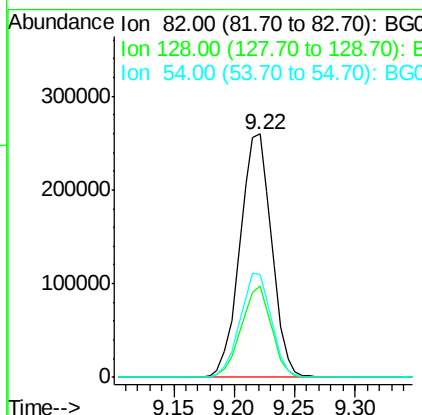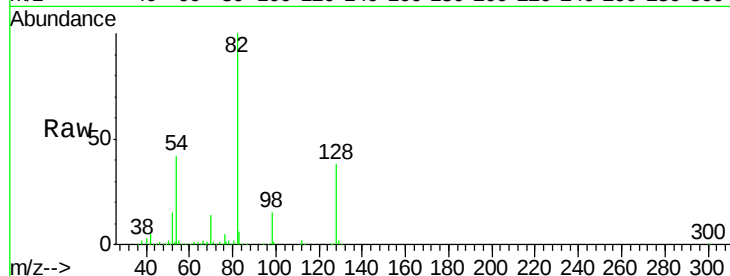

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1939
 Delta R.T. -0.02 min
 Lab File: BG035286.D
 Acq: 21 Jun 2018 5:17

Tgt Ion: 164 Resp: 143162
 Ion Ratio Lower Upper
 164 100
 162 96.7 78.8 118.2
 160 42.7 35.4 53.0

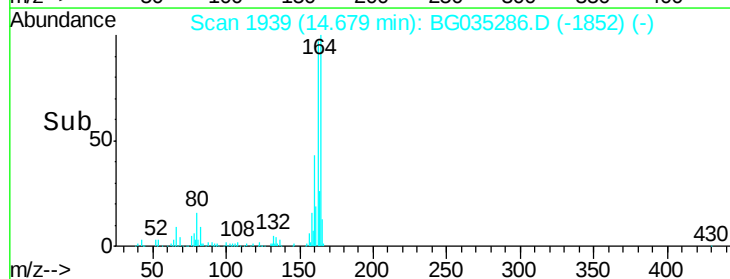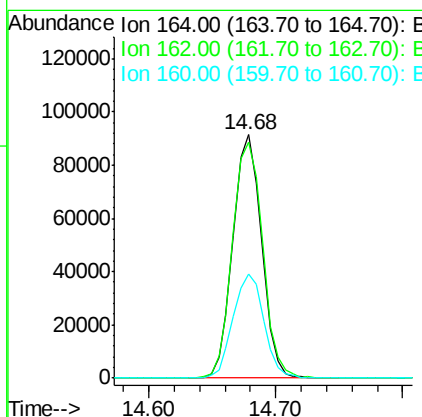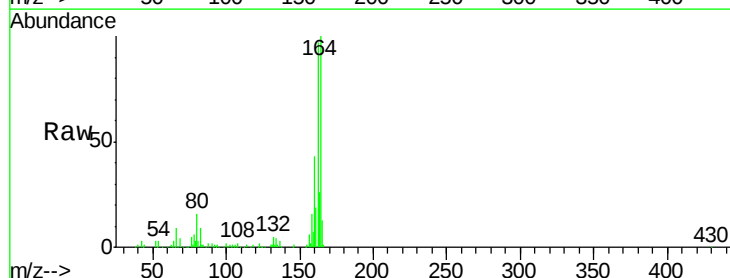


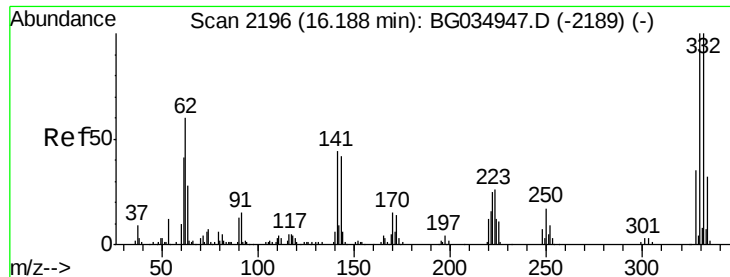




#41
 2,4,6-Tribromophenol
 Concen: 177.144 ng
 RT: 16.16 min Scan# 2192
 Delta R.T. -0.02 min
 Lab File: BG035286.D
 Acq: 21 Jun 2018 5:17

Instrument :
 BNA_G
 ClientSampleId :
 OR-01-061918

Tgt Ion:330 Resp: 324643
 Ion Ratio Lower Upper
 330 100
 332 97.8 77.0 115.6
 141 37.6 25.2 37.8

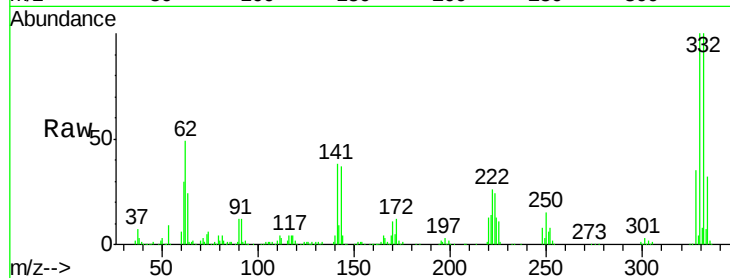


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

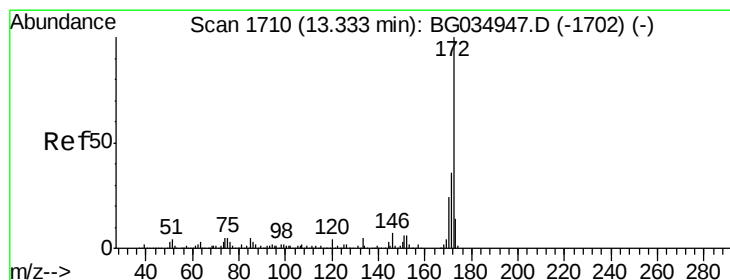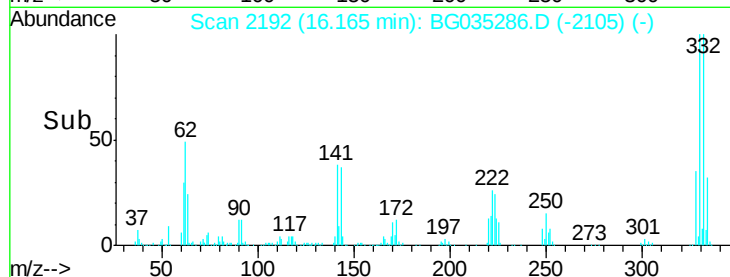
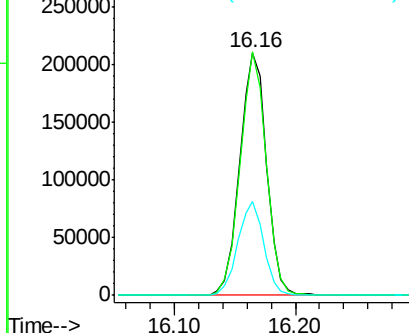



#44
 2-Fluorobiphenyl
 Concen: 95.741 ng
 RT: 13.30 min Scan# 1705
 Delta R.T. -0.02 min
 Lab File: BG035286.D
 Acq: 21 Jun 2018 5:17

Tgt Ion:172 Resp: 1054352
 Ion Ratio Lower Upper
 172 100
 171 35.0 30.0 45.0
 170 23.5 19.5 29.3

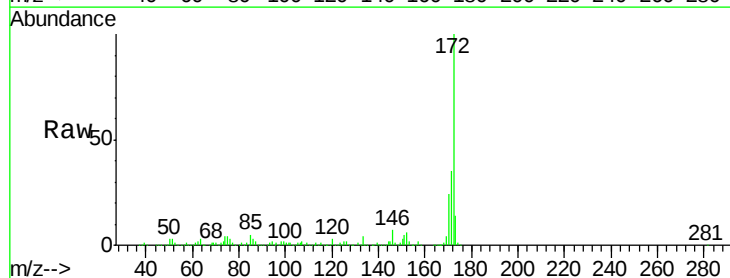

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

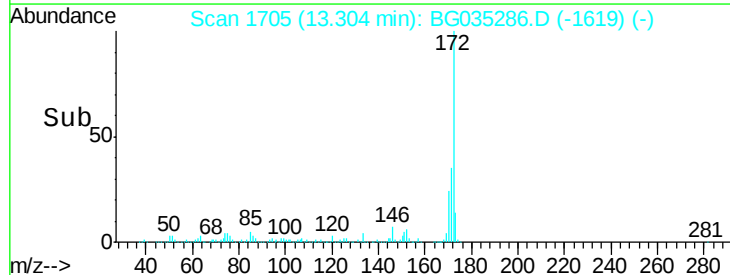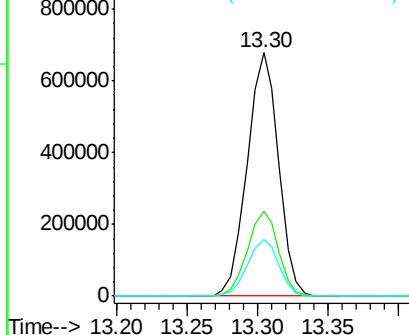

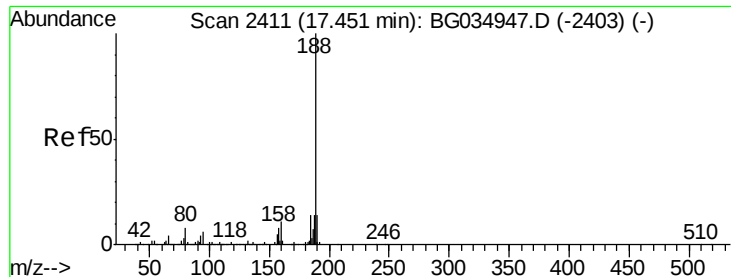

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.02 min

Lab File: BG035286.D

Acq: 21 Jun 2018 5:17

Instrument :

BNA_G

ClientSampleId :

OR-01-061918


Tgt Ion:188 Resp: 391280

Ion Ratio Lower Upper

188 100

94 5.7 6.9 10.3#




80 6.9 7.7 11.5#

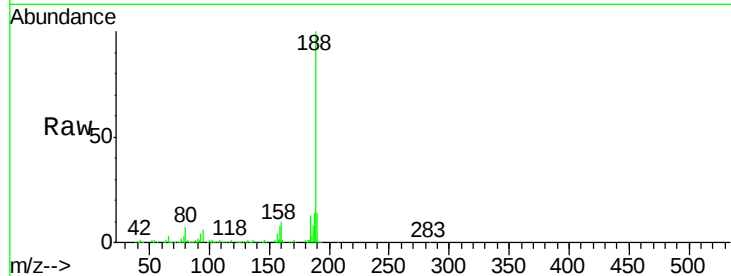

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

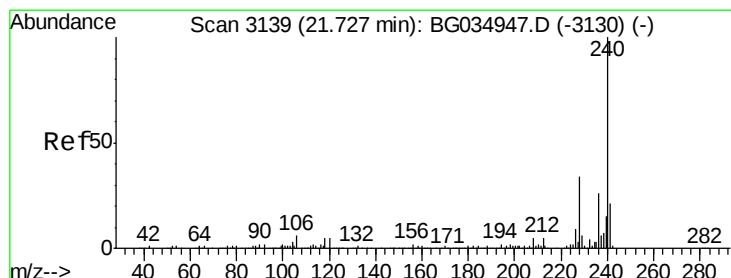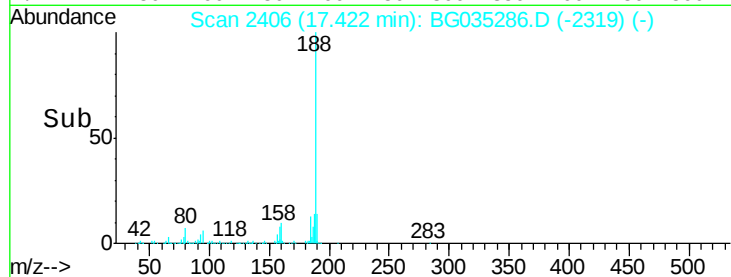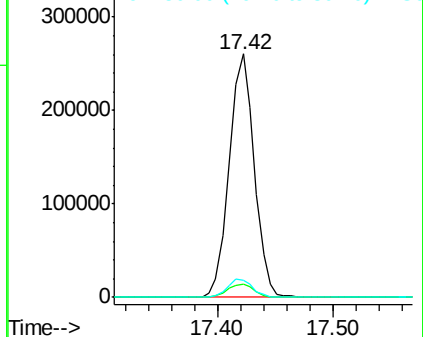

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3132

Delta R.T. -0.03 min

Lab File: BG035286.D

Acq: 21 Jun 2018 5:17


Tgt Ion:240 Resp: 430402

Ion Ratio Lower Upper

240 100

120 5.9 6.8 10.2#



236 26.2 20.9 31.3

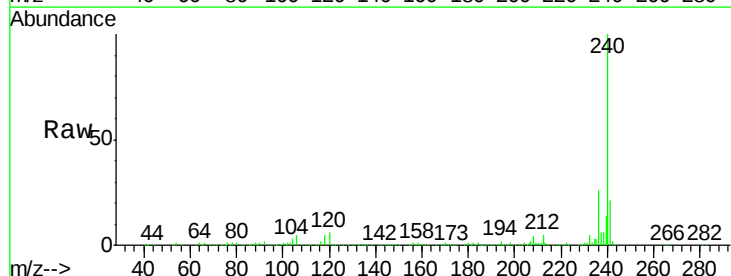


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

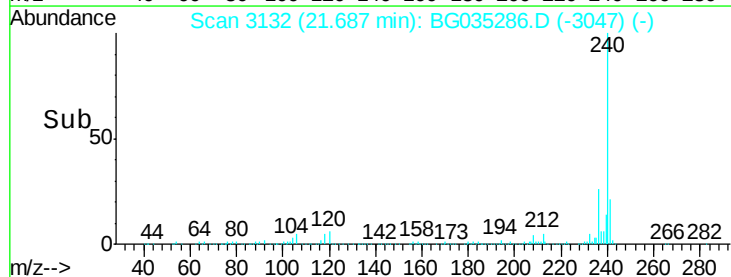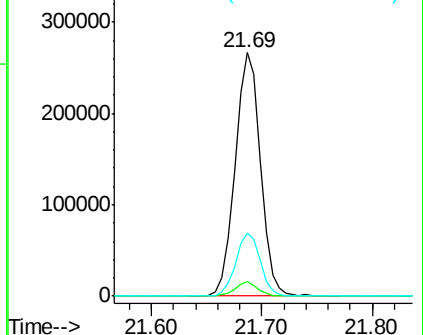

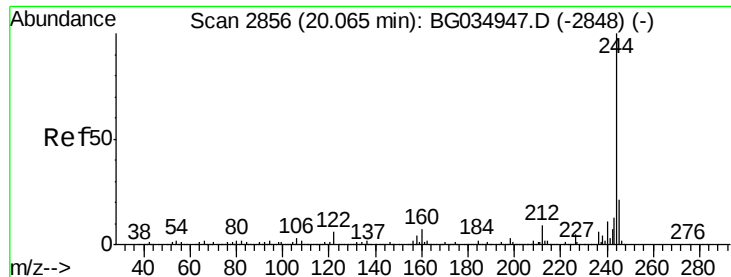

#78

Terphenyl-d14

Concen: 94.783 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035286.D

Acq: 21 Jun 2018 5:17

Instrument :

BNA_G

ClientSampleId :

OR-01-061918


Tgt Ion:244 Resp: 1947556

Ion Ratio Lower Upper

244 100

212 9.7 5.8 8.8#




122 6.7 7.0 10.4#

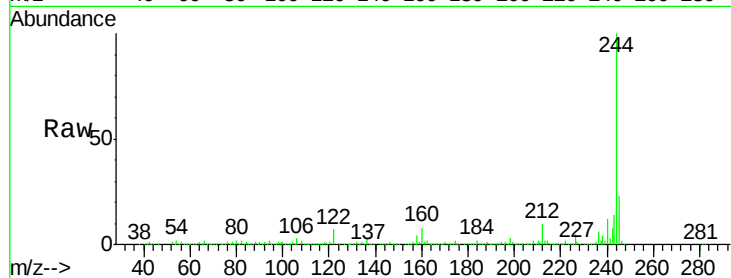

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

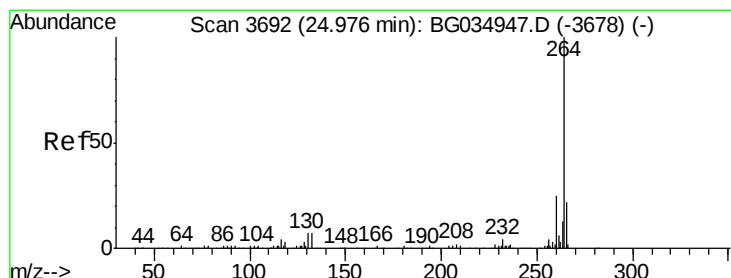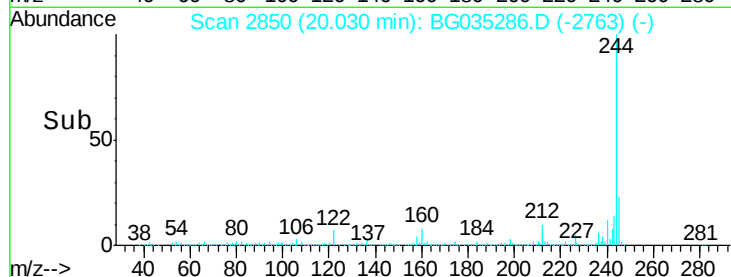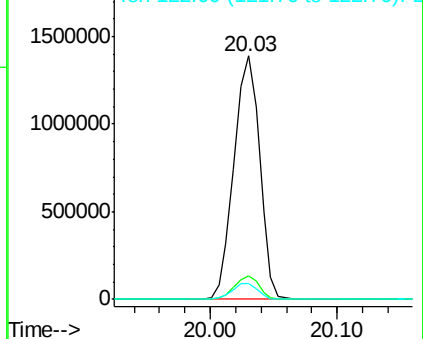

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.91 min Scan# 3681

Delta R.T. -0.04 min

Lab File: BG035286.D

Acq: 21 Jun 2018 5:17


Tgt Ion:264 Resp: 411661

Ion Ratio Lower Upper

264 100

260 24.1 17.4 26.0

265 21.1 17.7 26.5

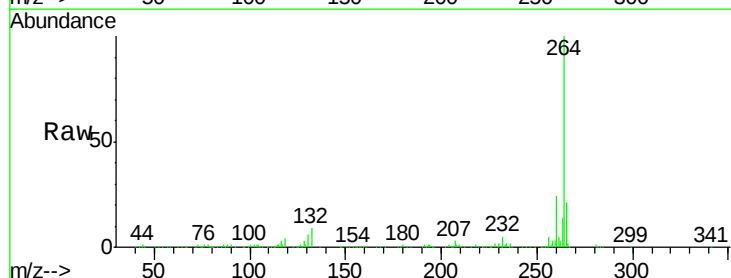

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

