


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062018\
 Data File : BG035261.D
 Acq On : 20 Jun 2018 10:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

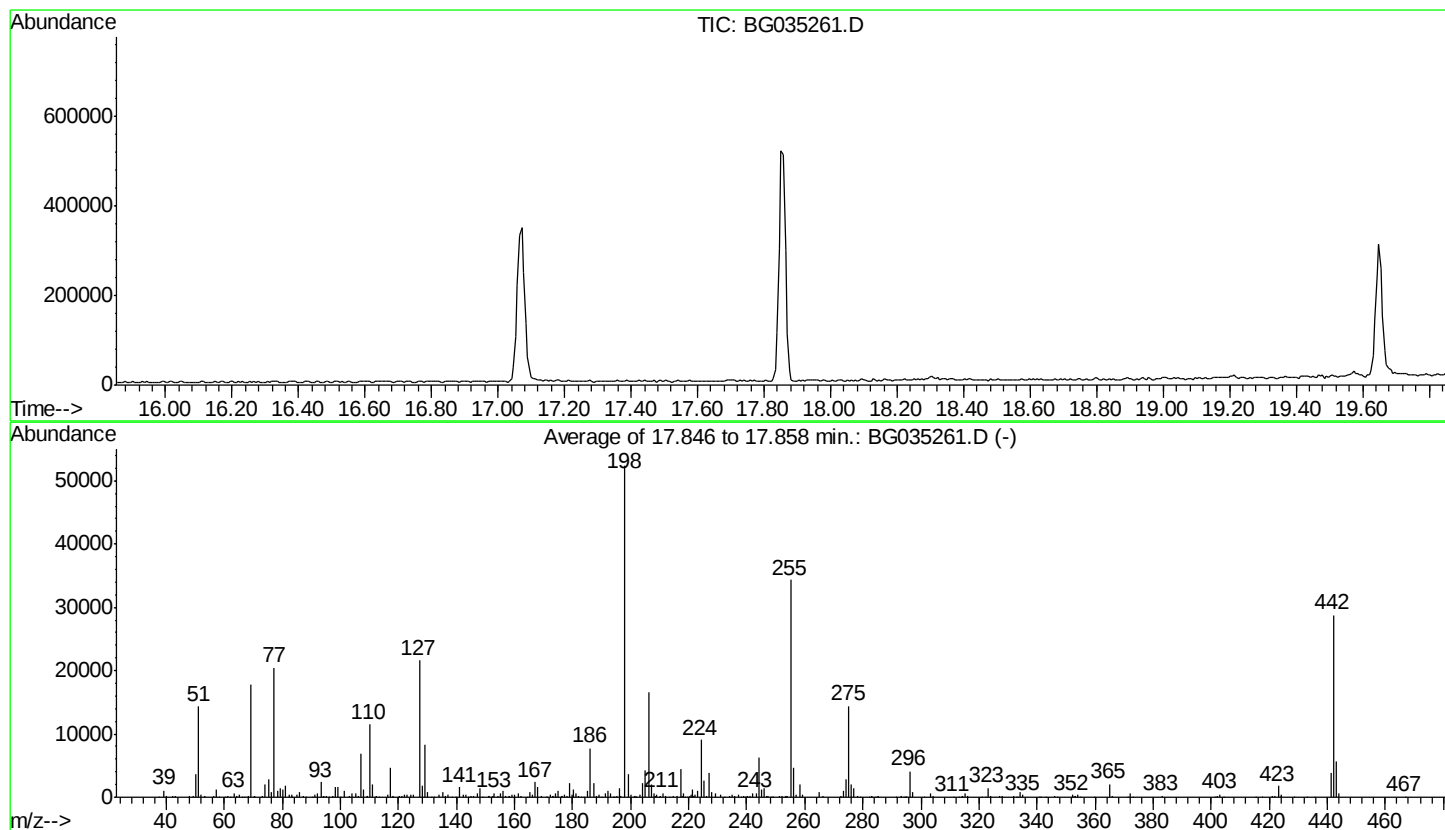

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	14329	PASS
68	69	0.00	2	0.8	148	PASS
69	198	0.00	100	34.0	17788	PASS
70	69	0.00	2	0.8	136	PASS
127	198	10	80	41.3	21631	PASS
197	198	0.00	2	0.4	226	PASS
198	198	100	100	100.0	52384	PASS
199	198	5	9	6.9	3623	PASS
275	198	10	60	27.5	14425	PASS
365	198	1	100	3.9	2061	PASS
441	443	0.01	100	68.2	3898	PASS
442	198	50	100	54.9	28770	PASS
443	442	15	24	19.9	5715	PASS