


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062018\
 Data File : BG035277.D
 Acq On : 20 Jun 2018 23:28
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

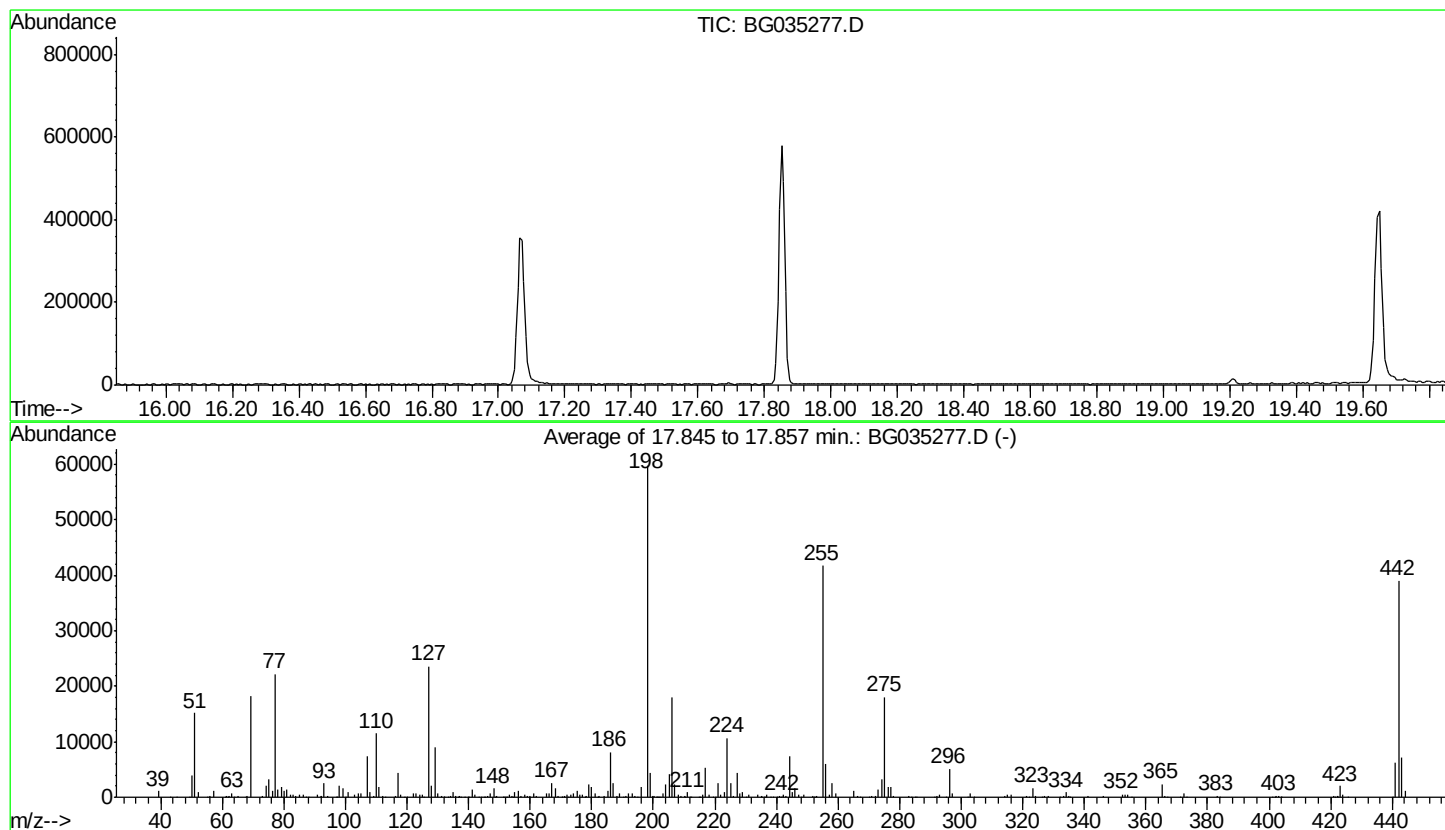

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	15159	PASS
68	69	0.00	2	0.7	126	PASS
69	198	0.00	100	30.6	18253	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.4	23528	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59712	PASS
199	198	5	9	7.4	4448	PASS
275	198	10	60	30.2	18038	PASS
365	198	1	100	4.1	2421	PASS
441	443	0.01	100	88.1	6314	PASS
442	198	50	100	65.4	39066	PASS
443	442	15	24	18.3	7168	PASS