

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062019\
 Data File : BG041362.D
 Acq On : 20 Jun 2019 18:22
 Operator : HP/JU
 Sample : K3157-07 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-061719-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.148	6	10	19	rVB3	27772	46161	7.60%	1.062%
2	5.622	425	431	439	rBV2	100283	177325	29.18%	4.078%
3	7.237	700	706	717	rBV2	109263	201158	33.10%	4.626%
4	7.608	764	769	777	rBV	113206	207191	34.10%	4.765%
5	8.084	843	850	857	rBV	150809	257961	42.45%	5.933%
6	8.407	899	905	913	rBV	93412	169034	27.82%	3.888%
7	9.264	1044	1051	1065	rBV	65645	143965	23.69%	3.311%
8	10.904	1323	1330	1338	rBV	186839	346686	57.05%	7.973%
9	13.336	1737	1744	1753	rBV	207861	338476	55.70%	7.785%
10	14.165	1878	1885	1891	rVB	19597	31275	5.15%	0.719%
11	14.723	1973	1980	1987	rBV2	309694	503397	82.84%	11.578%
12	16.209	2227	2233	2240	rBV	167532	259348	42.68%	5.965%
13	17.467	2441	2447	2454	rBV2	380501	607687	100.00%	13.976%
14	18.313	2589	2591	2597	rBV7	20987	37095	6.10%	0.853%
15	19.223	2744	2746	2749	rBV3	39512	52231	8.60%	1.201%
16	19.253	2749	2751	2755	rVB3	53295	60360	9.93%	1.388%
17	20.064	2885	2889	2893	rVB	356697	421737	69.40%	9.699%
18	21.750	3172	3176	3183	rVB	296324	486973	80.14%	11.200%


Sum of corrected areas: 4348060

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062019\
Data File : BG041362.D
Acq On : 20 Jun 2019 18:22
Operator : HP/JU
Sample : K3157-07 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

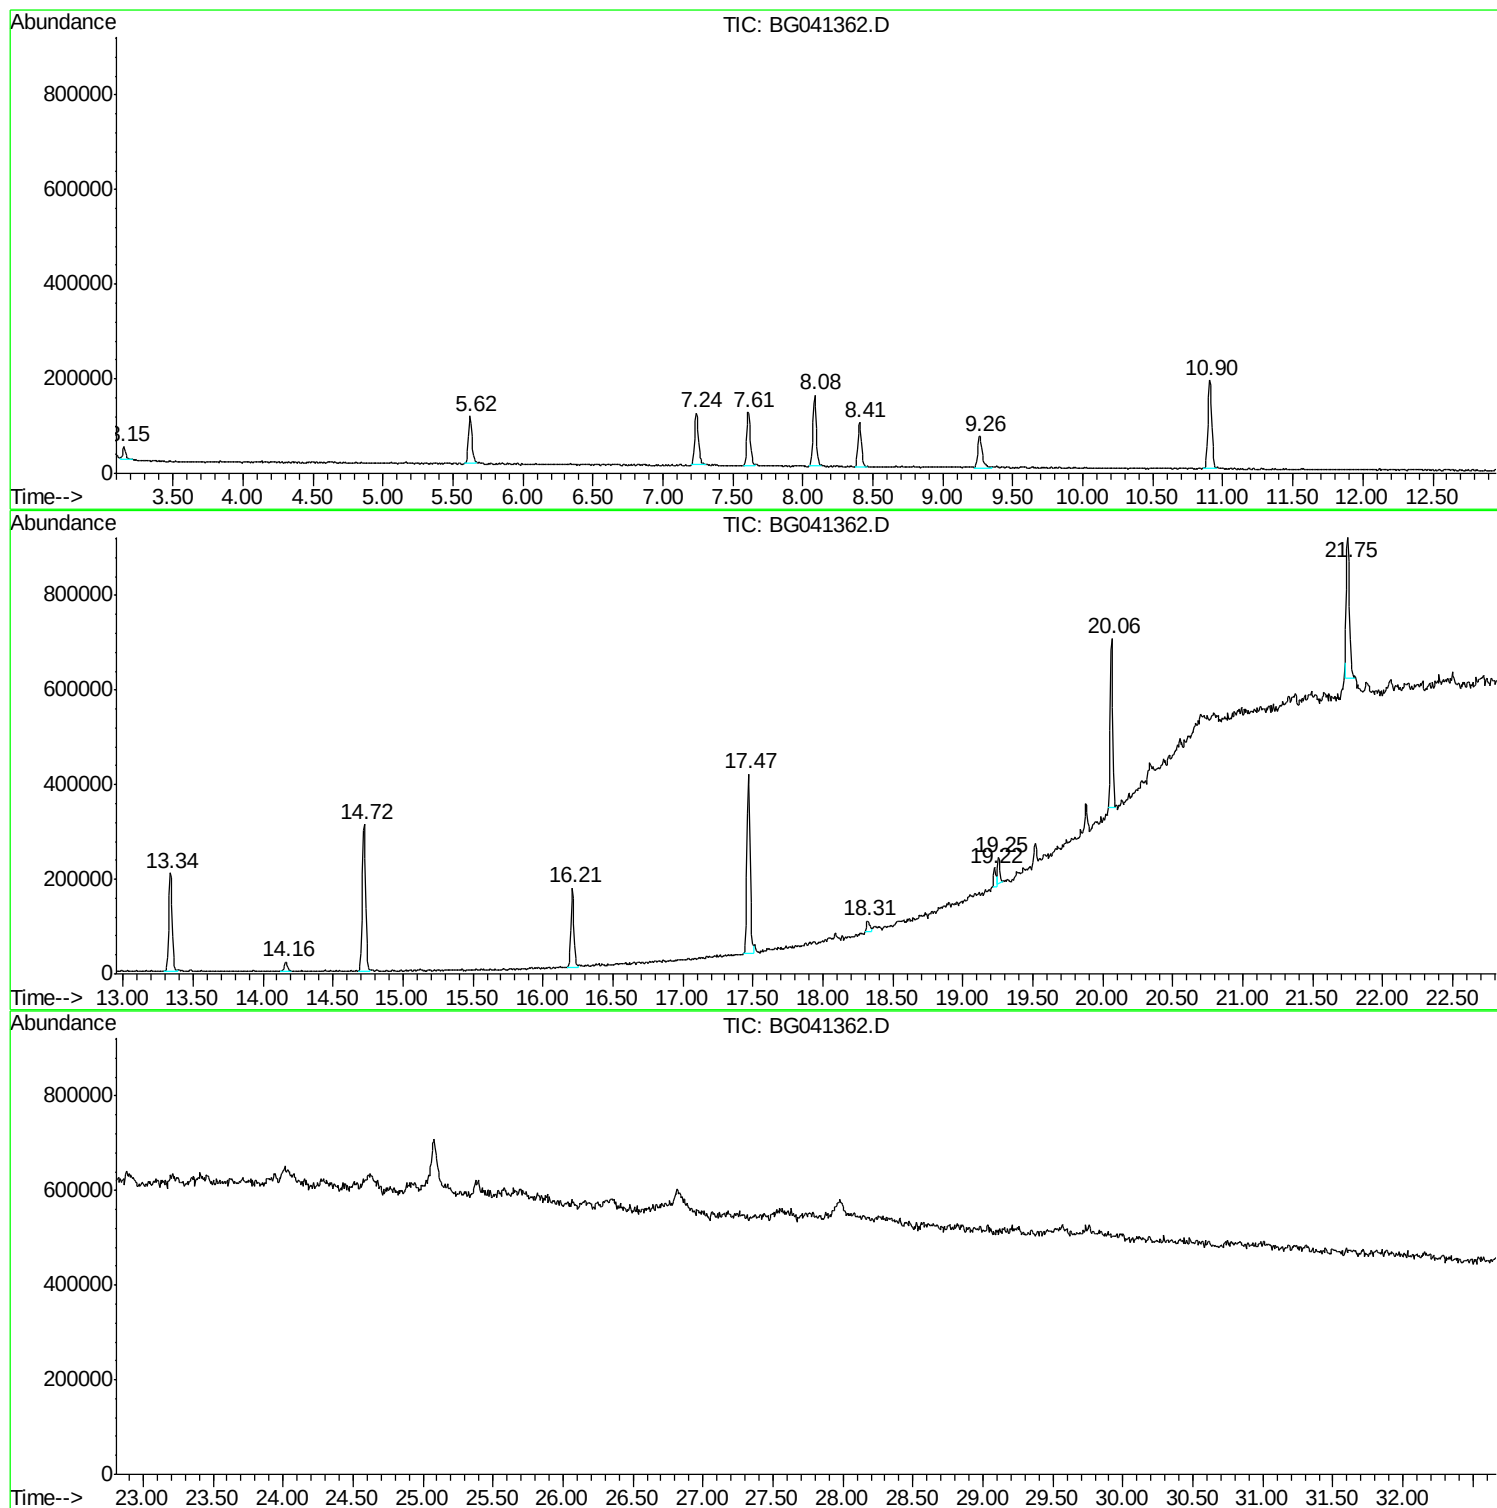

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062019\
Data File : BG041362.D
Acq On : 20 Jun 2019 18:22
Operator : HP/JU
Sample : K3157-07 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-D










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.15 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.15	3.58 ng	46161	1,4-Dichlorobenzene-d4	8.08

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Methylpentan-3-yl propyl carbo...	188	C10H20O3	1000372-82-3	12
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3			1-Propene-1-thiol	74	C3H6S	000925-89-3	9
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
5			Silane, trimethyl-3-penten-2-yl-...	142	C8H18Si	053264-56-5	9

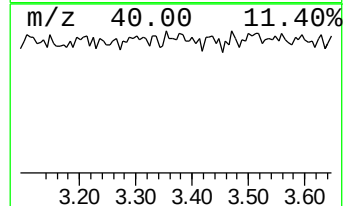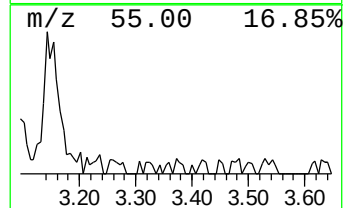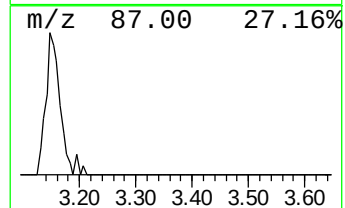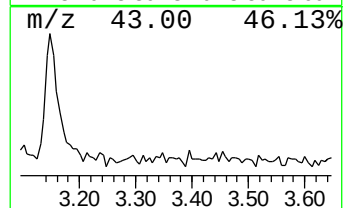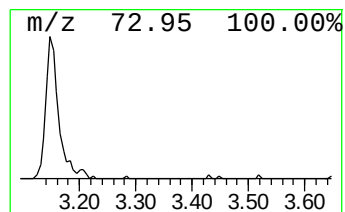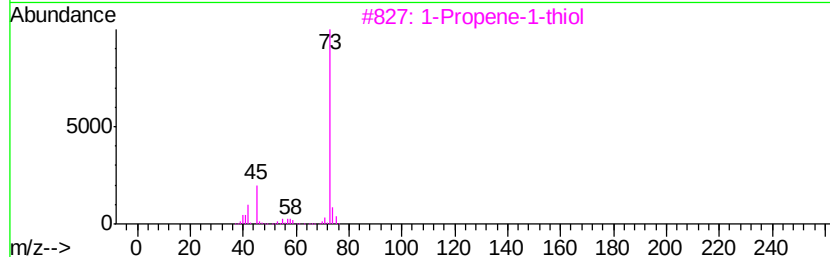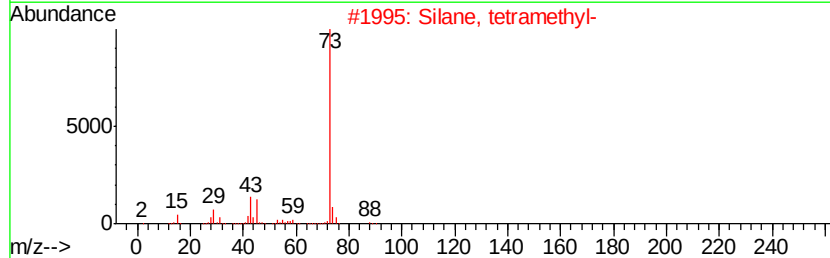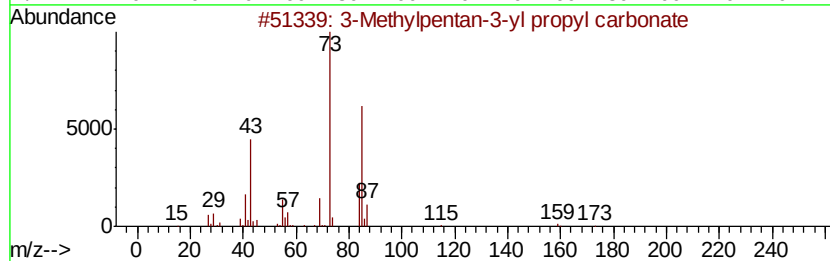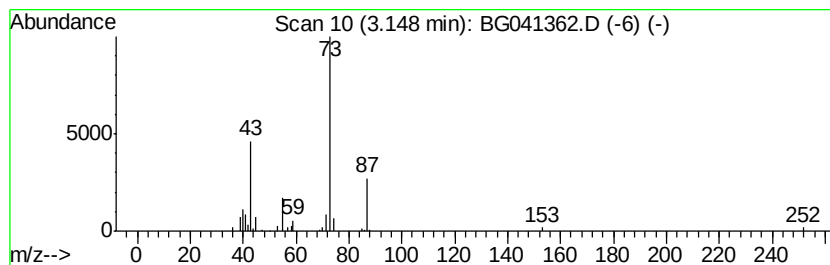

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062019\
Data File : BG041362.D
Acq On : 20 Jun 2019 18:22
Operator : HP/JU
Sample : K3157-07 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-D










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.61	16.06 ng	207191	1,4-Dichlorobenzene-d4	8.08

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		1H-Indenol	132	C9H8O	056631-57-3	27
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	22

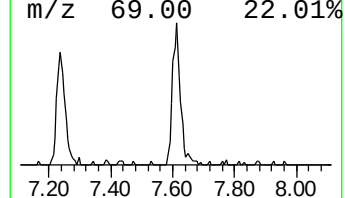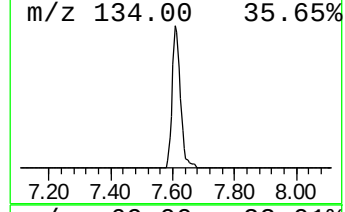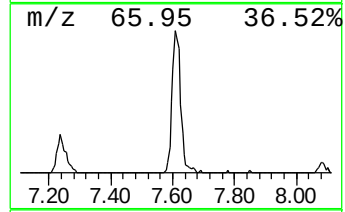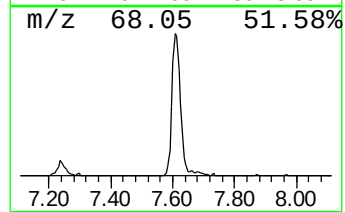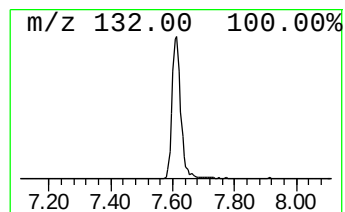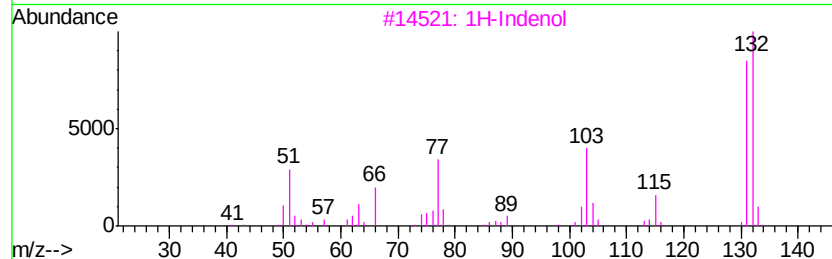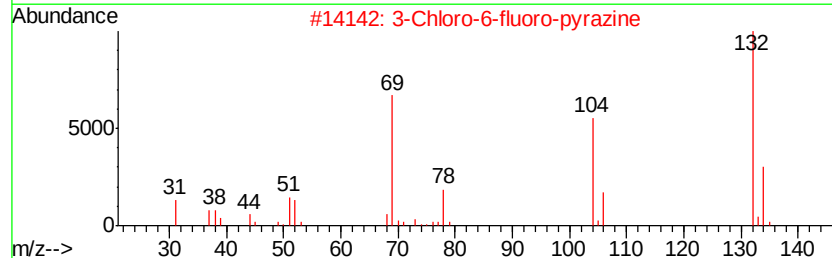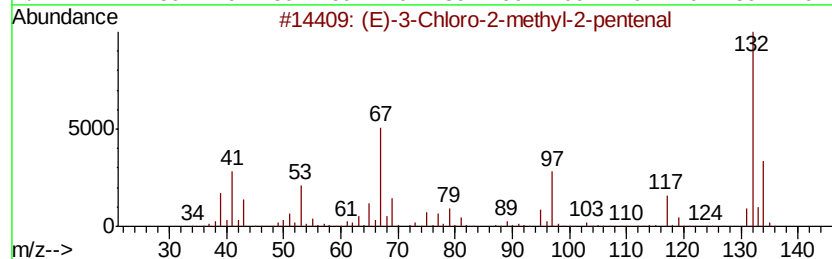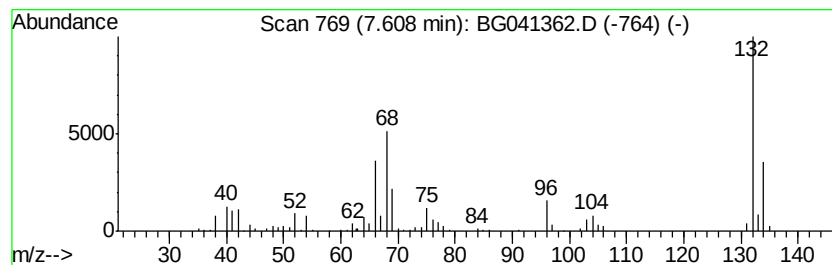

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062019\
Data File : BG041362.D
Acq On : 20 Jun 2019 18:22
Operator : HP/JU
Sample : K3157-07 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-061719-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.15	3.15	3.6	ng	46161	1	8.08	257961	20.0
unknown7.61	7.61	16.1	ng	207191	1	8.08	257961	20.0