


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062019\
 Data File : BG041352.D
 Acq On : 20 Jun 2019 11:24
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

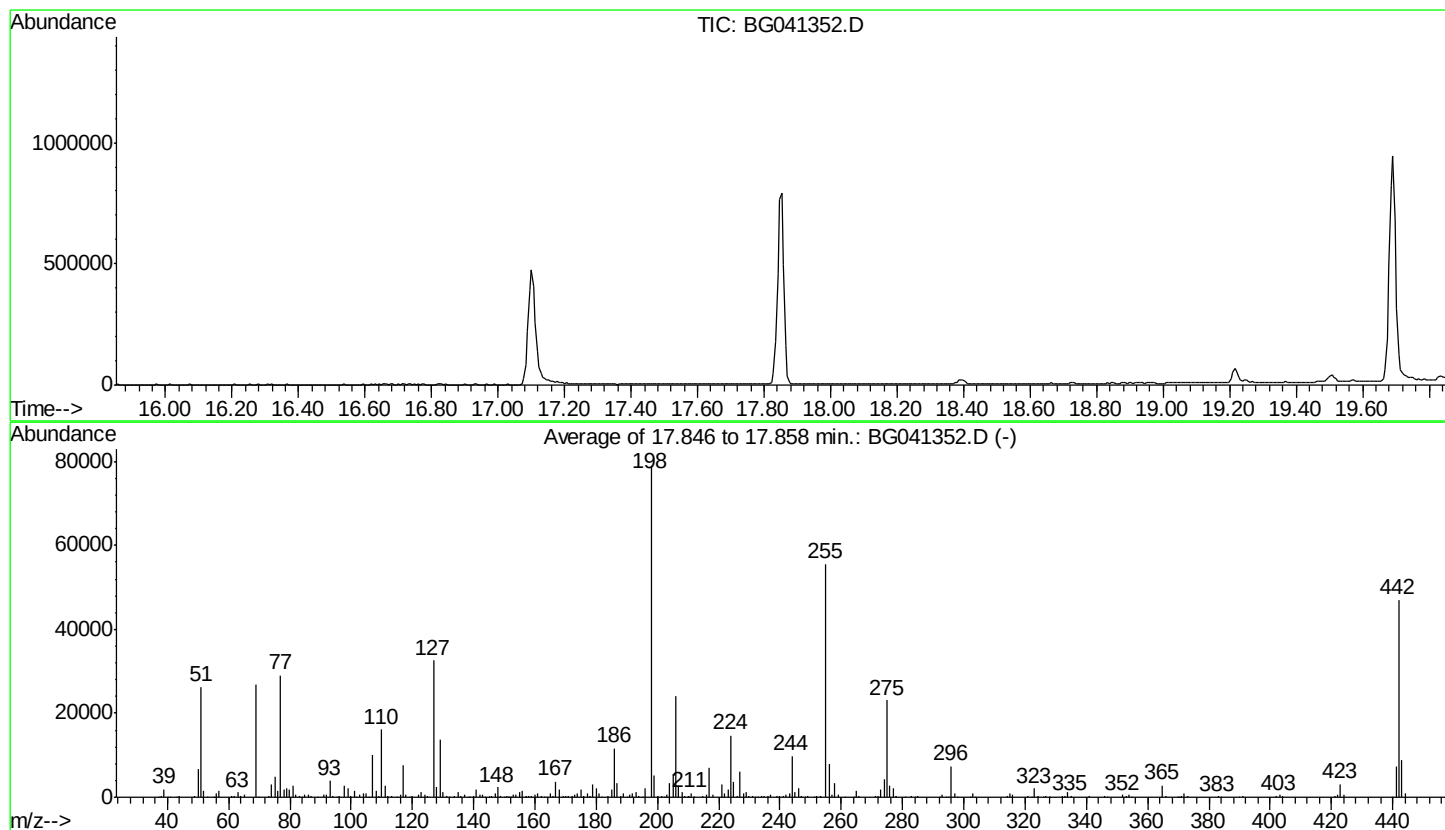

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	26240	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	26753	PASS
70	69	0.00	2	0.5	124	PASS
127	198	10	80	41.3	32605	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78997	PASS
199	198	5	9	6.4	5087	PASS
275	198	10	60	29.3	23112	PASS
365	198	1	100	3.6	2838	PASS
441	198	0.01	100	9.4	7442	PASS
442	198	50	100	59.6	47112	PASS
443	442	15	24	19.1	8995	PASS