
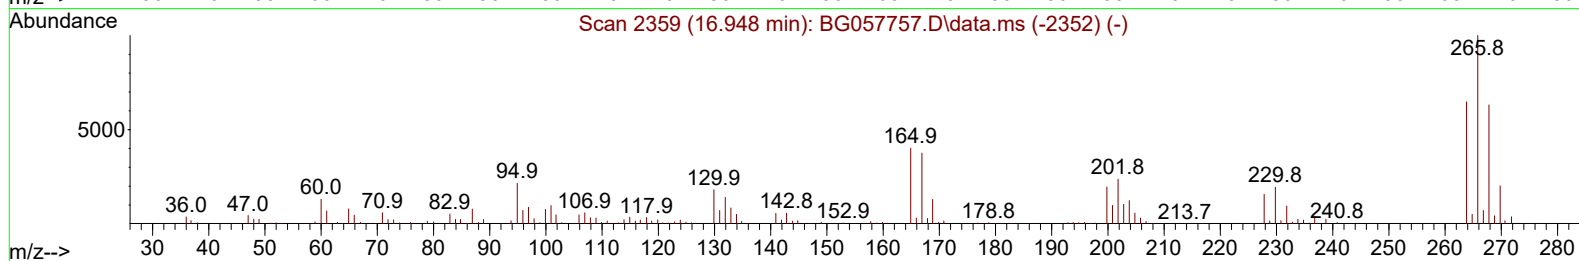
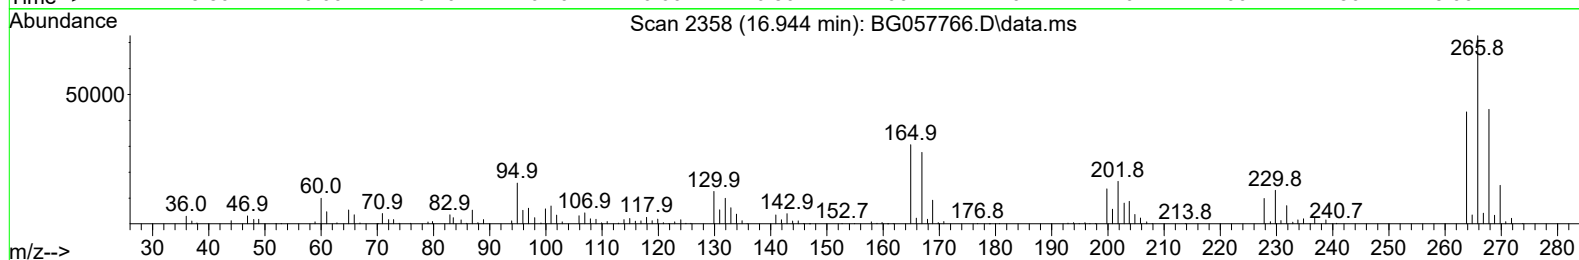


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062023\
Data File : BG057766.D
Acq On : 20 Jun 2023 7:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 09:12:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

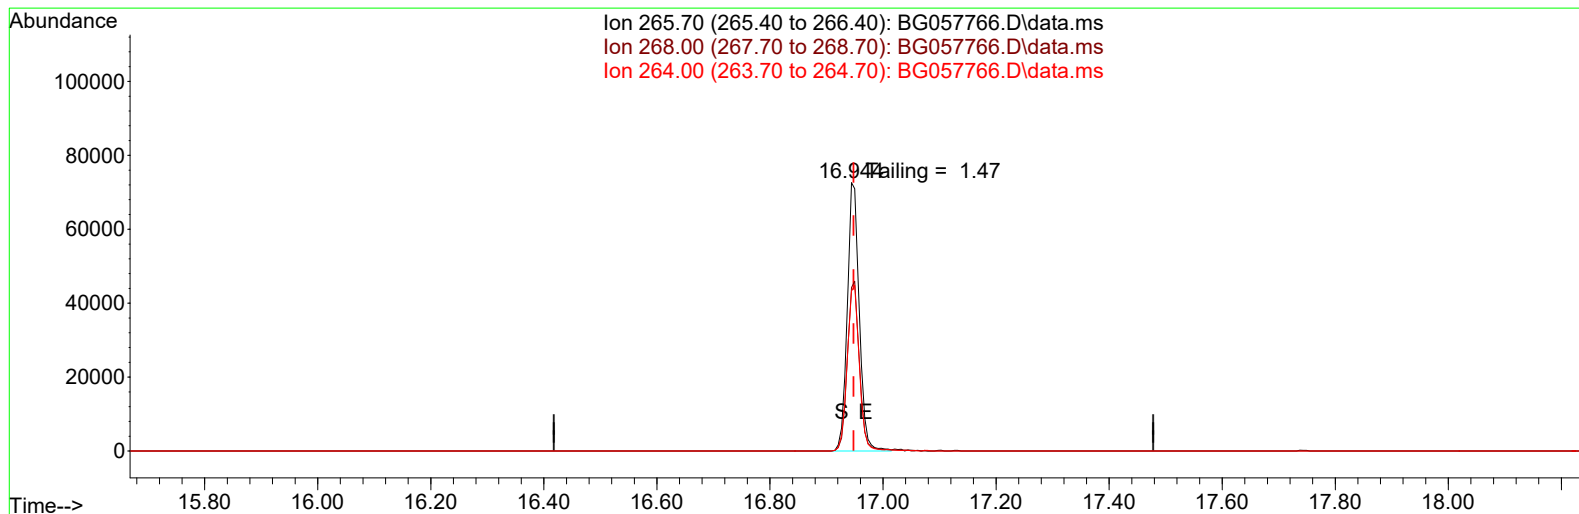

TIC: BG057766.D\data.ms

(70) Pentachlorophenol (C)




16.944min (-0.004) 28194.52 ng

response 107193

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	60.95
264.00	64.70	59.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062023\
Data File : BG057766.D
Acq On : 20 Jun 2023 7:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 09:12:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

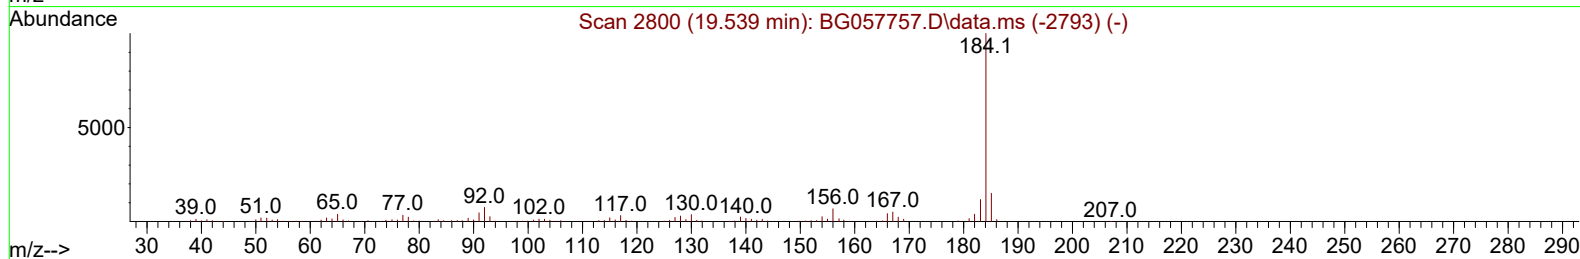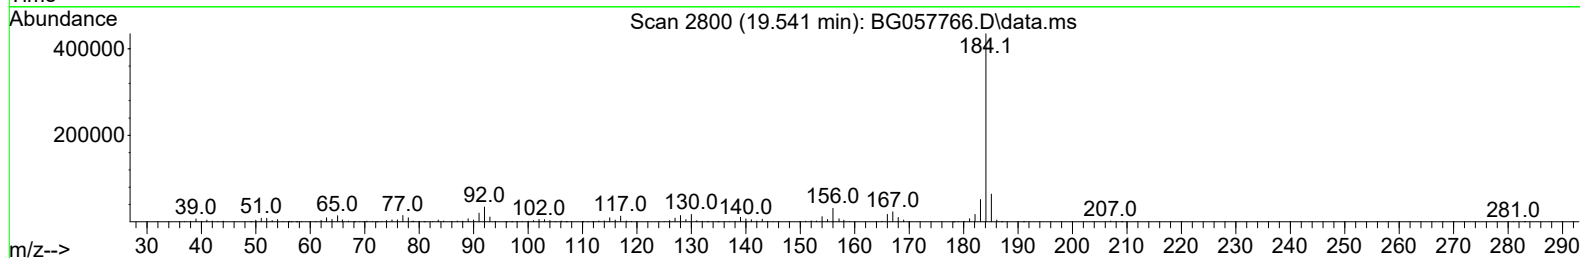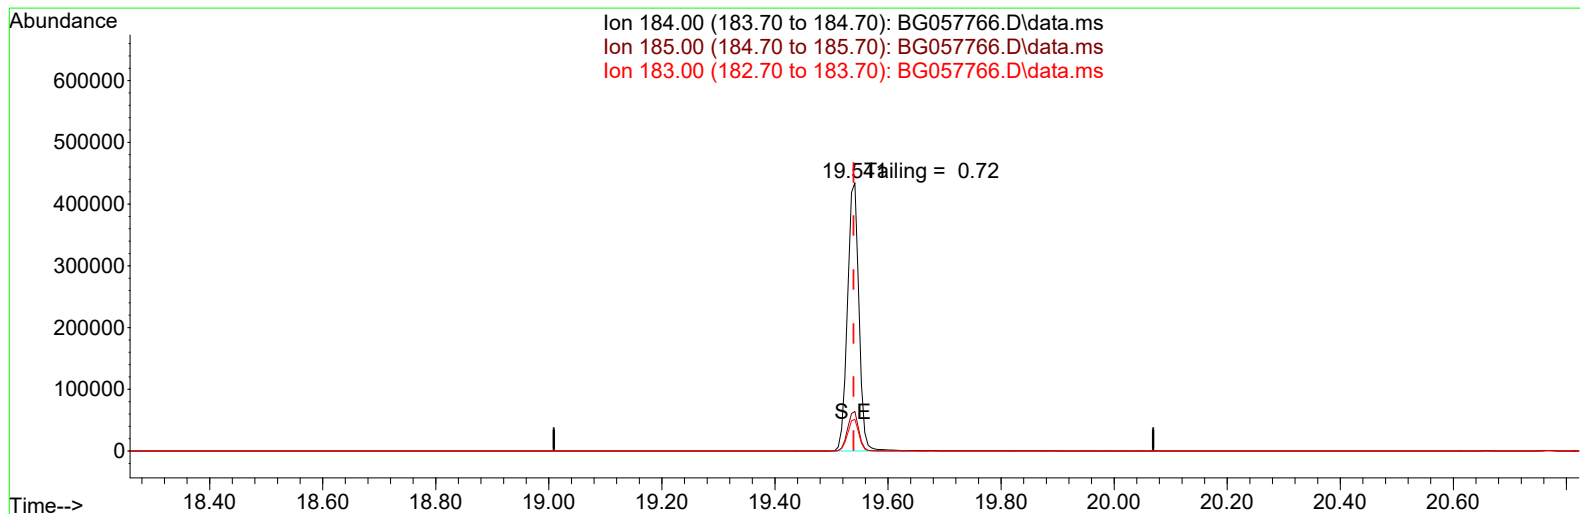

TIC: BG057766.D\data.ms

(77) Benzidine**19.541min (+ 0.002) 0.00 ng****response 611968**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.75
183.00	11.70	11.84
0.00	0.00	0.00