
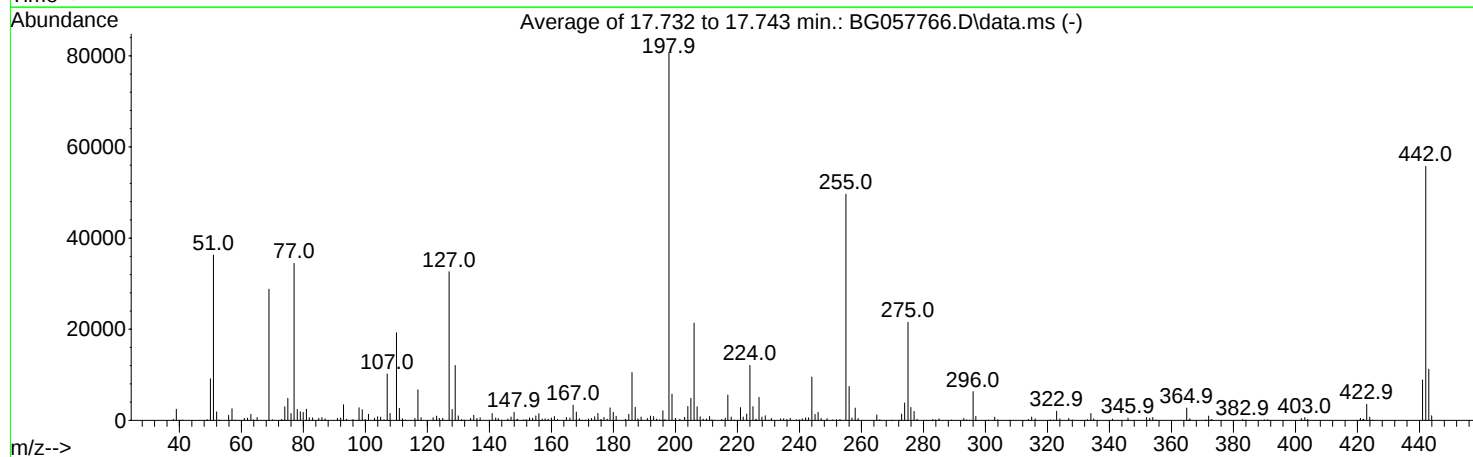


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG062023\  
 Data File : BG057766.D  
 Acq On : 20 Jun 2023 7:54  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG061923.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jun 20 03:40:38 2023

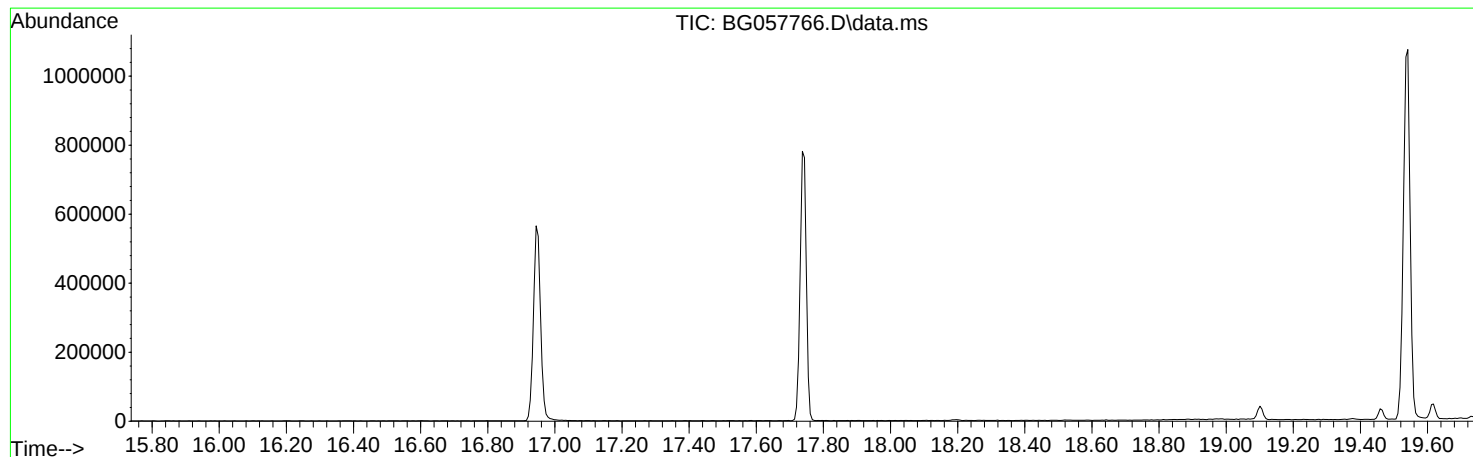

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 44.9         | 36256      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 35.7         | 28781      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 129        | PASS                |
| 127            | 198             | 10              | 80              | 40.4         | 32632      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 80725      | PASS                |
| 199            | 198             | 5               | 9               | 7.1          | 5768       | PASS                |
| 275            | 198             | 10              | 60              | 26.7         | 21539      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 2708       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.0         | 8894       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 55731      | PASS                |
| 443            | 442             | 15              | 24              | 20.2         | 11246      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/20/2023     | BNA_G            | <u>BG057766.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 261442           | 20.769             |
| DDD           | 8676             | 20.328             |
| DDE           | 66               | 19.823             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 8742          | 270184           | 3.24               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG062023\  
Data File : BG057766.D  
Acq On : 20 Jun 2023 7:54  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Jun 20 09:12:56 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG061923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 20 03:40:38 2023  
Response via : Initial Calibration

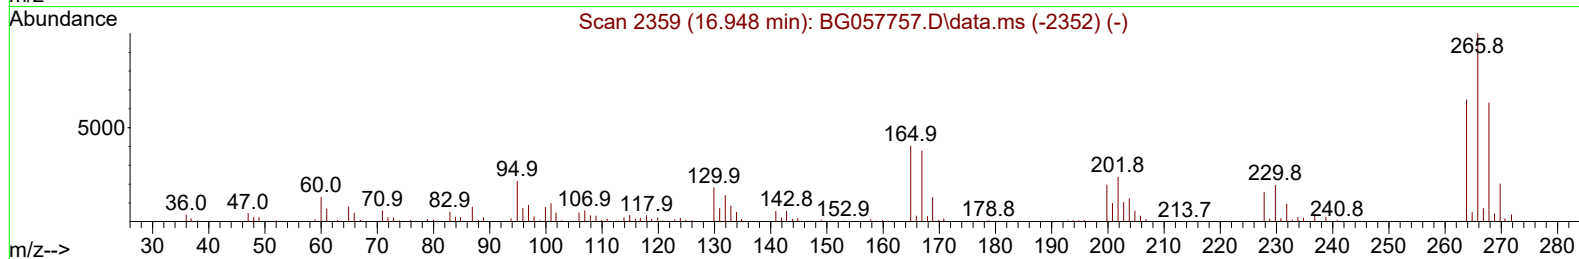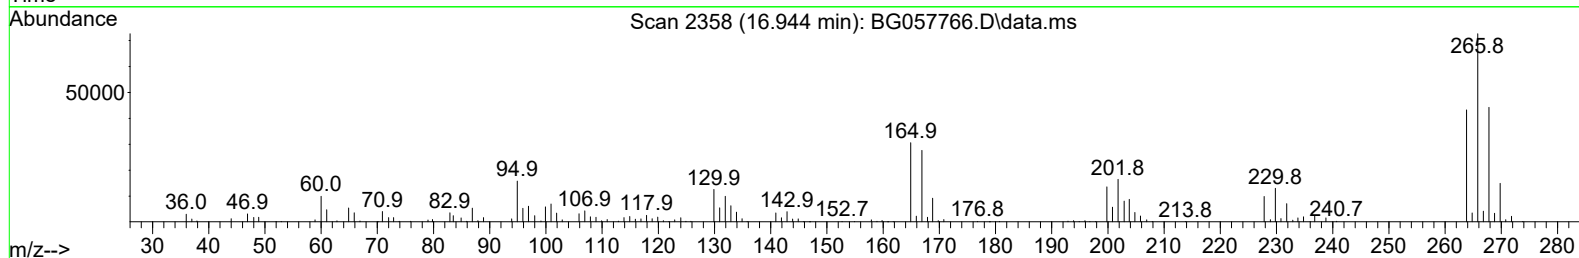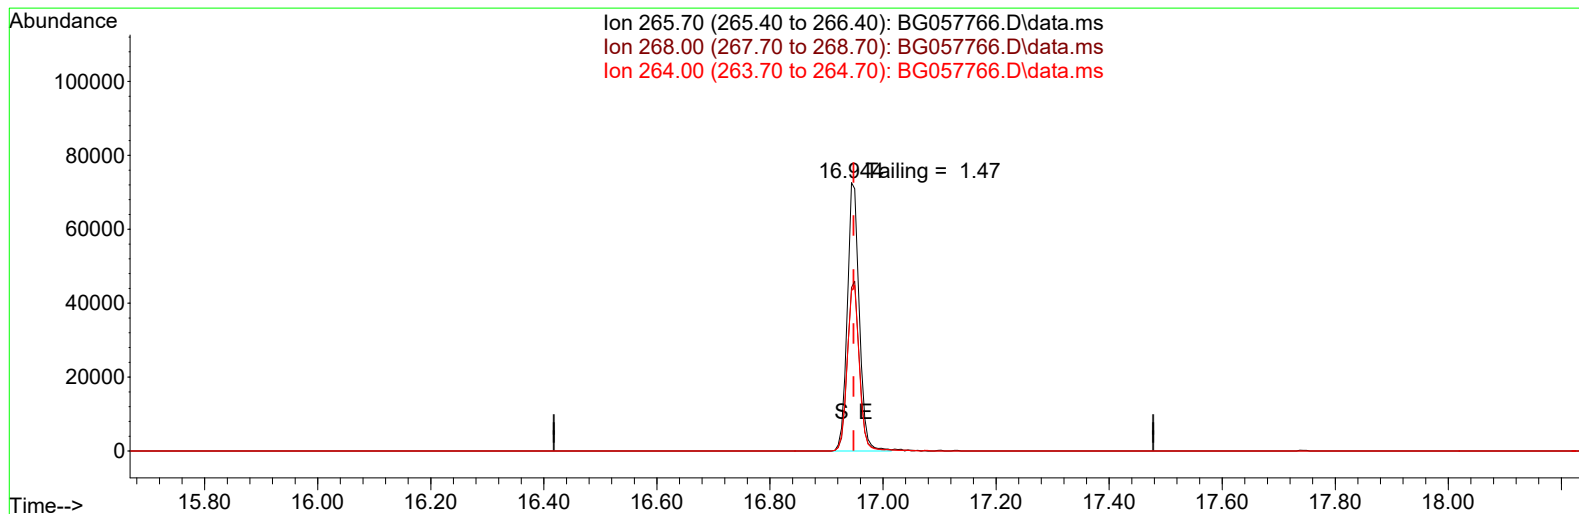

TIC: BG057766.D\data.ms

**(70) Pentachlorophenol (C)**

**16.944min (-0.004) 28194.52 ng**




**response 107193**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 60.95  |
| 264.00 | 64.70  | 59.56  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG062023\  
Data File : BG057766.D  
Acq On : 20 Jun 2023 7:54  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Jun 20 09:12:56 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG061923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 20 03:40:38 2023  
Response via : Initial Calibration

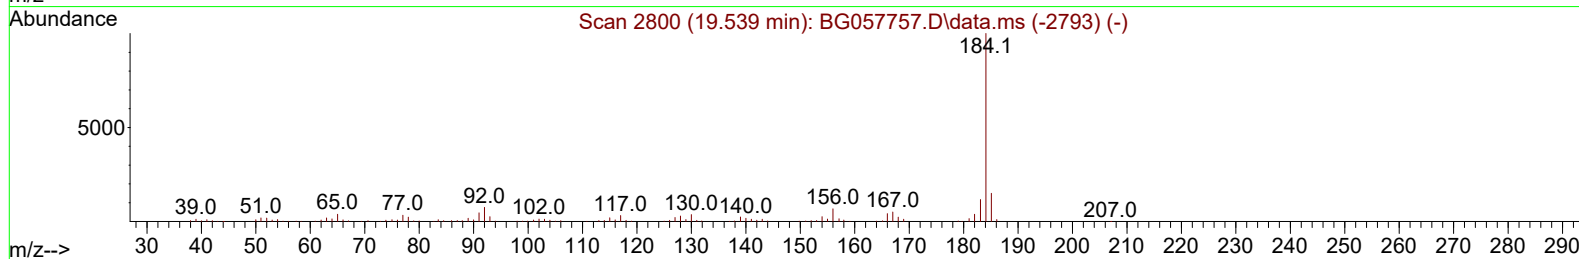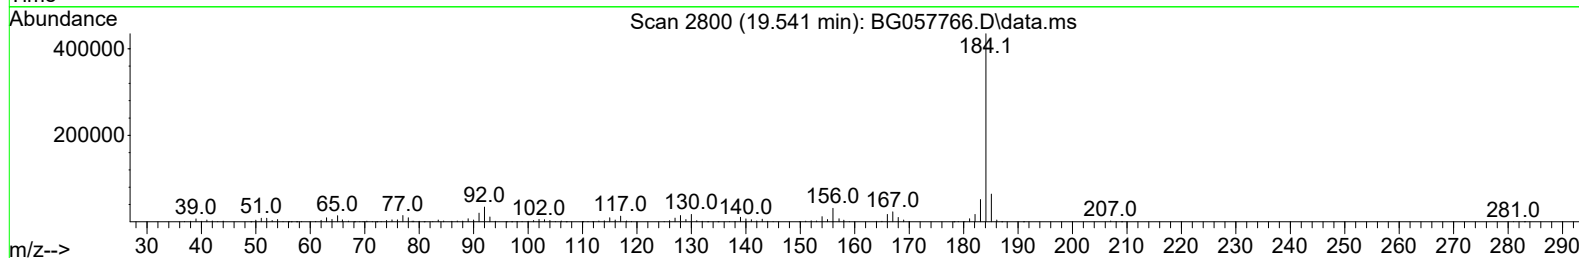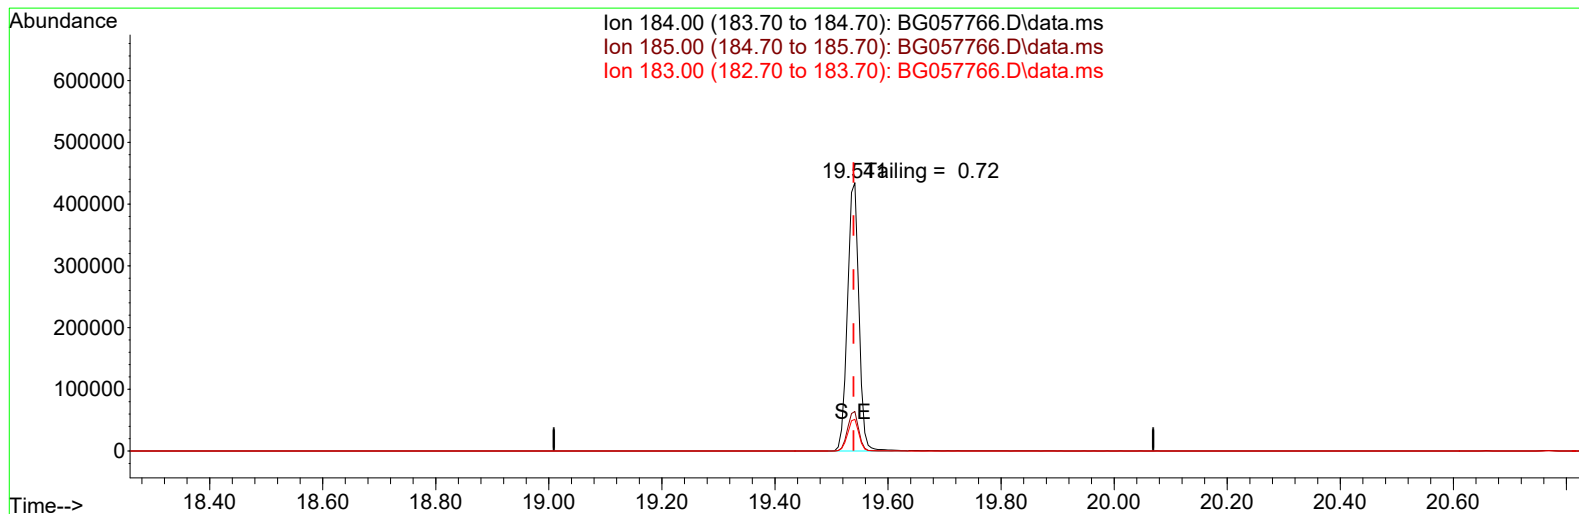

TIC: BG057766.D\data.ms

(77) Benzidine

19.541min (+ 0.002) 0.00 ng

response 611968

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.75  |
| 183.00 | 11.70  | 11.84  |
| 0.00   | 0.00   | 0.00   |