
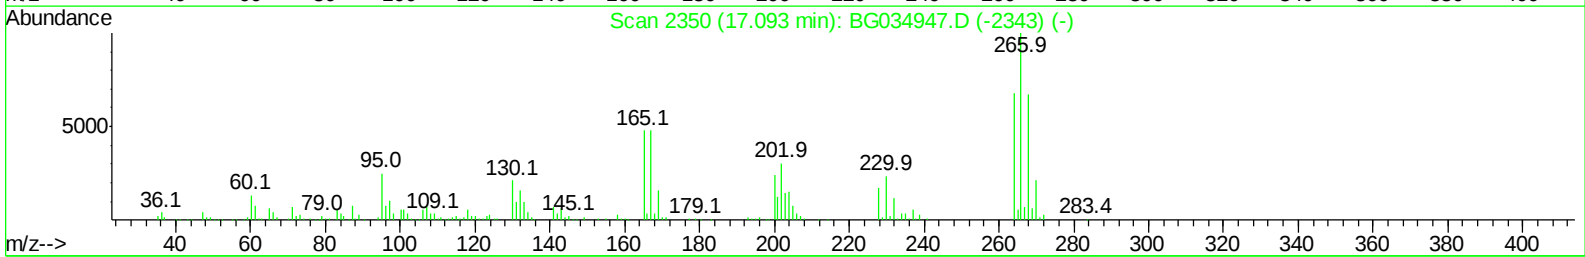
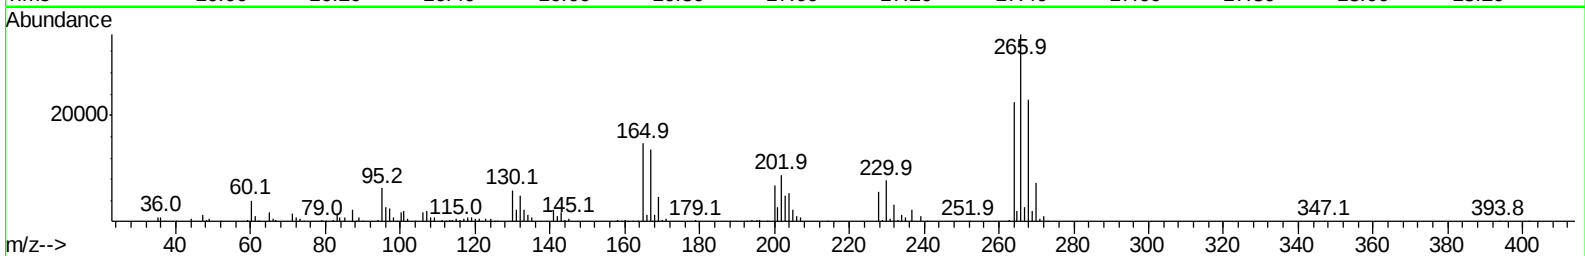


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062118\
Data File : BG035295.D
Acq On : 21 Jun 2018 12:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 06:19:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

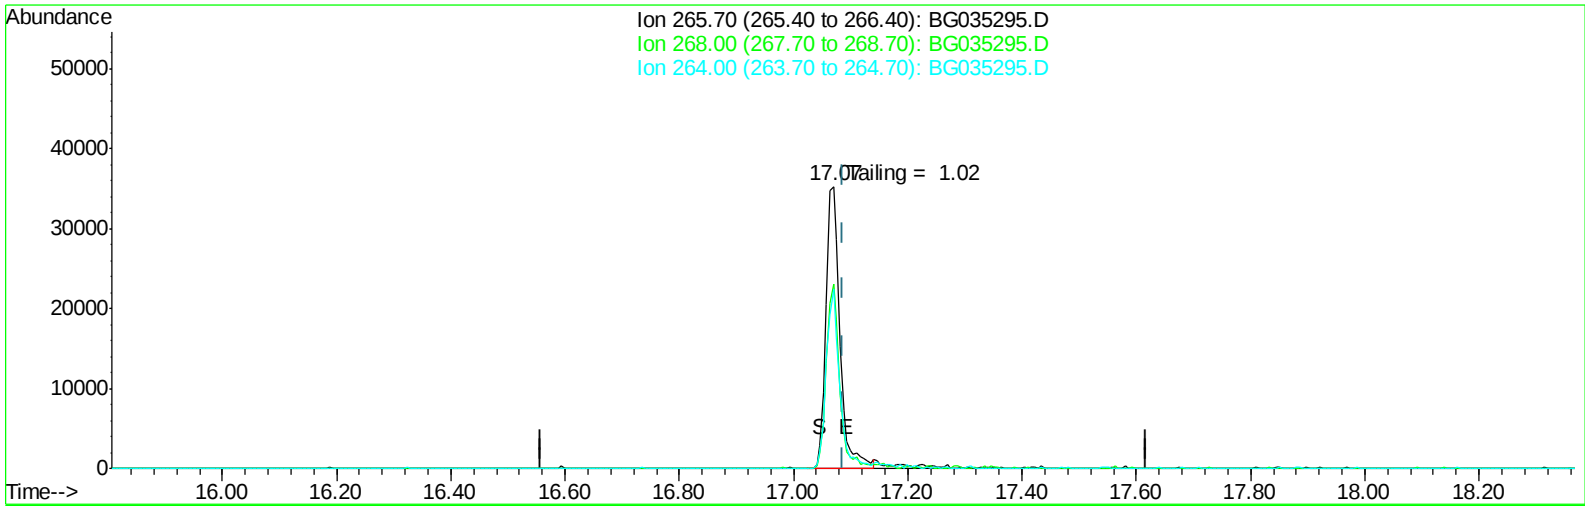

TIC: BG035295.D

(69) Pentachlorophenol (C)




17.070min (-0.018) 135665.87ng

response 59263

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.27
264.00	62.00	63.56
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062118\
Data File : BG035295.D
Acq On : 21 Jun 2018 12:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 06:19:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

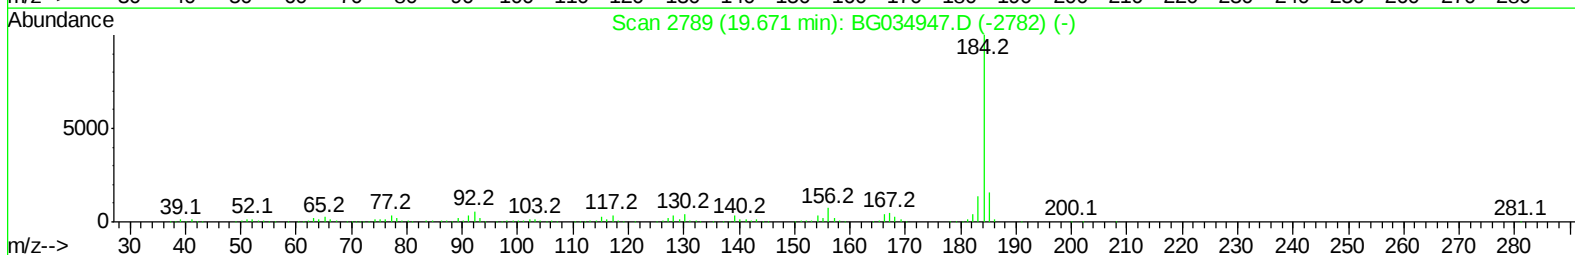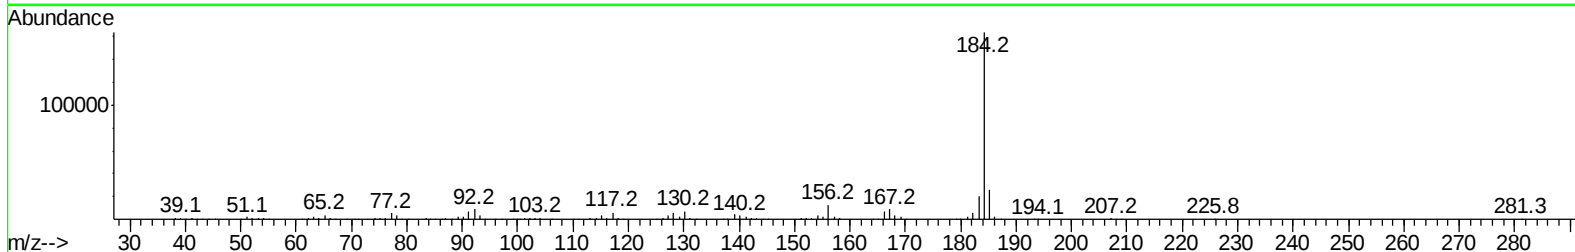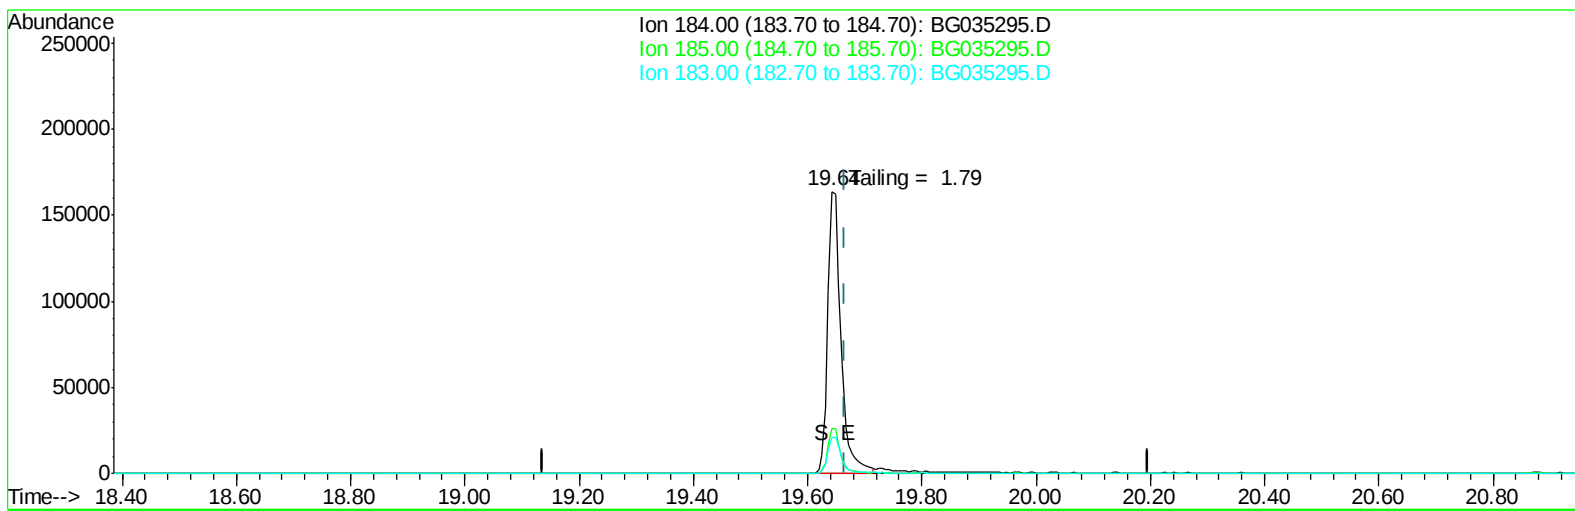

TIC: BG035295.D

(76) Benzidine




19.643min (-0.024) 77705.10ng

response 263073

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.75
183.00	13.30	12.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062118\
Data File : BG035295.D
Acq On : 21 Jun 2018 12:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 06:19:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

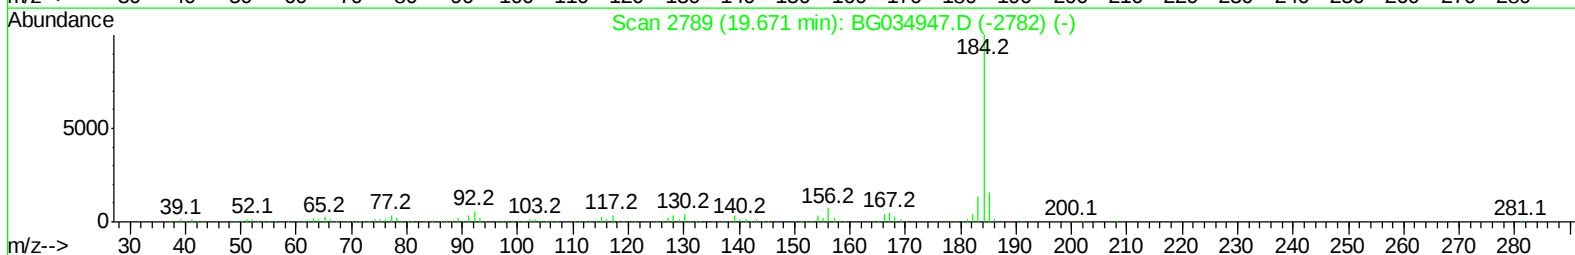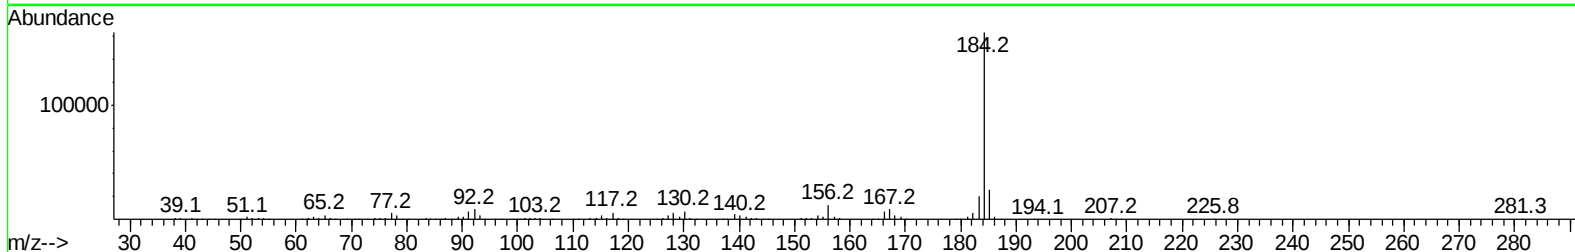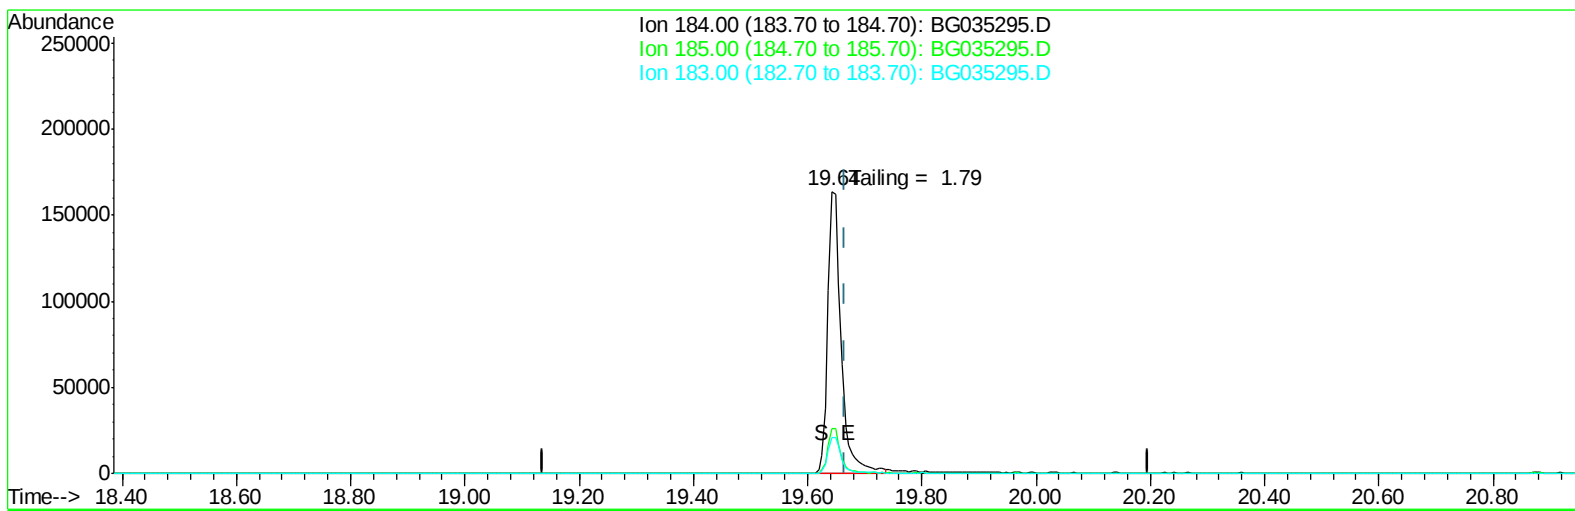

TIC: BG035295.D

(76) Benzidine

19.643min (-0.024) 77705.10ng

response 263073

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.75
183.00	13.30	12.71
0.00	0.00	0.00