
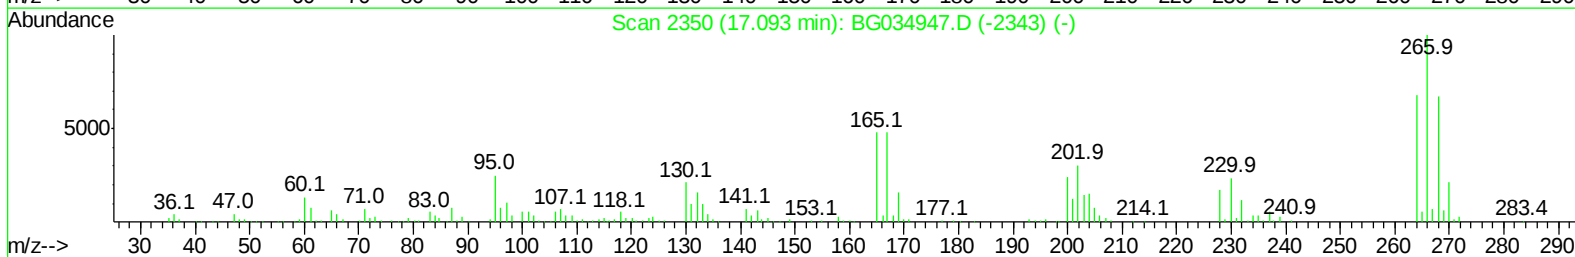
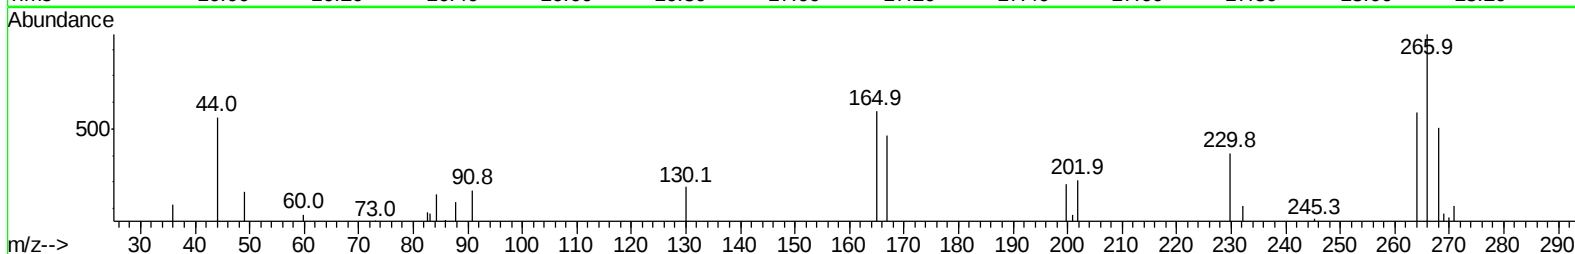


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062118\
Data File : BG035313.D
Acq On : 22 Jun 2018 1:10
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 06:21:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

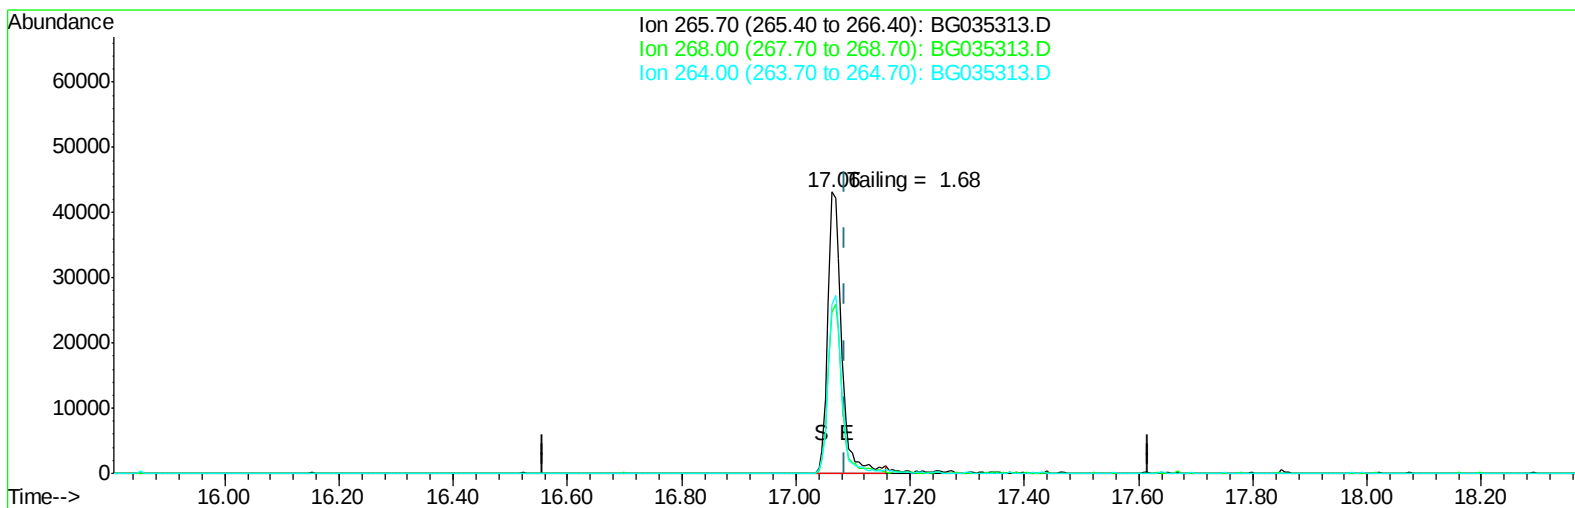

TIC: BG035313.D

(69) Pentachlorophenol (C)




17.063min (-0.025) 134344.78ng

response 70866

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.38
264.00	62.00	60.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062118\
Data File : BG035313.D
Acq On : 22 Jun 2018 1:10
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 06:21:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

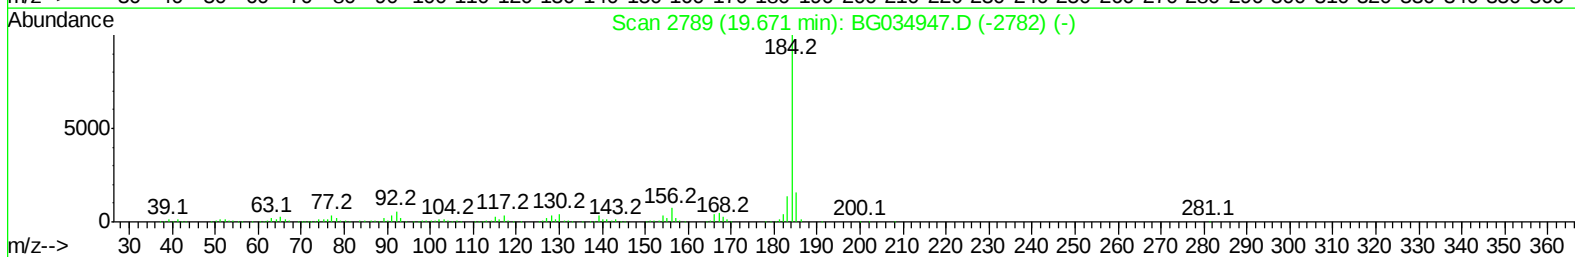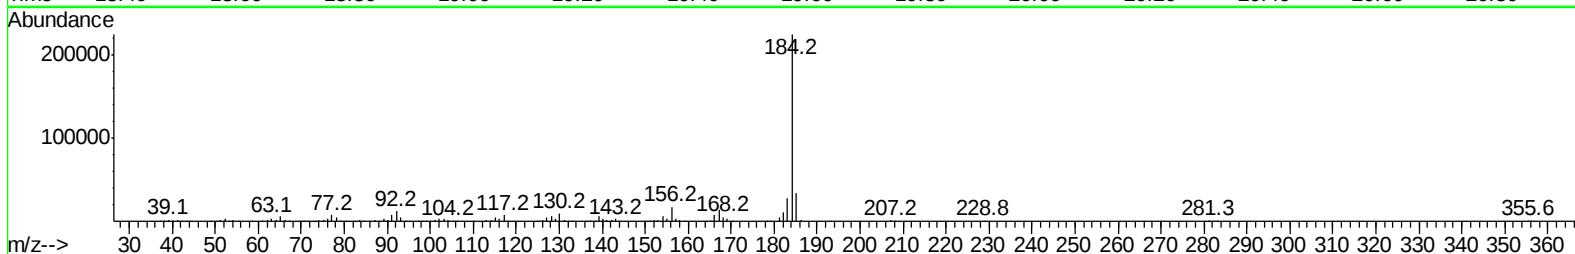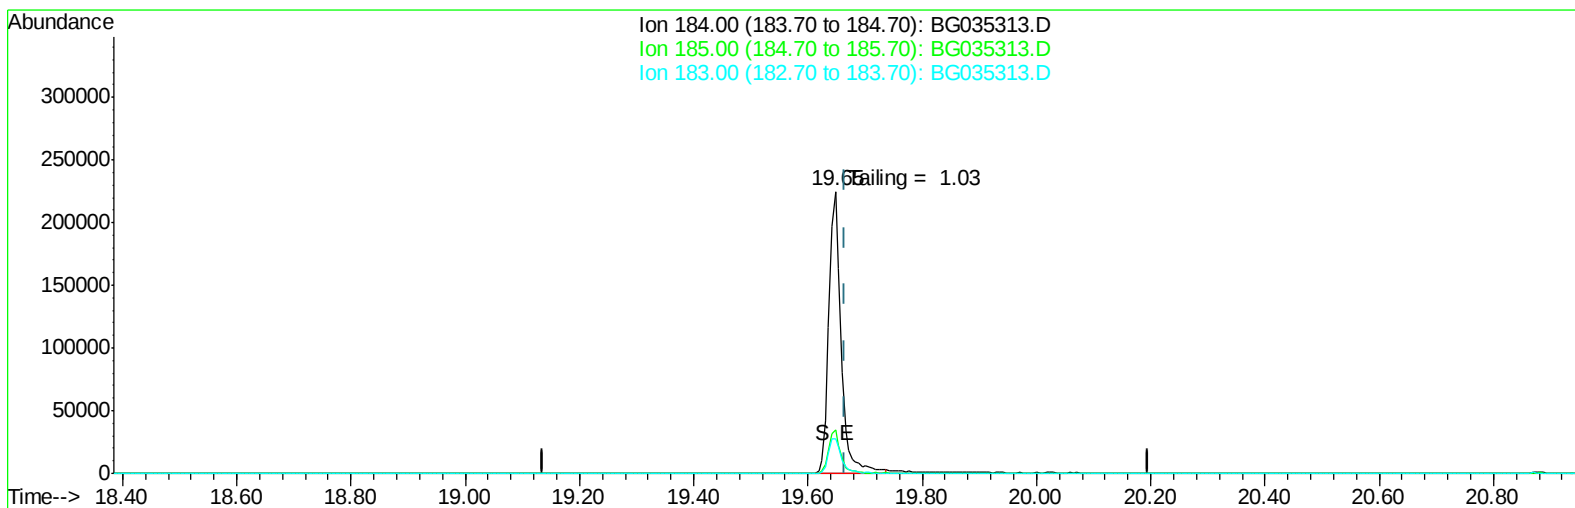

TIC: BG035313.D

(76) Benzidine

19.648min (-0.019) 0.00ng

response 341162

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.49
183.00	13.30	12.24
0.00	0.00	0.00