

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062118\
 Data File : BG035326.D
 Acq On : 22 Jun 2018 9:33
 Operator : JU/SJ
 Sample : J3603-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 26KV-TP-11

Quant Time: Jun 22 10:53:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	51344	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	175167	20.00	ng	-0.02
38) Acenaphthene-d10	14.67	164	116541	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	321572	20.00	ng	-0.02
75) Chrysene-d12	21.68	240	354589	20.00	ng	-0.04
86) Perylene-d12	24.90	264	329324	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	406191	133.51	ng	0.00
7) Phenol-d6	7.21	99	502819	111.98	ng	-0.01
23) Nitrobenzene-d5	9.22	82	423806	115.01	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	279283	187.20	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	906293	101.10	ng	-0.03
78) Terphenyl-d14	20.02	244	1731158	102.27	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062118\
Data File : BG035326.D
Acq On : 22 Jun 2018 9:33
Operator : JU/SJ
Sample : J3603-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
26KV-TP-11

Quant Time: Jun 22 10:53:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

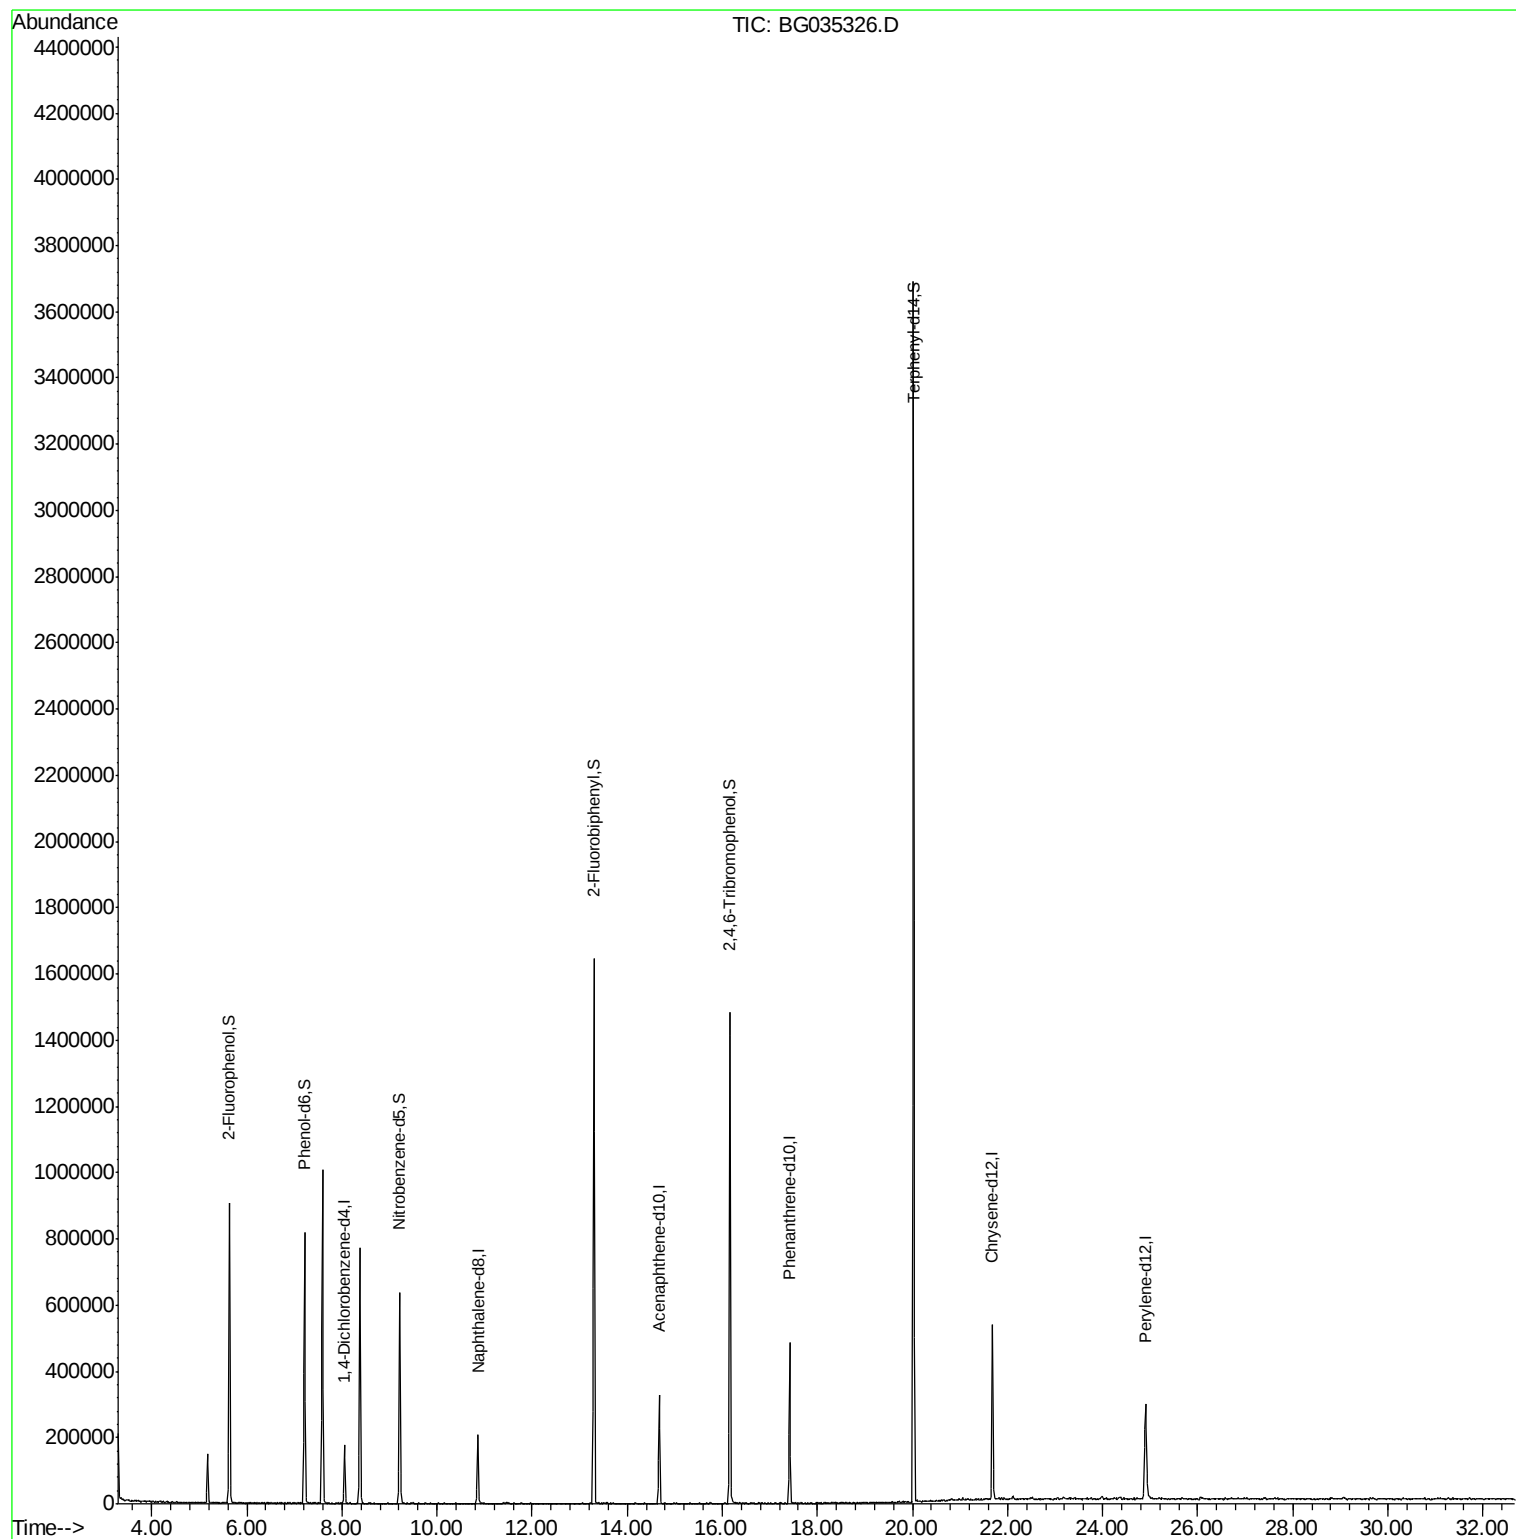

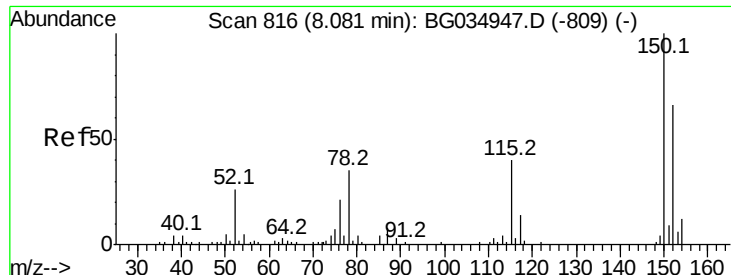


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 811
Delta R.T. -0.02 min
Lab File: BG035326.D
Acq: 22 Jun 2018 9:33

Instrument :
BNA_G
ClientSampleId :
26KV-TP-11

Tot Ion:152 Resp: 51344
Ion Ratio Lower Upper
152 100
150 134.4 126.6 189.8
115 59.2 53.0 79.4

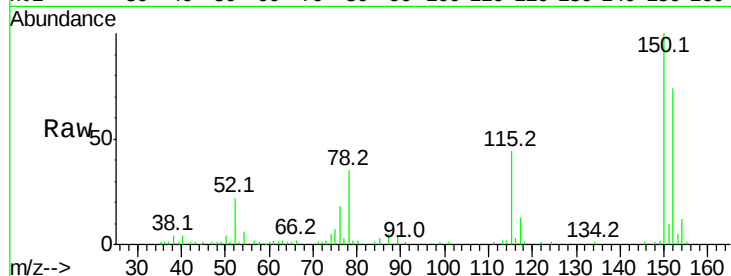


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

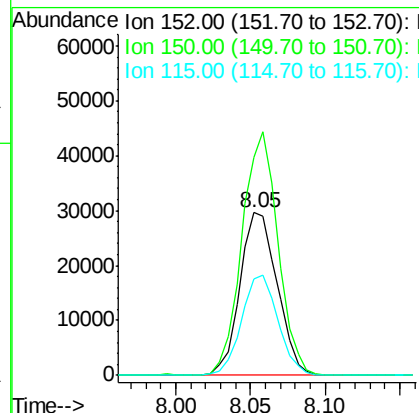



#5


2-Fluorophenol
Concen: 133.509 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG035326.D
Acq: 22 Jun 2018 9:33

Tgt Ion:112 Resp: 406191
Ion Ratio Lower Upper
112 100
64 61.8 56.3 84.5
63 33.5 30.1 45.1

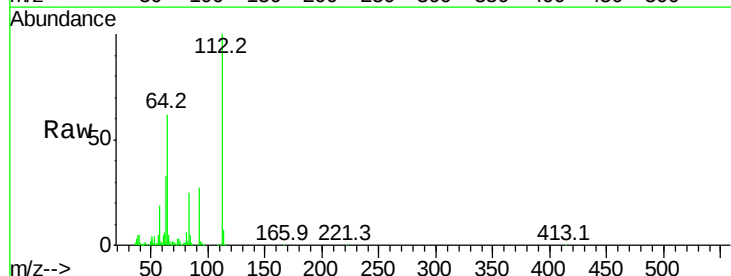

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

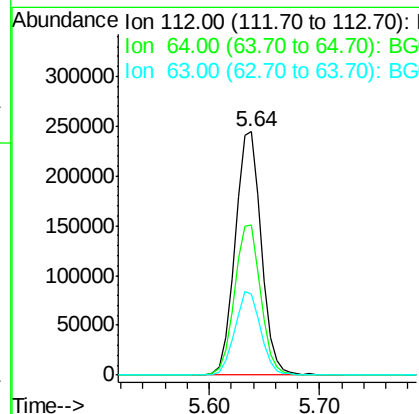

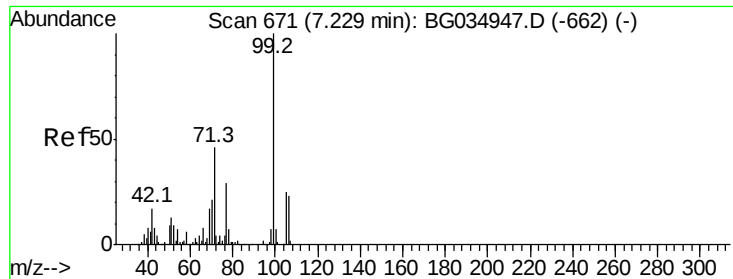

#7

Phenol-d6

Concen: 111.976 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33

Instrument :

BNA_G

ClientSampleId :

26KV-TP-11


Tot Ion: 99 Resp: 502819

Ion Ratio Lower Upper




99 100

42 15.2 14.1 21.1

71 42.0 26.1 39.1#

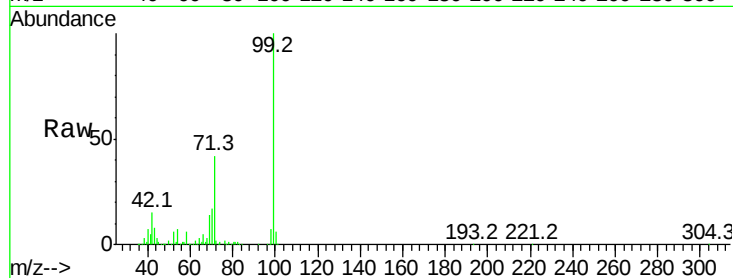

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

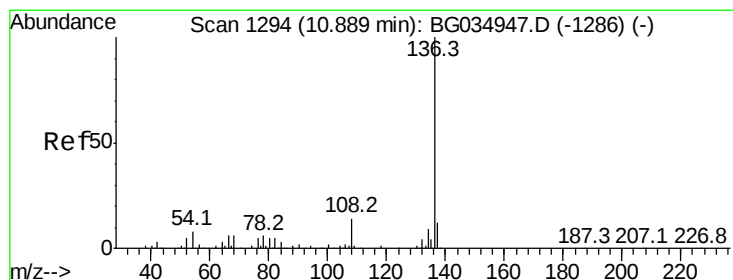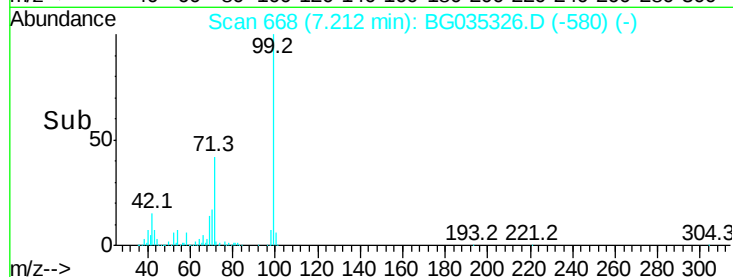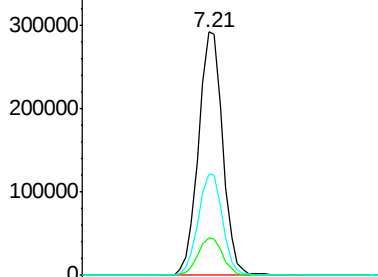

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.02 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33

Tgt Ion: 136 Resp: 175167


Ion Ratio Lower Upper

136 100



137 11.4 9.2 13.8


54 6.7 10.3 15.5#

68 4.4 4.5 6.7#

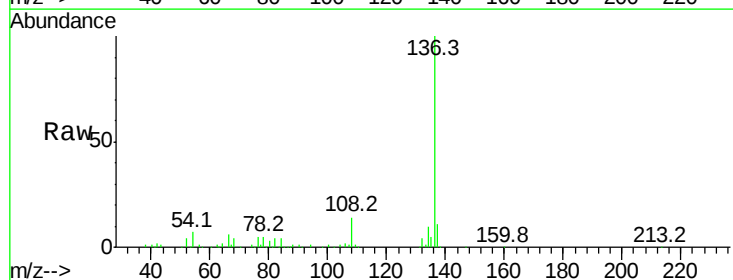

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

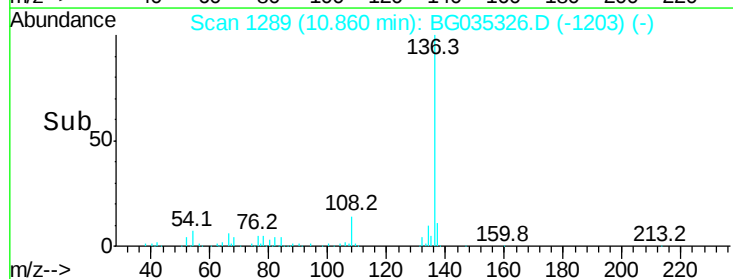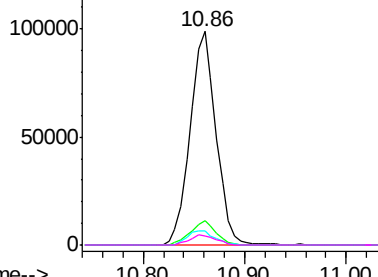

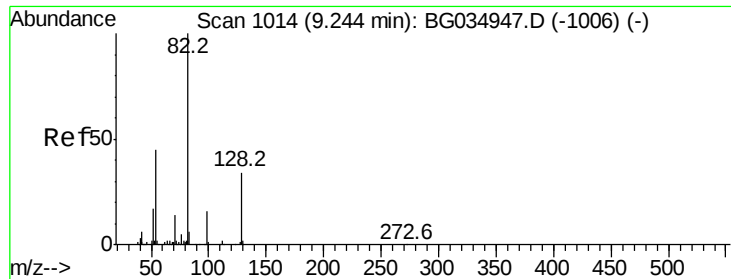

#23

Nitrobenzene-d5

Concen: 115.006 ng

RT: 9.22 min Scan# 1009

Delta R.T. -0.02 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33

Instrument :

BNA_G

ClientSampleId :

26KV-TP-11


Tot Ion: 82 Resp: 423806

Ion Ratio Lower Upper

82 100

128 36.3 29.7 44.5




54 41.2 43.1 64.7#

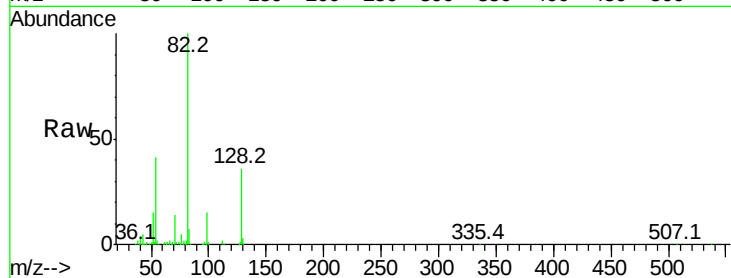

Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

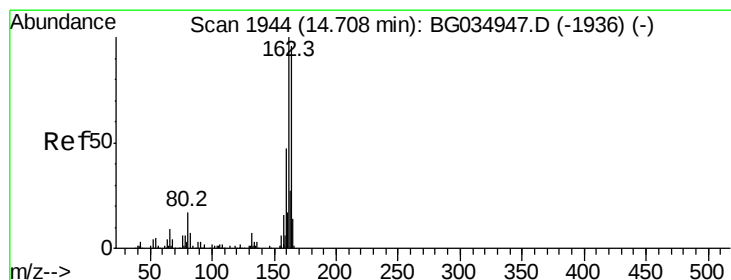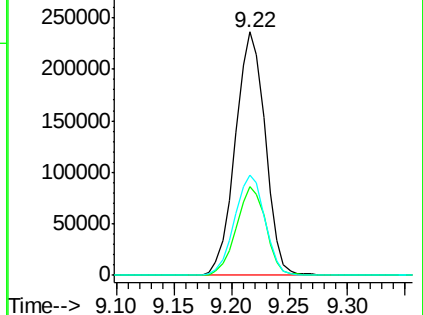

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1938

Delta R.T. -0.02 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33


Tgt Ion:164 Resp: 116541

Ion Ratio Lower Upper

164 100

162 93.8 78.8 118.2



160 43.6 35.4 53.0

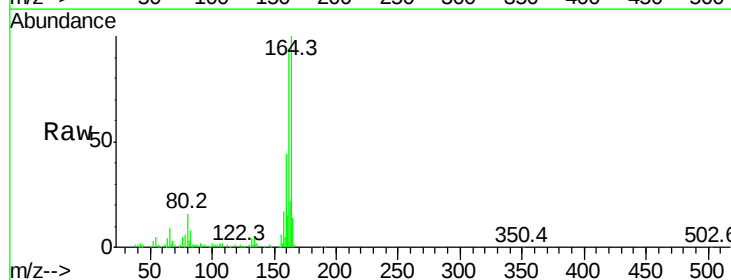


Abundance Ion 164.00 (163.70 to 164.70): BGC

Ion 162.00 (161.70 to 162.70): BGC

Ion 160.00 (159.70 to 160.70): BGC

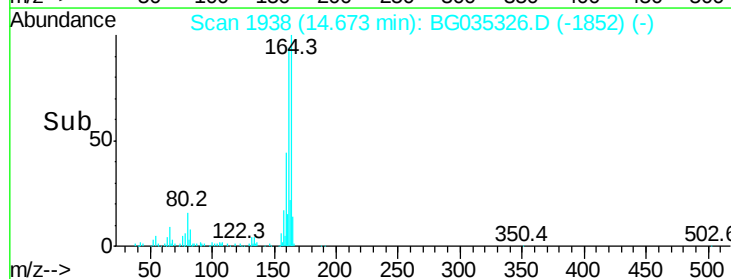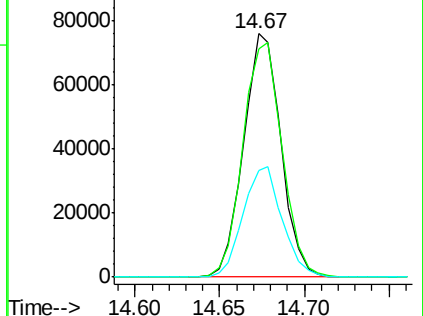


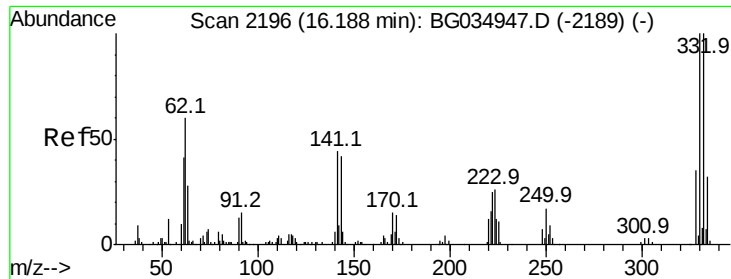




#41
 2,4,6-Tribromophenol
 Concen: 187.203 ng
 RT: 16.16 min Scan# 2192
 Delta R.T. -0.02 min
 Lab File: BG035326.D
 Acq: 22 Jun 2018 9:33

Instrument :
 BNA_G
 ClientSampleId :
 26KV-TP-11

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	77.0	115.6
141	37.3	25.2	37.8

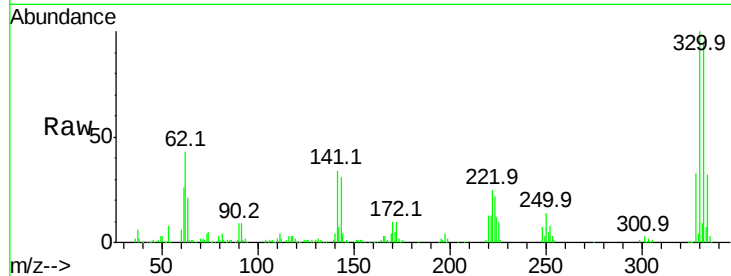


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

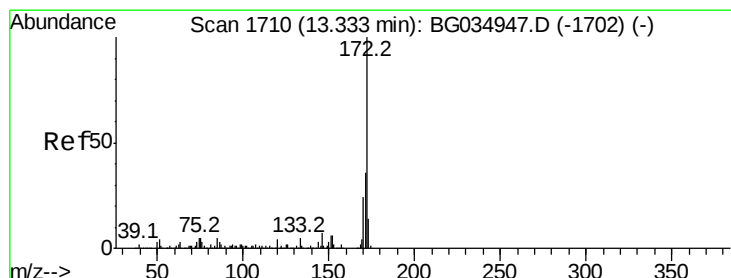
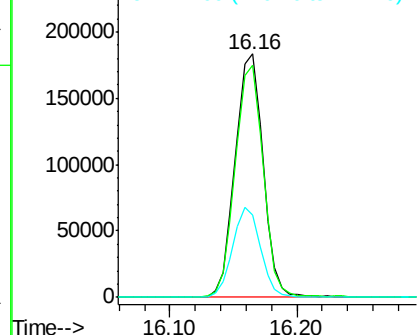



#44
 2-Fluorobiphenyl
 Concen: 101.096 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.03 min
 Lab File: BG035326.D
 Acq: 22 Jun 2018 9:33

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.6	30.0	45.0
170	22.5	19.5	29.3

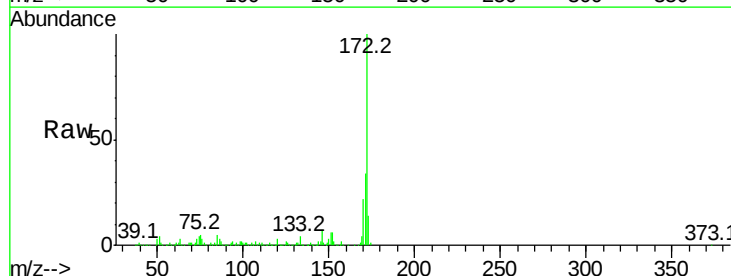

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

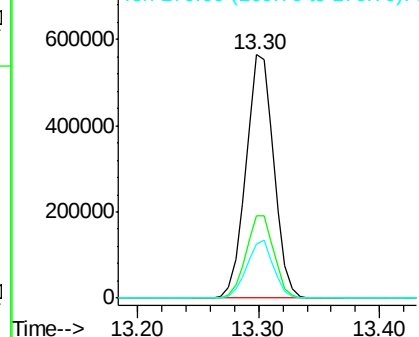



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2405

Delta R.T. -0.02 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33

Instrument :

BNA_G

ClientSampleId :

26KV-TP-11


Tot Ion:188 Resp: 321572

Ion Ratio Lower Upper

188 100

94 6.1 6.9 10.3#




80 7.4 7.7 11.5#

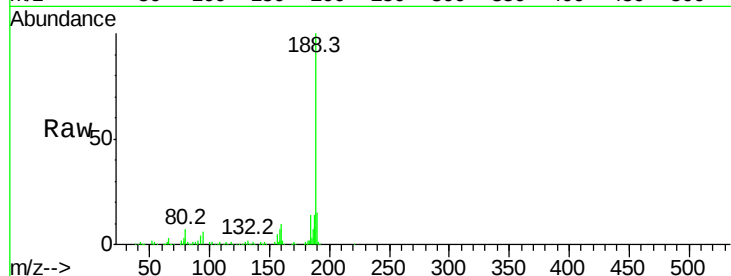

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

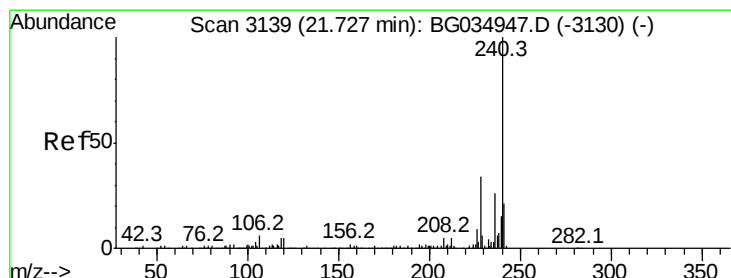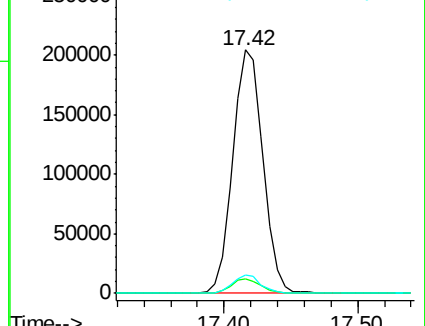

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3131

Delta R.T. -0.04 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33


Tgt Ion:240 Resp: 354589

Ion Ratio Lower Upper

240 100

120 4.4 6.8 10.2#



236 25.2 20.9 31.3

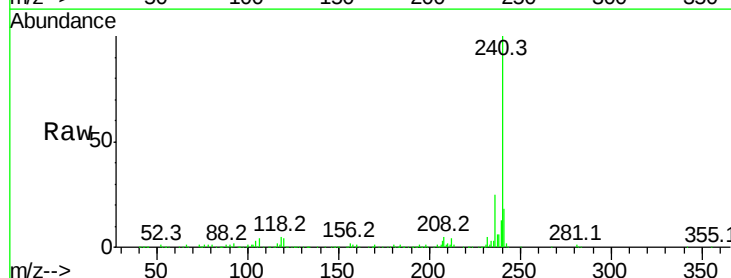


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

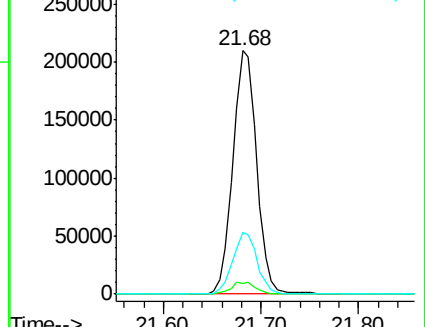



#78

Terphenyl-d14

Concen: 102.265 ng

RT: 20.02 min Scan# 2849

Delta R.T. -0.02 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33

Instrument :

BNA_G

ClientSampleId :

26KV-TP-11


Tot Ion:244 Resp: 1731158

Ion Ratio Lower Upper

244 100

212 9.4 5.8 8.8#




122 6.8 7.0 10.4#

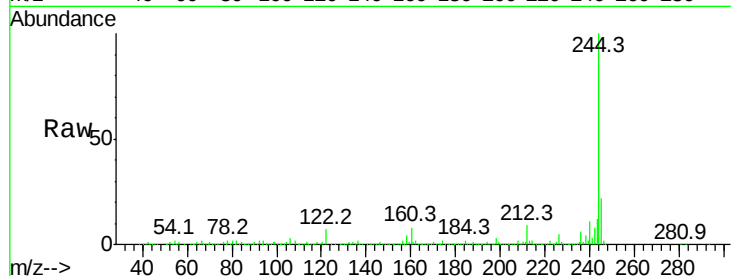

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

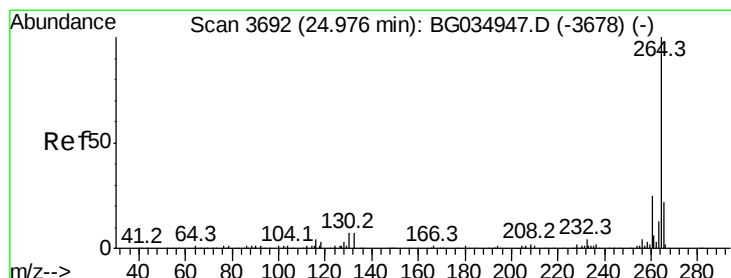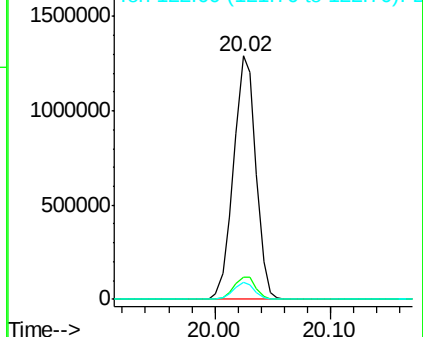

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.90 min Scan# 3679

Delta R.T. -0.05 min

Lab File: BG035326.D

Acq: 22 Jun 2018 9:33


Tgt Ion:264 Resp: 329324

Ion Ratio Lower Upper

264 100

260 24.8 17.4 26.0

265 21.2 17.7 26.5

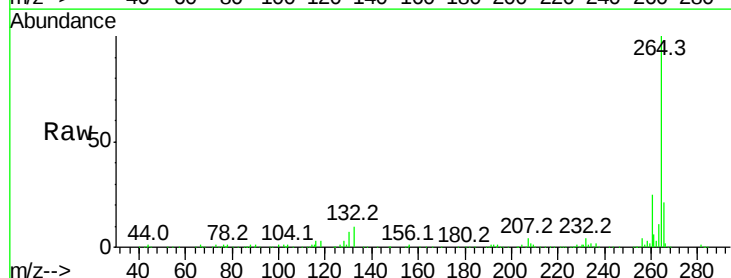

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

