


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062118\
 Data File : BG035295.D
 Acq On : 21 Jun 2018 12:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

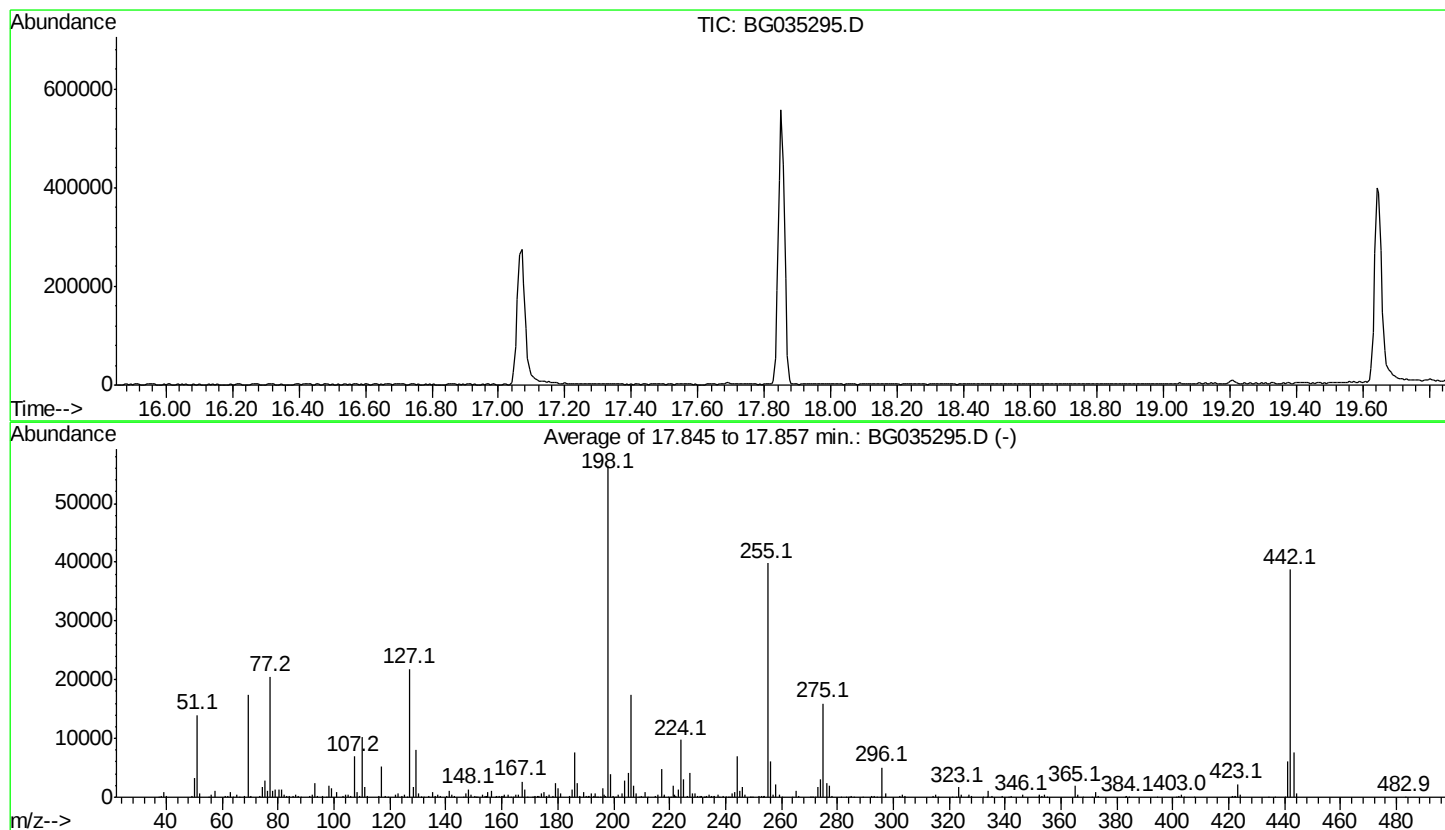

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	14057	PASS
68	69	0.00	2	0.9	151	PASS
69	198	0.00	100	31.1	17531	PASS
70	69	0.00	2	0.9	158	PASS
127	198	10	80	38.7	21821	PASS
197	198	0.00	2	0.8	434	PASS
198	198	100	100	100.0	56434	PASS
199	198	5	9	7.0	3960	PASS
275	198	10	60	28.4	16017	PASS
365	198	1	100	3.4	1902	PASS
441	443	0.01	100	80.9	6120	PASS
442	198	50	100	68.7	38746	PASS
443	442	15	24	19.5	7561	PASS