


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062118\
 Data File : BG035313.D
 Acq On : 22 Jun 2018 1:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

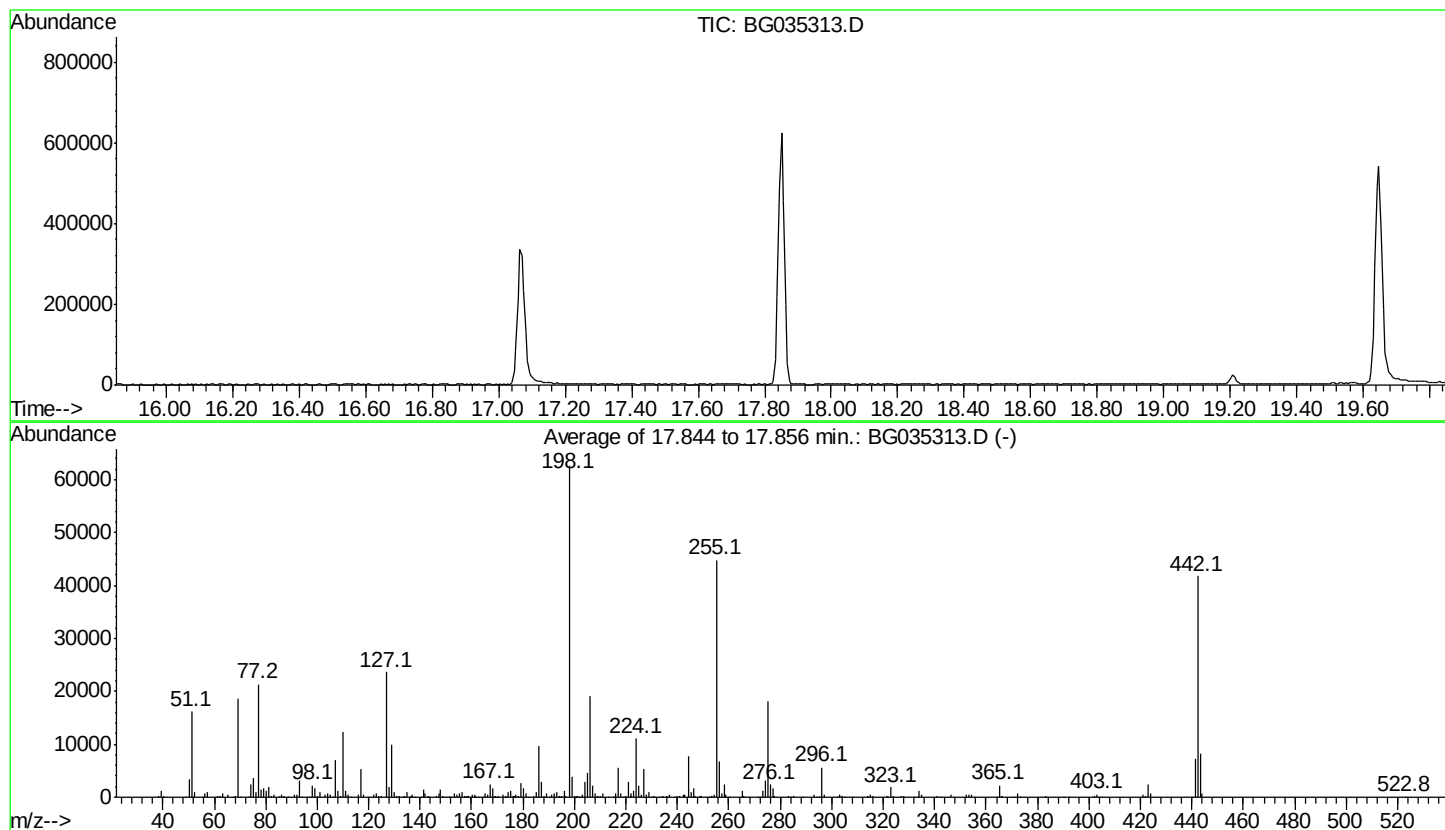

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	16181	PASS
68	69	0.00	2	1.4	267	PASS
69	198	0.00	100	29.7	18606	PASS
70	69	0.00	2	0.5	84	PASS
127	198	10	80	37.7	23621	PASS
197	198	0.00	2	0.3	203	PASS
198	198	100	100	100.0	62634	PASS
199	198	5	9	6.3	3967	PASS
275	198	10	60	29.1	18242	PASS
365	198	1	100	3.6	2231	PASS
441	443	0.01	100	88.7	7286	PASS
442	198	50	100	66.8	41816	PASS
443	442	15	24	19.6	8215	PASS