
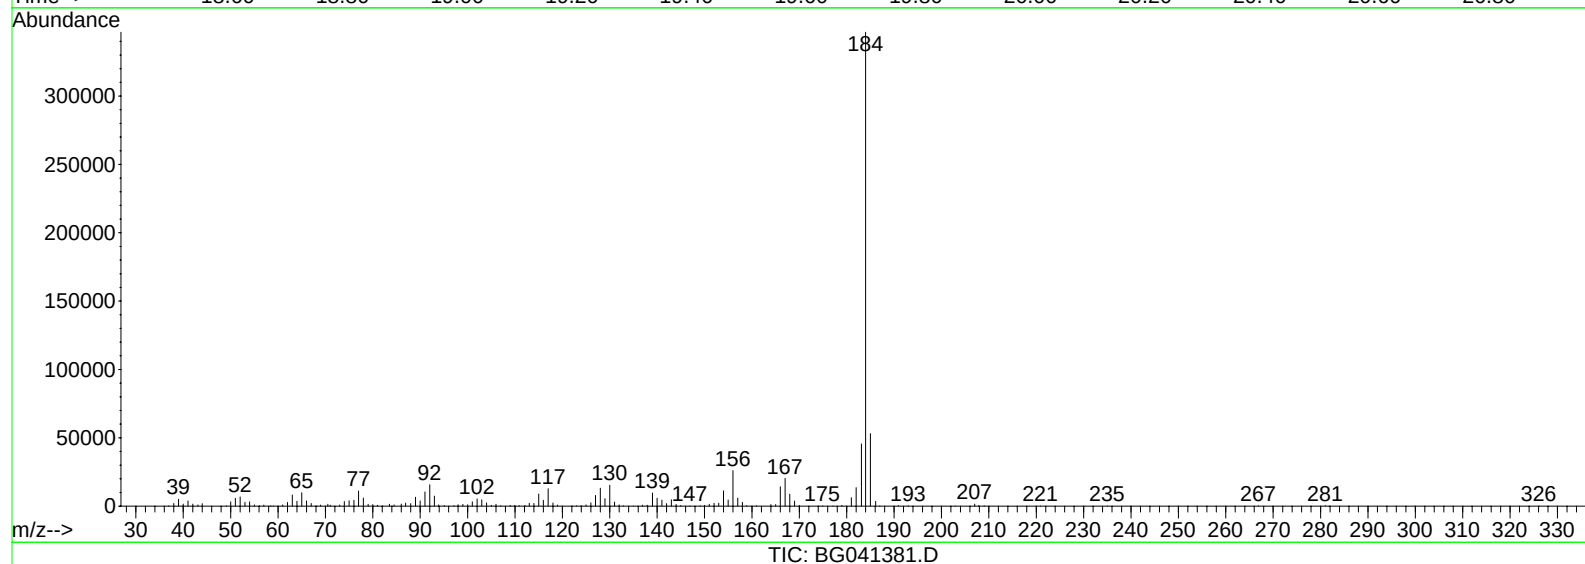


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062119\
Data File : BG041381.D
Acq On : 21 Jun 2019 18:03
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:34:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

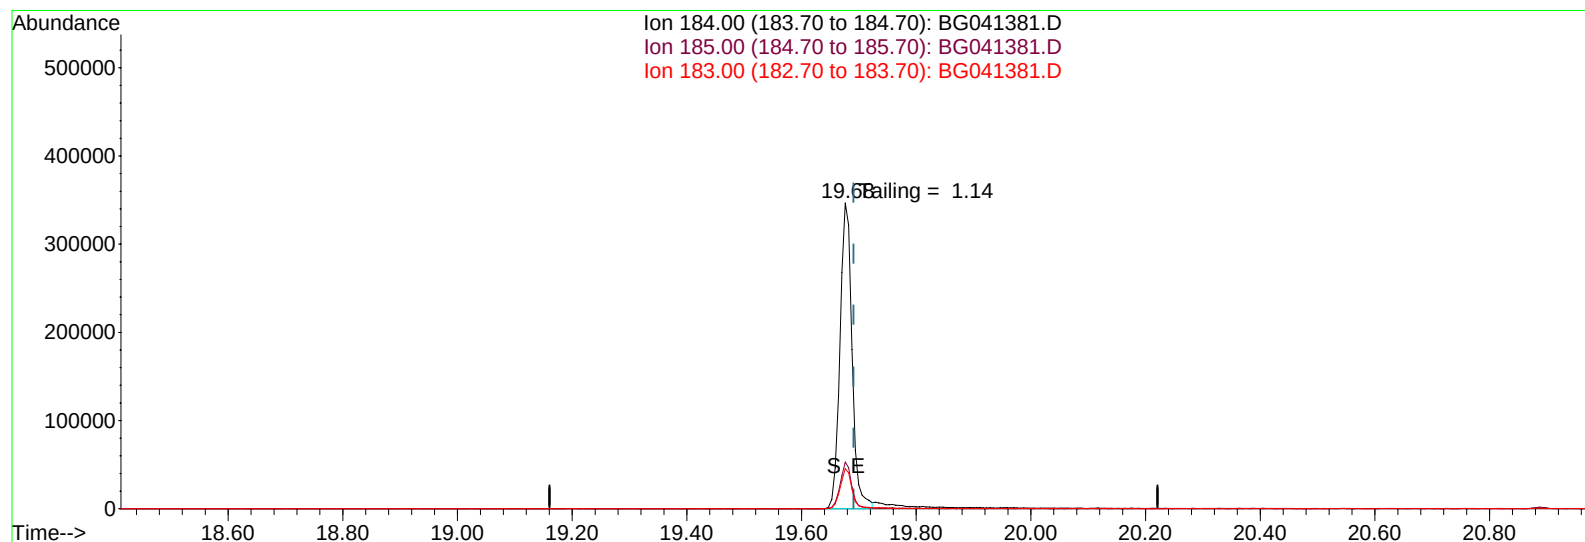

(77) Benzidine



19.676min (-0.015) 316119.25ng

response 527587

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.28
183.00	12.00	13.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062119\
Data File : BG041381.D
Acq On : 21 Jun 2019 18:03
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:34:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

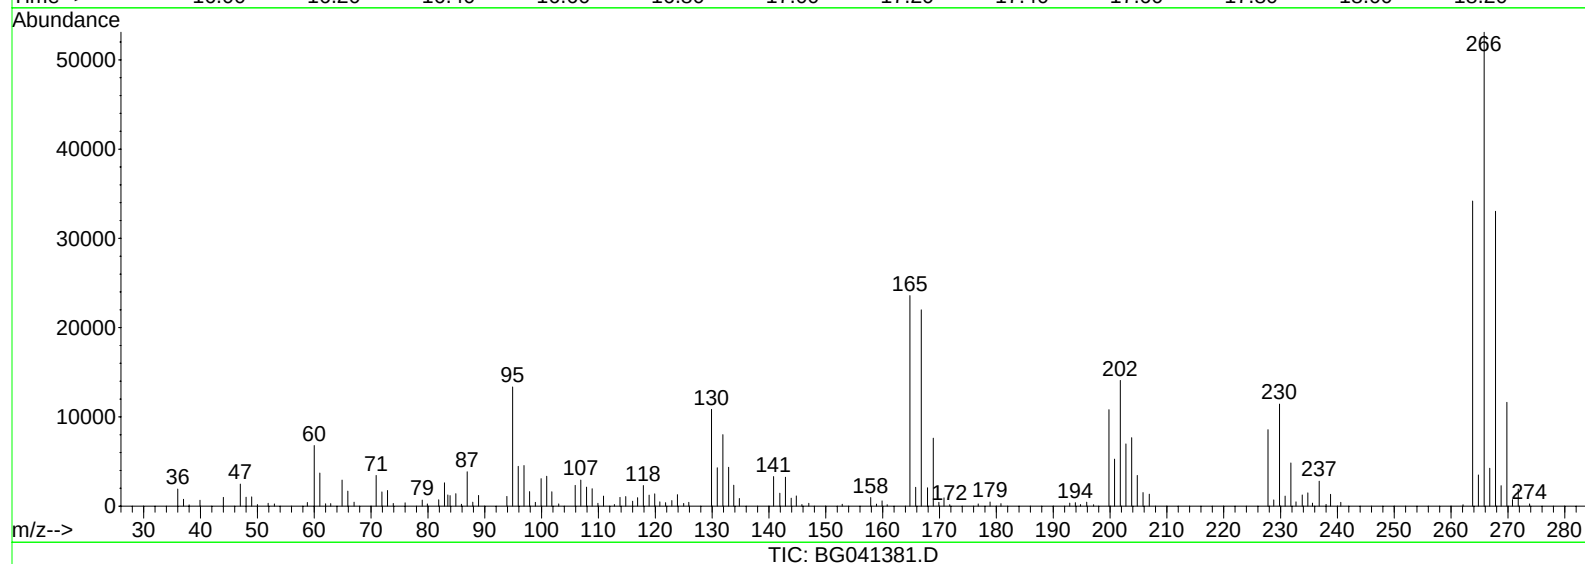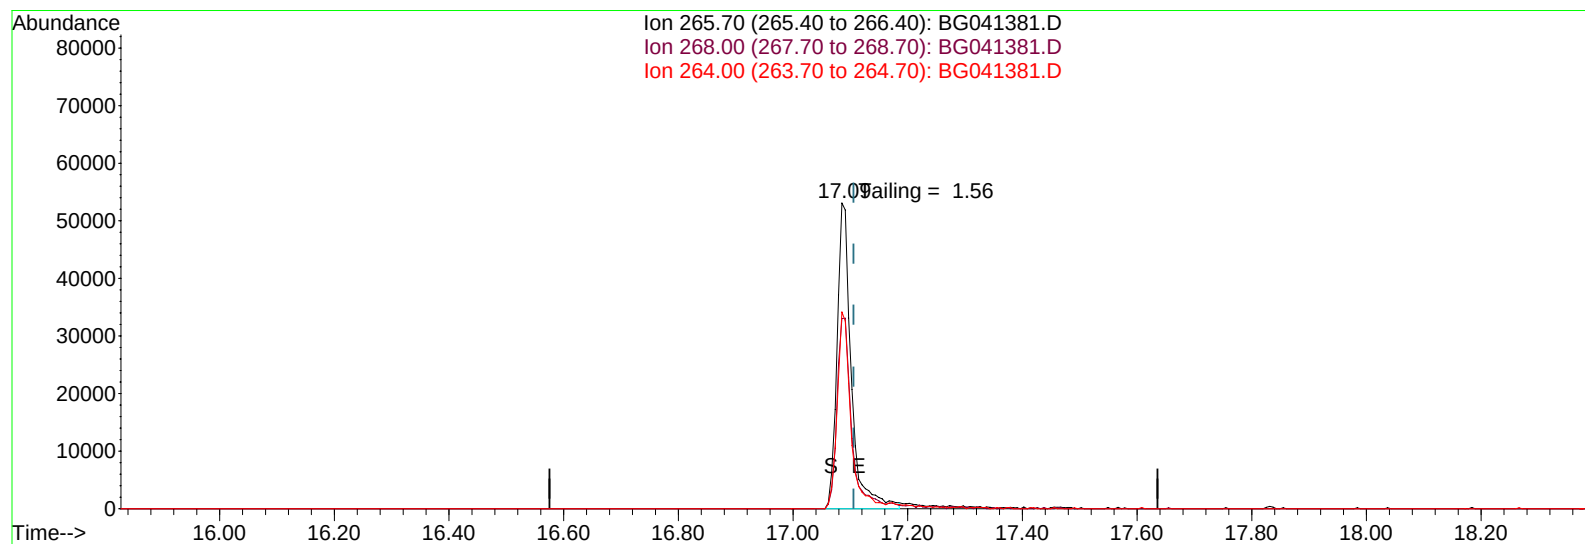

(70) Pentachlorophenol (C)

17.085min (-0.020) 32265.19ng

response 94250

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.23
264.00	64.00	64.38
0.00	0.00	0.00