
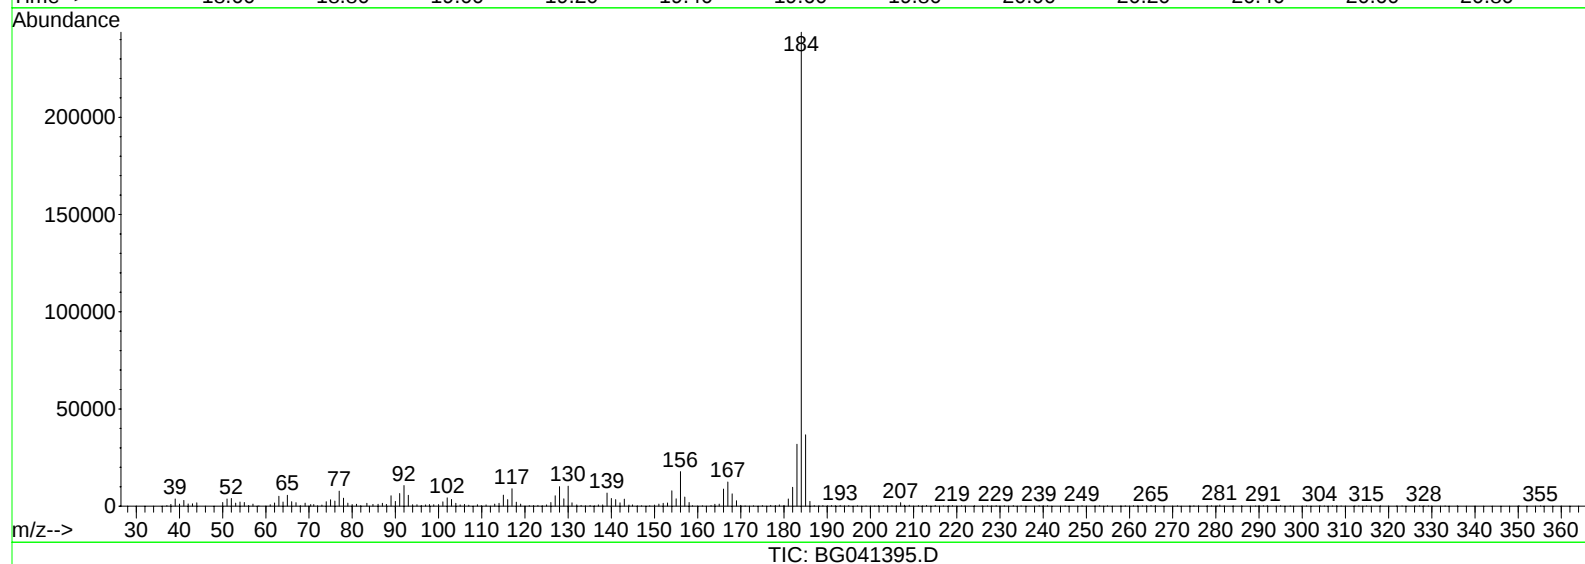


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062119\
Data File : BG041395.D
Acq On : 22 Jun 2019 5:25
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:11:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

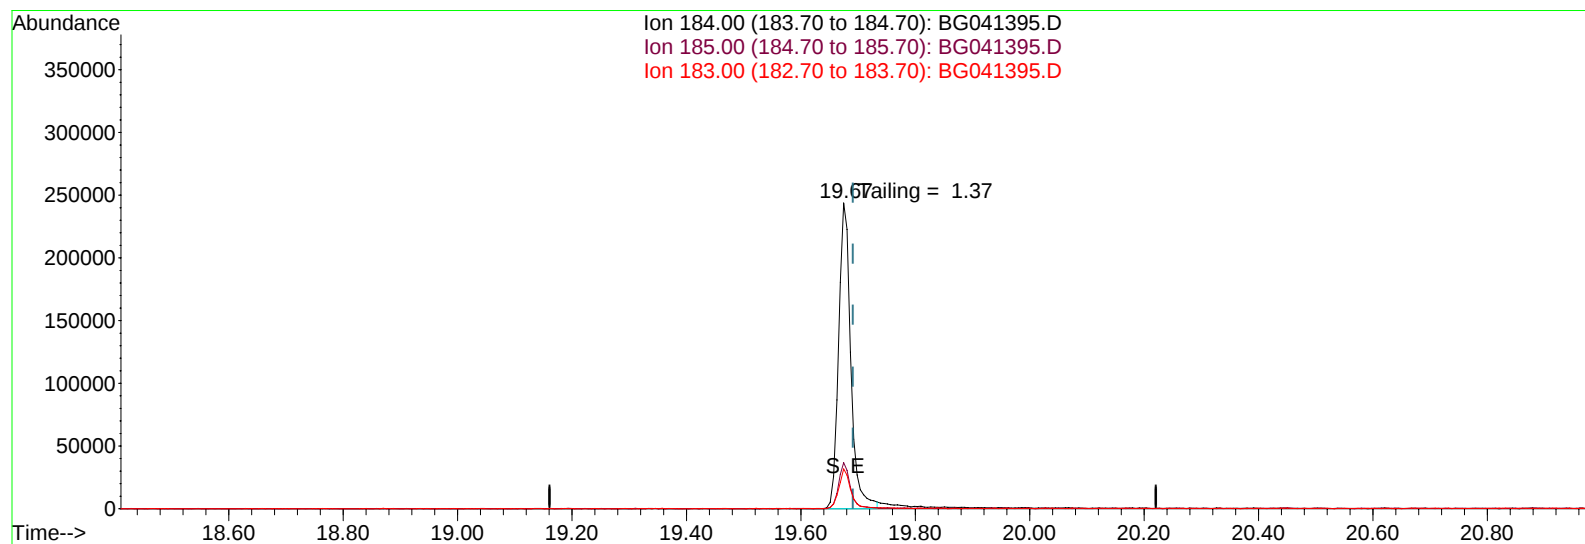

TIC: BG041395.D

(77) Benzidine



19.675min (-0.016) 108466.10ng

response 372543

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.06
183.00	12.00	13.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062119\
Data File : BG041395.D
Acq On : 22 Jun 2019 5:25
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:11:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

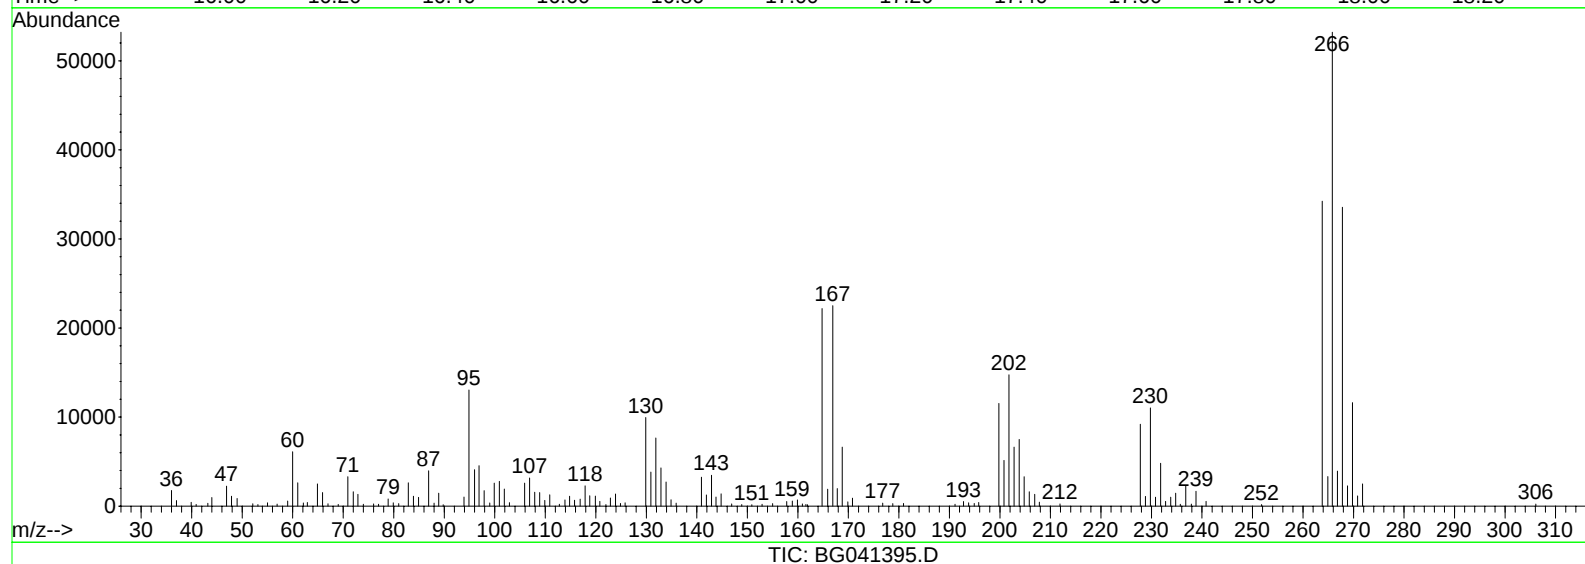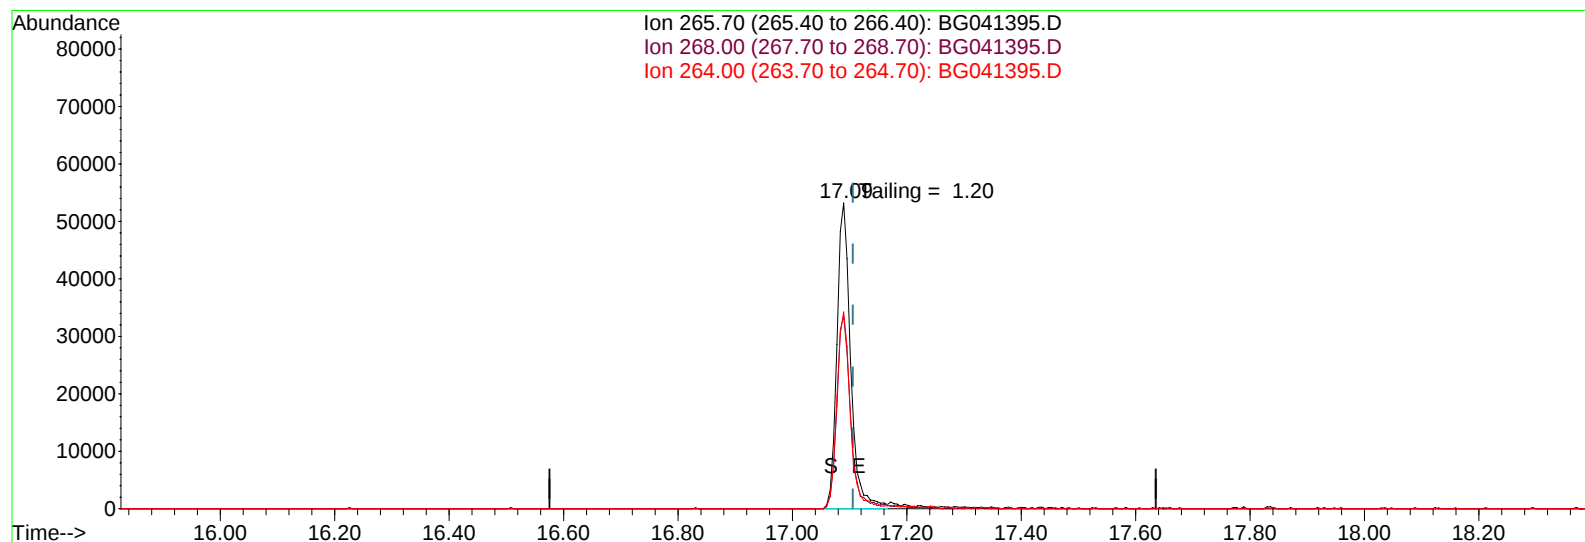

(70) Pentachlorophenol (C)

17.089min (-0.016) 32497.66ng

response 88708

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.07
264.00	64.00	64.37
0.00	0.00	0.00