
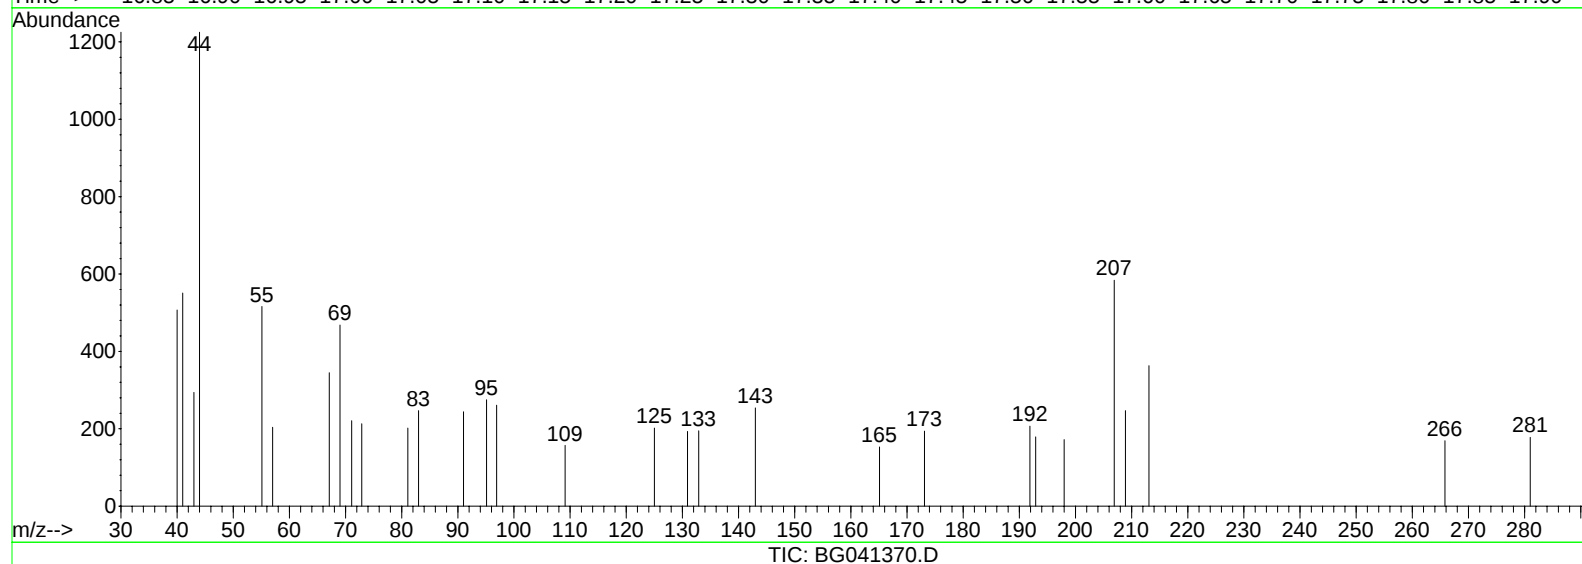


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062119\
Data File : BG041370.D
Acq On : 21 Jun 2019 8:58
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 02:14:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

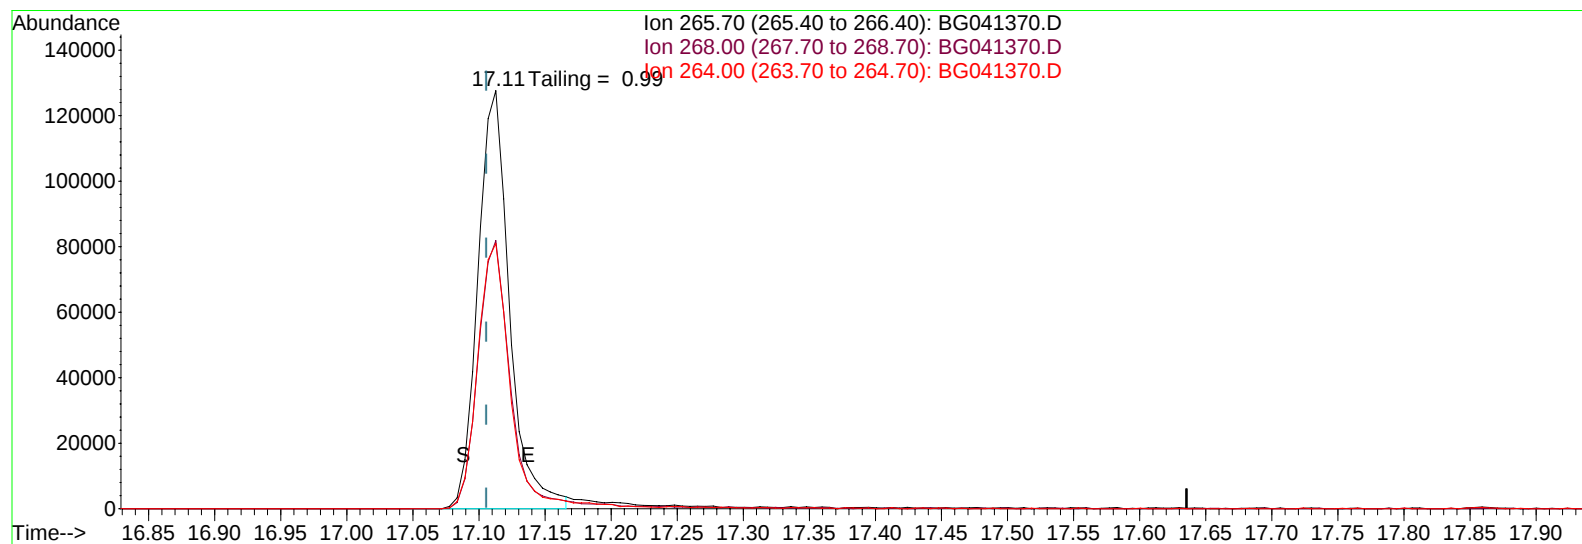

(70) Pentachlorophenol (C)



18.535min (+1.429) 253.44ng

response 115

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	0.00#
264.00	64.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062119\
 Data File : BG041370.D
 Acq On : 21 Jun 2019 8:58
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 02:14:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 14:58:02 2019
 Response via : Initial Calibration

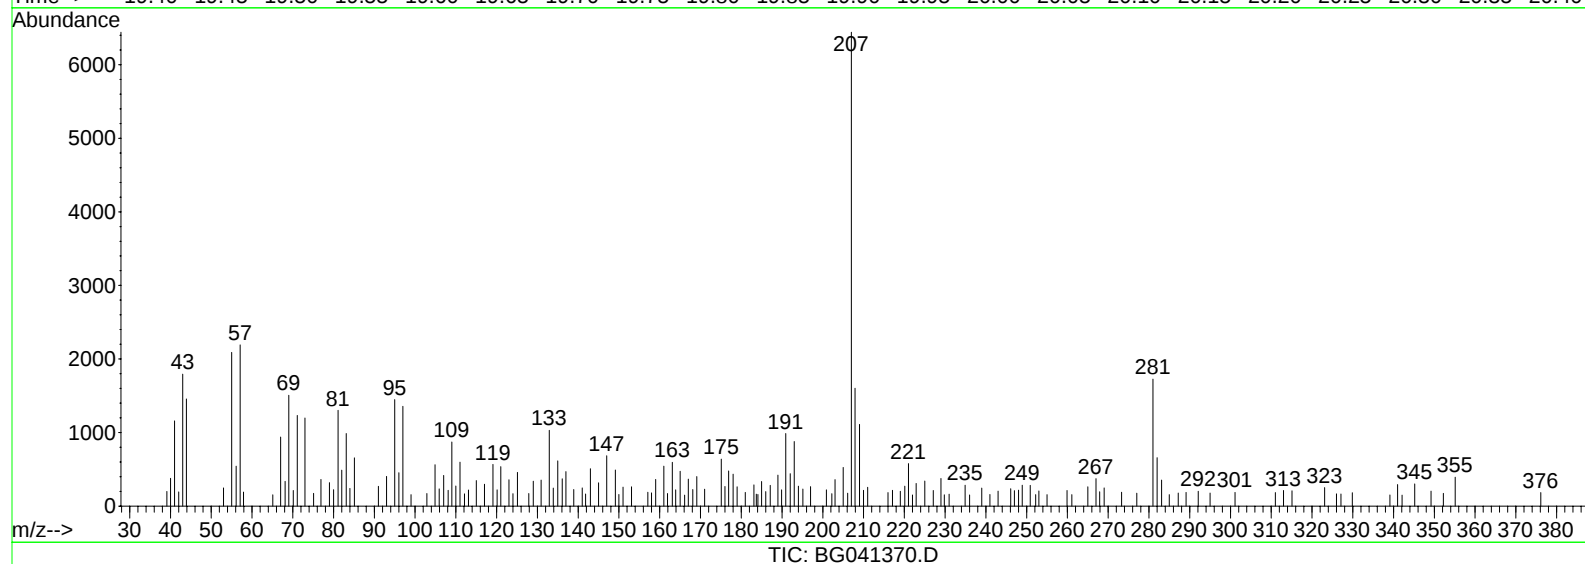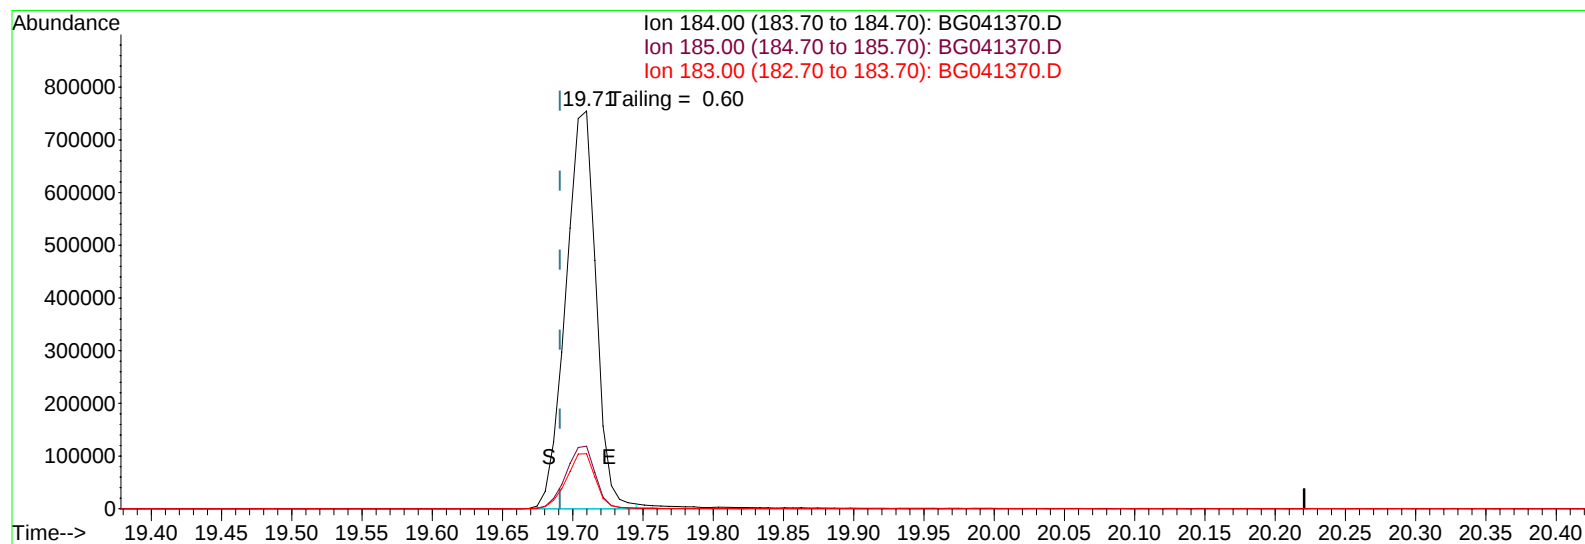

(77) Benzidine

21.361min (+1.670) 220.76ng

response 283

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	104.35#
183.00	12.00	140.68#
0.00	0.00	0.00