

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062119\
 Data File : BG041373.D
 Acq On : 21 Jun 2019 11:31
 Operator : HP/JU
 Sample : PB120785BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120785BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.608	422	429	443	rBV	468313	759630	33.82%	7.460%
2	7.224	695	704	716	rBV	472719	839419	37.37%	8.244%
3	7.600	761	768	779	rBV	467642	807545	35.95%	7.931%
4	8.070	842	848	859	rVB	104392	175885	7.83%	1.727%
5	8.393	895	903	913	rBV	370089	641255	28.55%	6.298%
6	9.251	1042	1049	1059	rBV	279406	523601	23.31%	5.142%
7	10.896	1322	1329	1338	rBV	112479	217307	9.68%	2.134%
8	13.328	1736	1743	1753	rBV	795663	1211399	53.94%	11.897%
9	14.709	1970	1978	1990	rBV2	193268	316882	14.11%	3.112%
10	16.201	2225	2232	2251	rBV	576486	942280	41.95%	9.254%
11	17.459	2439	2446	2465	rBV	273229	429548	19.13%	4.219%
12	20.056	2881	2888	2896	rBV	1729541	2246000	100.00%	22.058%
13	21.730	3167	3173	3181	rBV2	320155	545398	24.28%	5.356%
14	25.044	3728	3737	3747	rVB2	181531	525922	23.42%	5.165%


Sum of corrected areas: 10182071

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062119\
Data File : BG041373.D
Acq On : 21 Jun 2019 11:31
Operator : HP/JU
Sample : PB120785BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120785BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

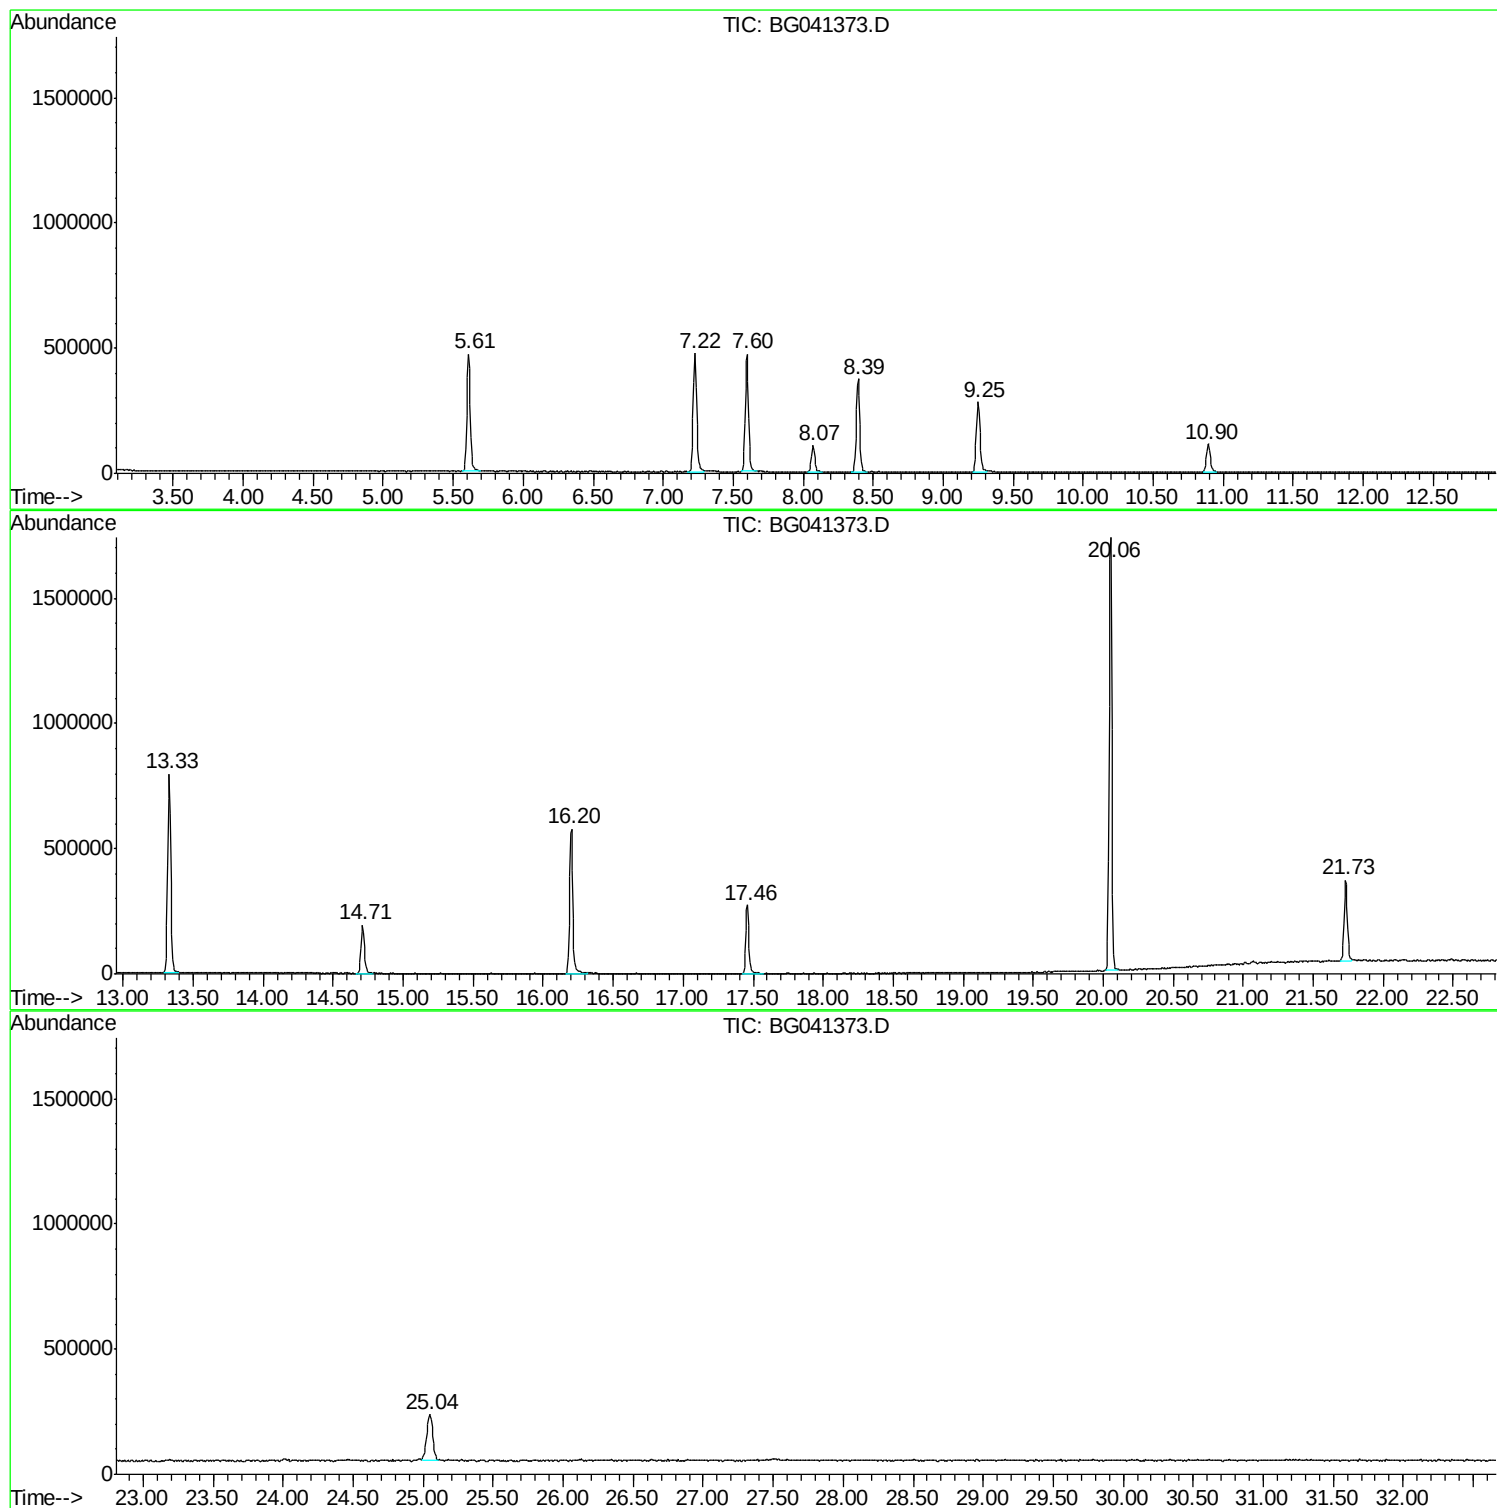

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062119\
Data File : BG041373.D
Acq On : 21 Jun 2019 11:31
Operator : HP/JU
Sample : PB120785BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120785BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.60	91.83 ng	807545	1,4-Dichlorobenzene-d4	8.07

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		5-Aminoindole	132	C8H8N2	005192-03-0	22
5		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16

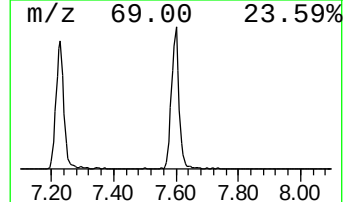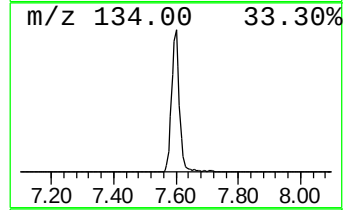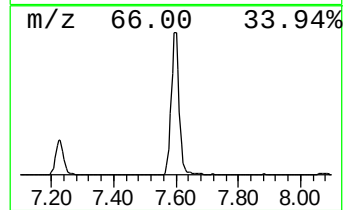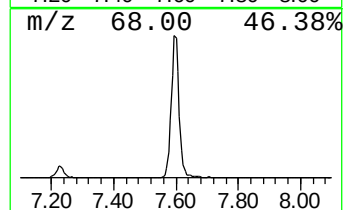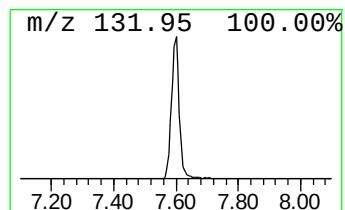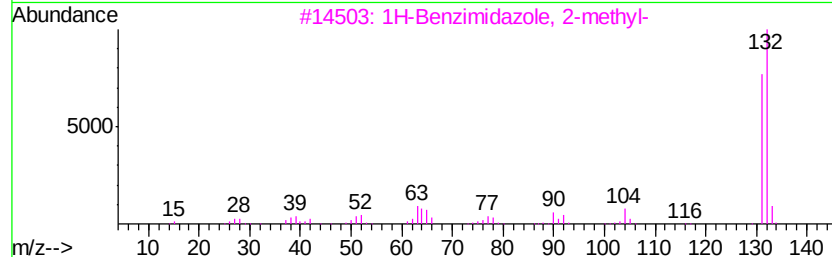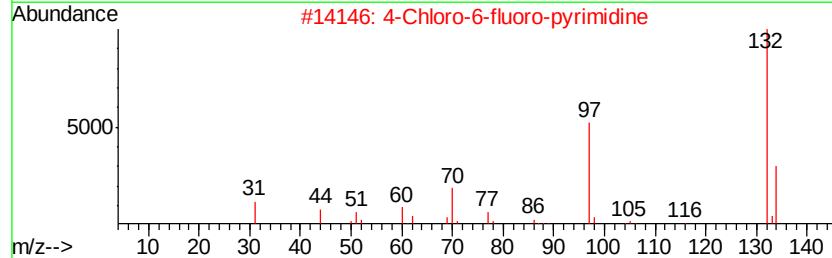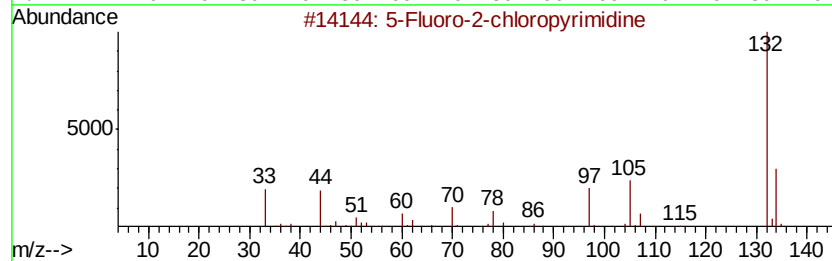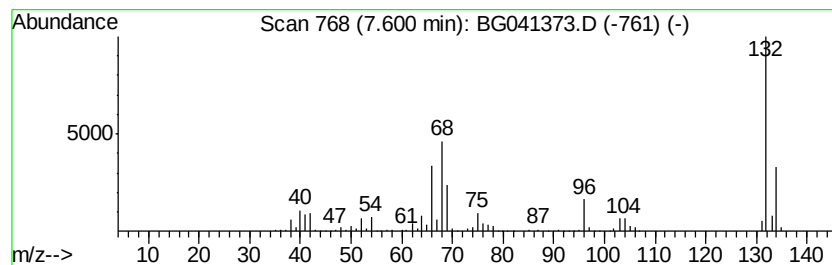

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062119\
Data File : BG041373.D
Acq On : 21 Jun 2019 11:31
Operator : HP/JU
Sample : PB120785BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120785BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.60	7.60	91.8	ng	807545	1	8.07	175885	20.0