


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062119\
 Data File : BG041370.D
 Acq On : 21 Jun 2019 8:58
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

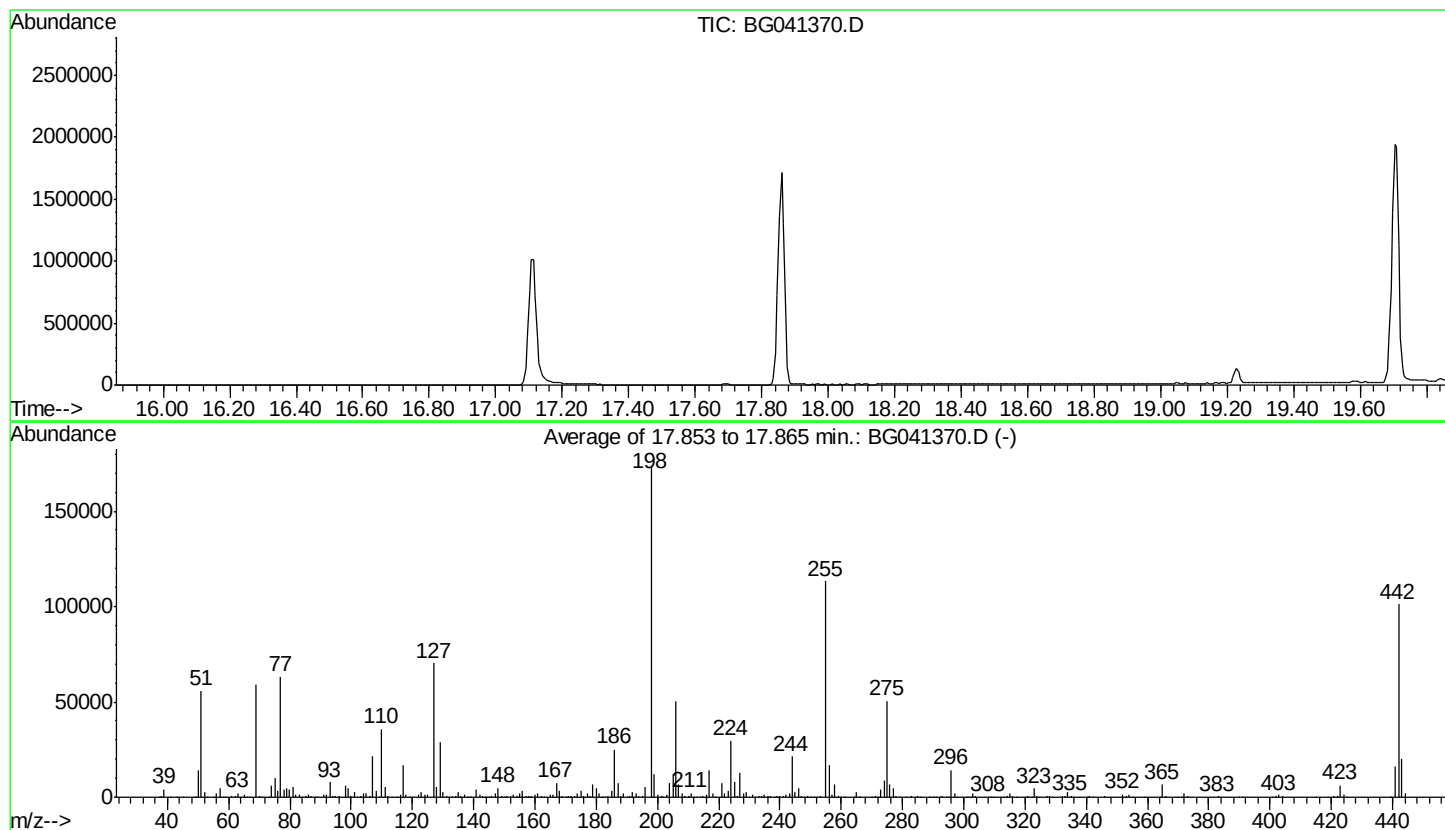

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	55866	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.0	59146	PASS
70	69	0.00	2	0.7	391	PASS
127	198	10	80	40.5	70338	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	173888	PASS
199	198	5	9	6.9	12073	PASS
275	198	10	60	29.1	50610	PASS
365	198	1	100	3.7	6520	PASS
441	198	0.01	100	9.2	16060	PASS
442	198	50	100	58.2	101216	PASS
443	442	15	24	19.9	20099	PASS