


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062119\
 Data File : BG041381.D
 Acq On : 21 Jun 2019 18:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

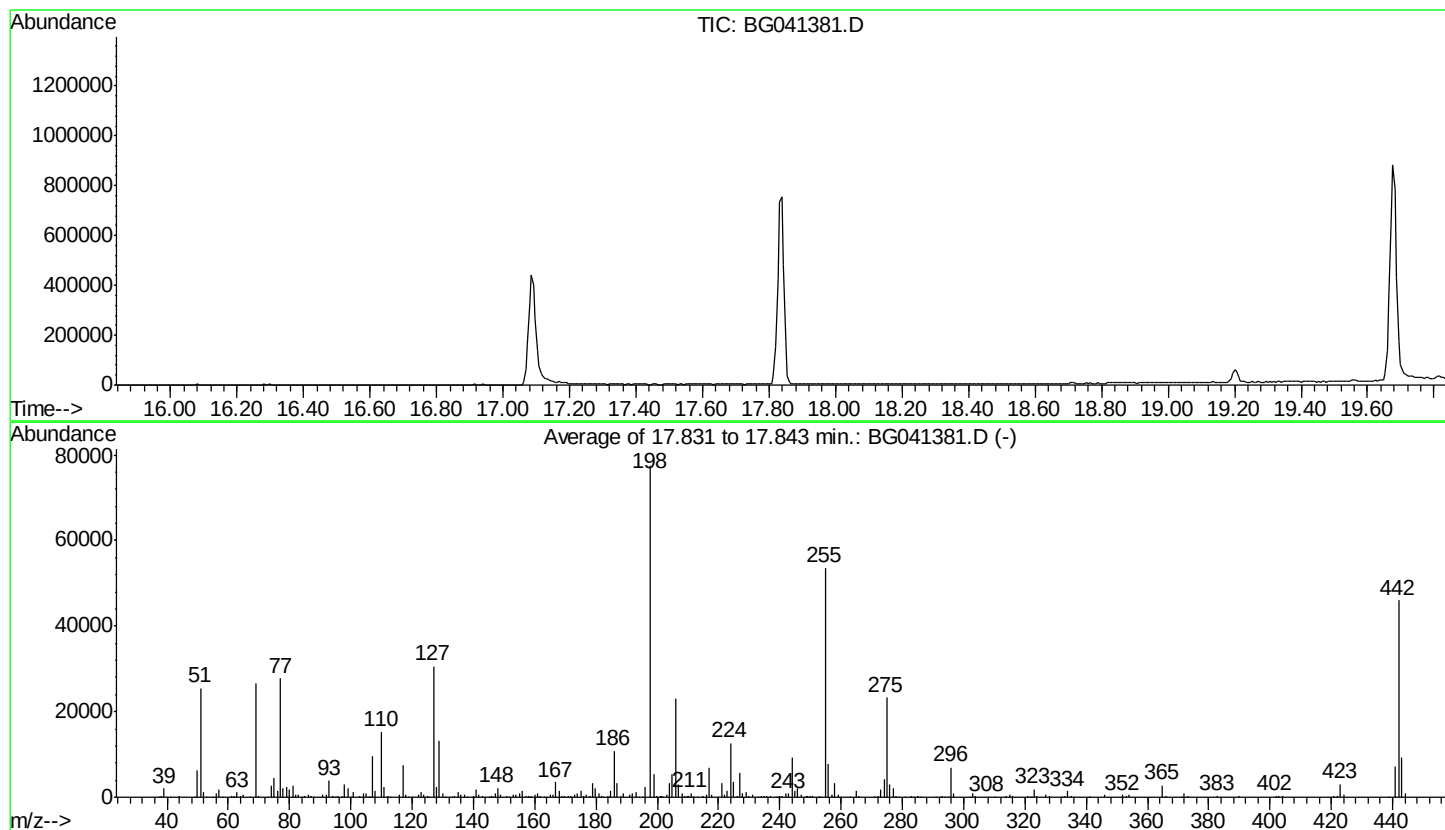

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	25486	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.2	26507	PASS
70	69	0.00	2	0.9	234	PASS
127	198	10	80	39.4	30517	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77490	PASS
199	198	5	9	6.8	5302	PASS
275	198	10	60	30.1	23330	PASS
365	198	1	100	3.6	2767	PASS
441	198	0.01	100	9.4	7311	PASS
442	198	50	100	59.4	46040	PASS
443	442	15	24	20.4	9391	PASS