

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053971.D
 Acq On : 21 Jun 2022 10:17
 Operator : CG/JU
 Sample : PB145611BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jun 21 23:06:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.076	152	19258	20.000	ng/ul	0.00
20) Naphthalene-d8	10.885	136	75402	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.704	164	59861	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.442	188	161272	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.719	240	180912	20.000	ng/ul	# 0.00
88) Perylene-d12	24.980	264	182647	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.505	96	2332	5.762	ng/uL	0.00
4) Pyridine-d5	3.916	84	33858	30.755	ng/ul	0.00
7) Phenol-d5	7.230	99	43739	31.703	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.395	67	26437	31.766	ng/ul	0.00
11) 2-Chlorophenol-d4	7.606	132	36813	33.460	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	36673	31.175	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	17864	31.918	ng/ul	0.00
24) 2-Nitrophenol-d4	9.962	143	20379	34.270	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.503	165	40787	31.001	ng/ul	0.00
31) 4-Chloroaniline-d4	11.014	131	52862	31.804	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	153431	32.581	ng/ul	0.00
49) Acenaphthylene-d8	14.392	160	161687	31.575	ng/ul	0.00
54) 4-Nitrophenol-d4	14.880	143	19479	30.209	ng/ul	0.00
60) Fluorene-d10	15.691	176	134445	31.784	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.803	200	22879	26.006	ng/ul	0.00
73) Anthracene-d10	17.542	188	243170	33.387	ng/ul	0.00
81) Pyrene-d10	19.827	212	314747	33.368	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.757	264	316710	34.352	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.775	70	947	1.021	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053971.D
Acq On : 21 Jun 2022 10:17
Operator : CG/JU
Sample : PB145611BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :


Quant Time: Jun 21 23:06:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

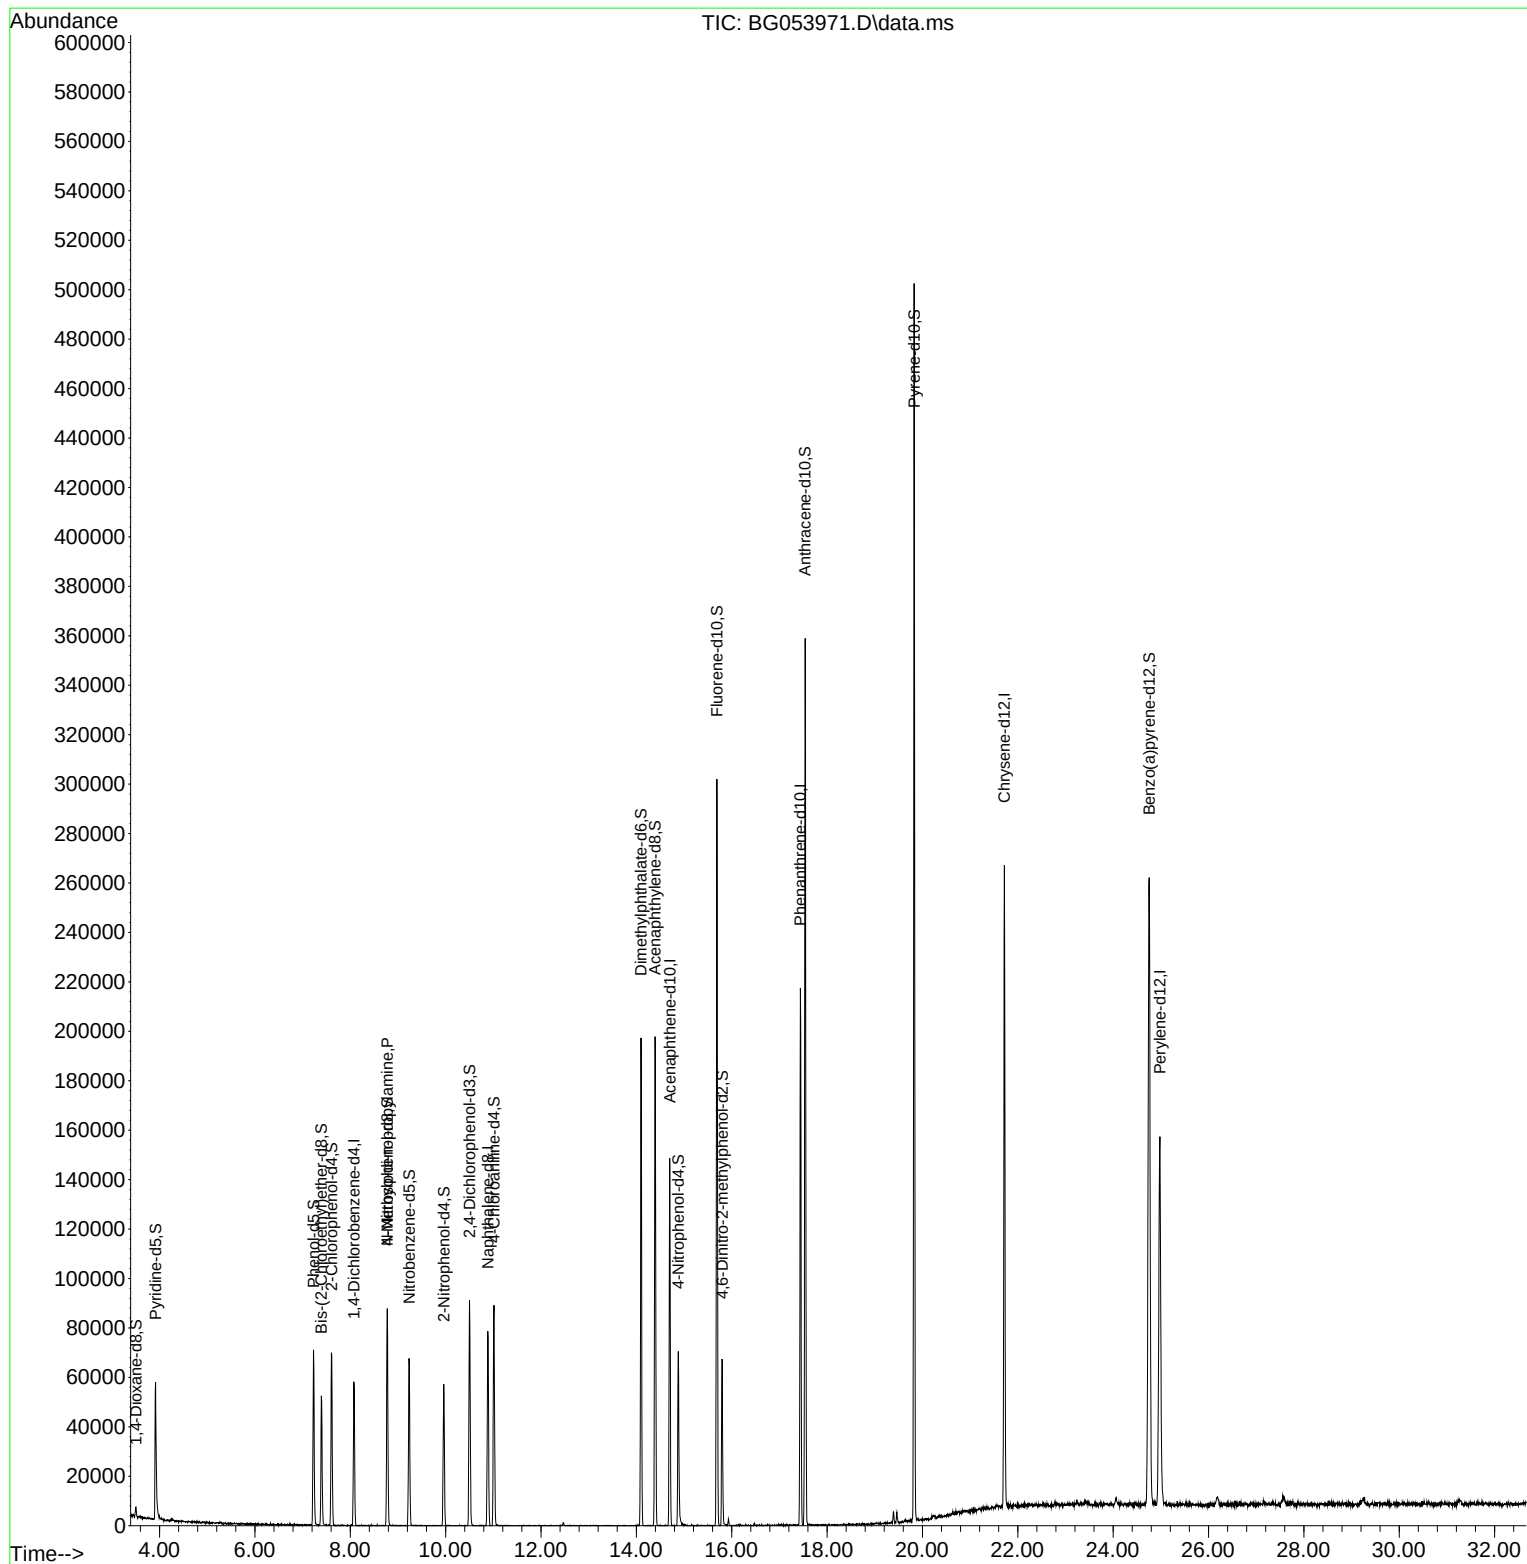

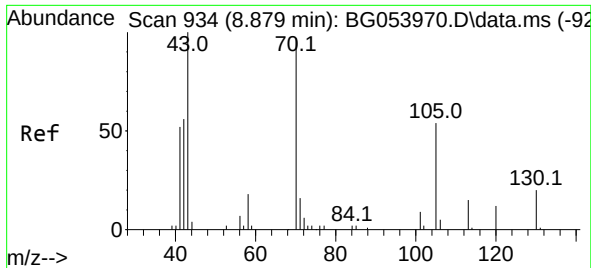

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.021 ng/ul
 RT: 8.775 min Scan# 917
 Delta R.T. -0.106 min
 Lab File: BG053971.D
 Acq: 21 Jun 2022 10:17

Instrument :
 BNA_G
 ClientSampleId :

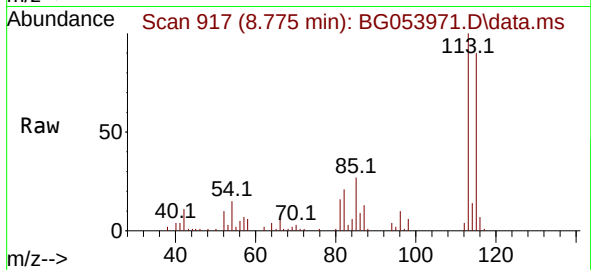

Tgt Ion: 70 Resp: 947

Ion	Ratio	Lower	Upper
70	100		
42	345.7	50.2	75.4#
101	0.0	7.1	10.7#
130	0.0	15.5	23.3#

