




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053976.D
Acq On : 21 Jun 2022 13:30
Operator : CG/JU
Sample : N3285-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R2

Manual IntegrationsAPPROVED

Quant Time: Jun 21 23:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022

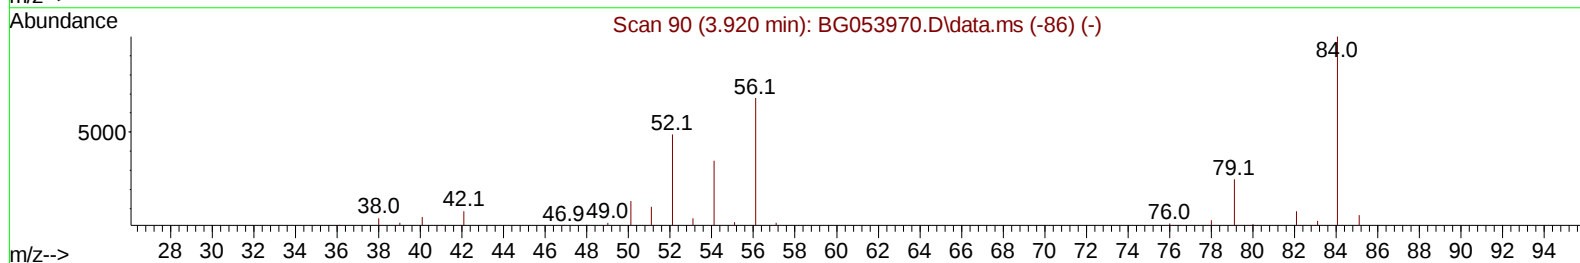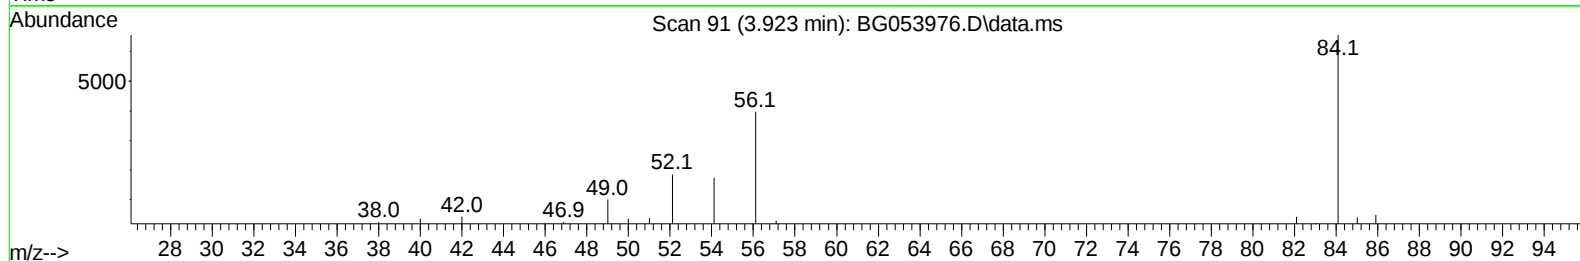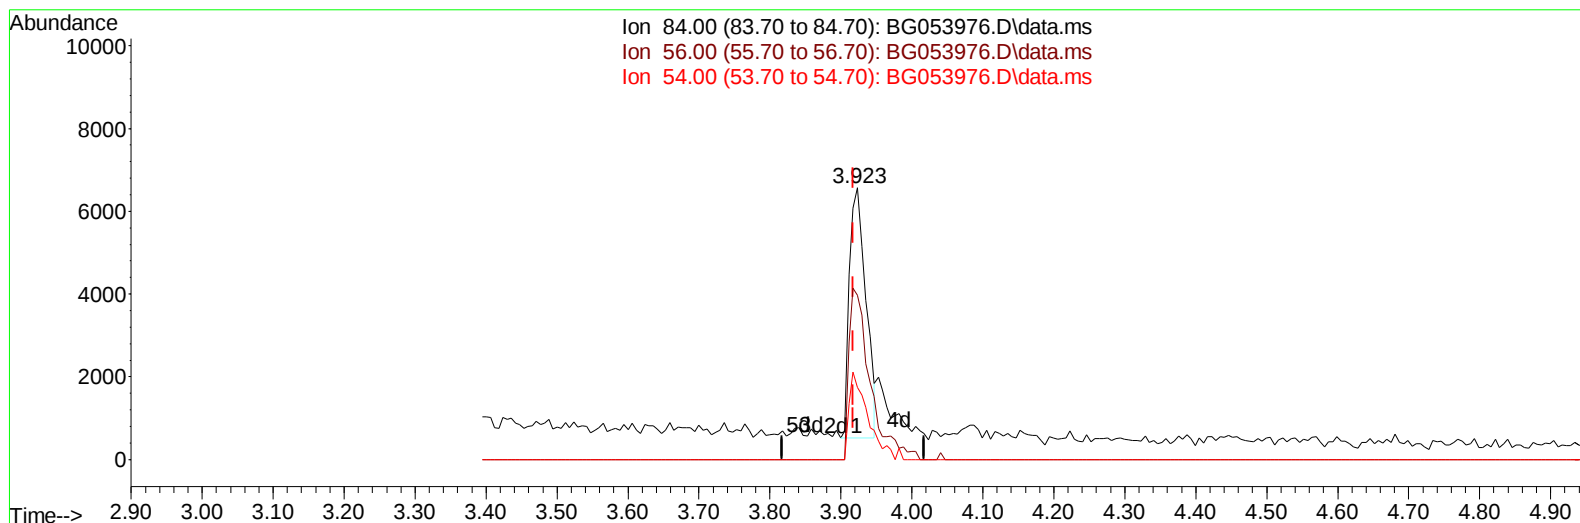

TIC: BG053976.D\data.ms

(4) Pyridine-d5 (S)

3.923min (+ 0.006) 8.29 ng/u1

response 9665

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	71.00	60.47
54.00	35.20	26.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053976.D
 Acq On : 21 Jun 2022 13:30
 Operator : CG/JU
 Sample : N3285-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4R2

Manual IntegrationsAPPROVED

Quant Time: Jun 21 23:07:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

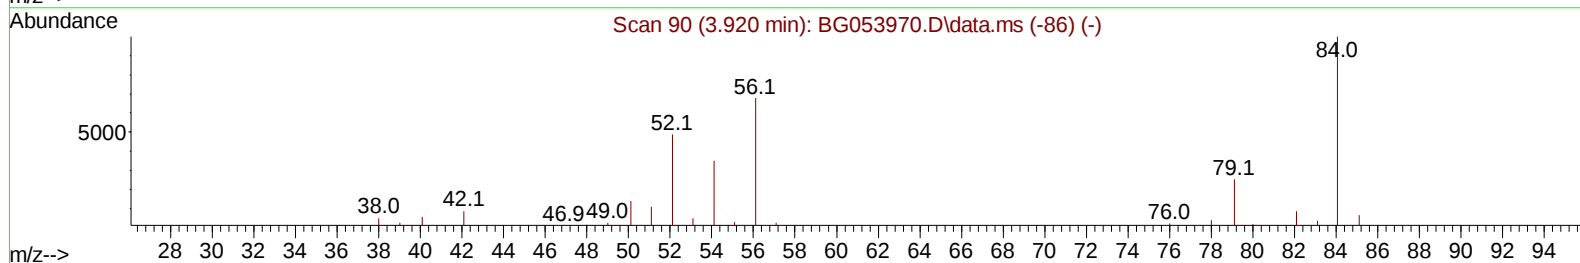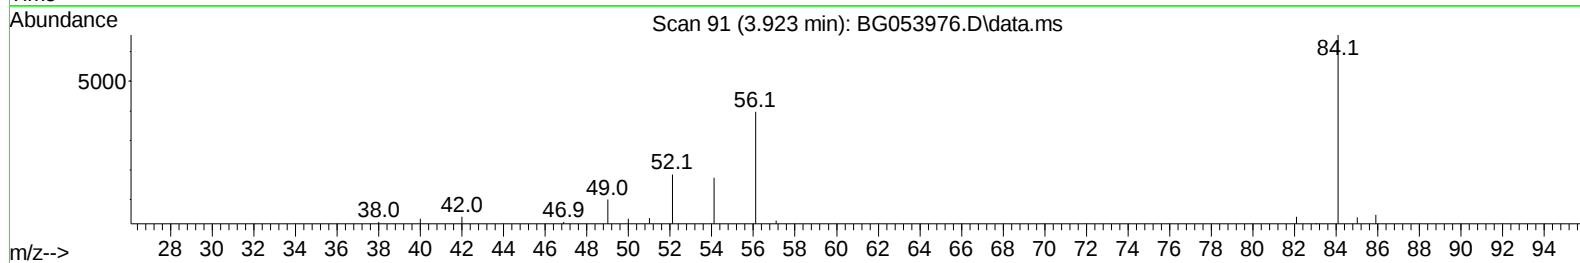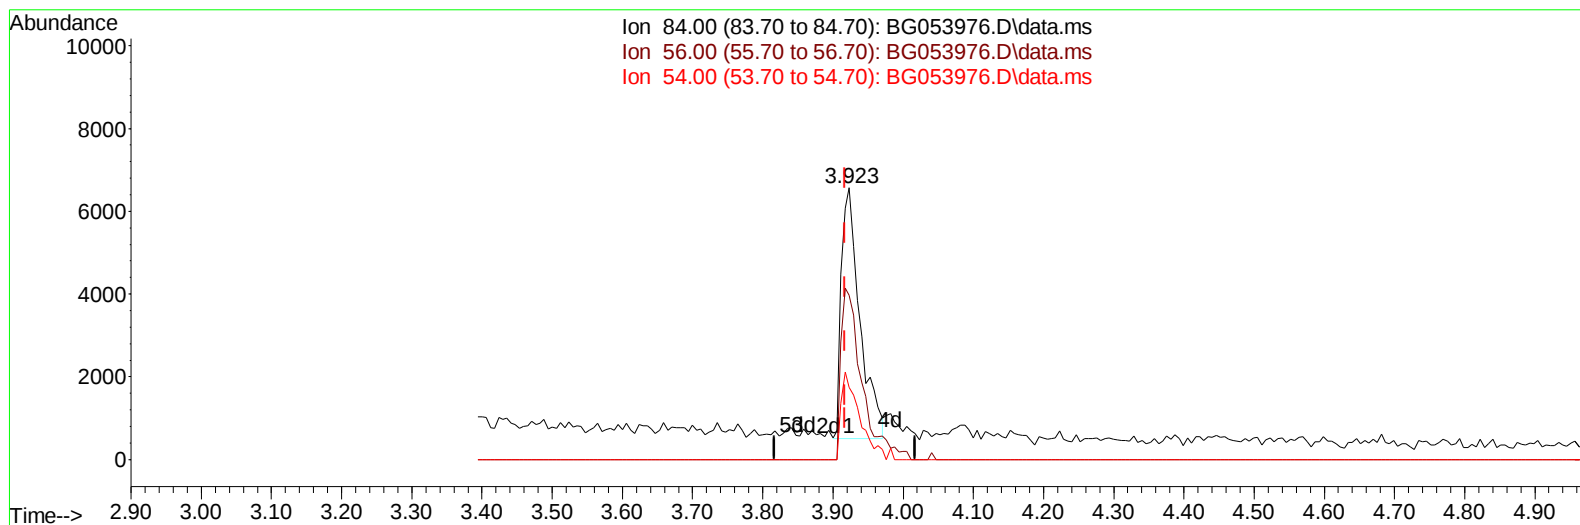

TIC: BG053976.D\data.ms

(4) Pyridine-d5 (S)

3.923min (+ 0.006) 9.50 ng/u1 m

response 11083

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	71.00	60.47
54.00	35.20	26.57#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053976.D
 Acq On : 21 Jun 2022 13:30
 Operator : CG/JU
 Sample : N3285-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4R2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 21 23:07:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.083	152	20406	20.000	ng/ul	0.00
20) Naphthalene-d8	10.886	136	80345	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.699	164	62043	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.443	188	167868	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.720	240	187504	20.000	ng/ul	# 0.00
88) Perylene-d12	24.981	264	189928	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.506	96	2109	4.917	ng/uL	0.00
4) Pyridine-d5	3.923	84	11083m	9.501	ng/ul	0.00
7) Phenol-d5	7.231	99	11366	7.775	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.396	67	28364	32.164	ng/ul	0.00
11) 2-Chlorophenol-d4	7.607	132	30013	25.745	ng/ul	0.00
15) 4-Methylphenol-d8	8.776	113	20352	16.327	ng/ul	0.00
21) Nitrobenzene-d5	9.235	128	18844	31.598	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	20893	32.973	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.504	165	40769	29.081	ng/ul	0.00
31) 4-Chloroaniline-d4	11.009	131	35695	20.154	ng/ul	0.00
46) Dimethylphthalate-d6	14.100	166	171146	35.065	ng/ul	0.00
49) Acenaphthylene-d8	14.393	160	176725	33.298	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	4889	7.315	ng/ul	0.00
60) Fluorene-d10	15.692	176	153810	35.083	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	28571	31.200	ng/ul	0.00
73) Anthracene-d10	17.543	188	280321	36.976	ng/ul	0.00
81) Pyrene-d10	19.828	212	370847	37.933	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.752	264	363834	37.950	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053976.D
Acq On : 21 Jun 2022 13:30
Operator : CG/JU
Sample : N3285-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R2

Manual IntegrationsAPPROVED

Quant Time: Jun 21 23:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022

