




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053983.D
 Acq On : 21 Jun 2022 18:02
 Operator : CG/JU
 Sample : N3355-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 22 03:32:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

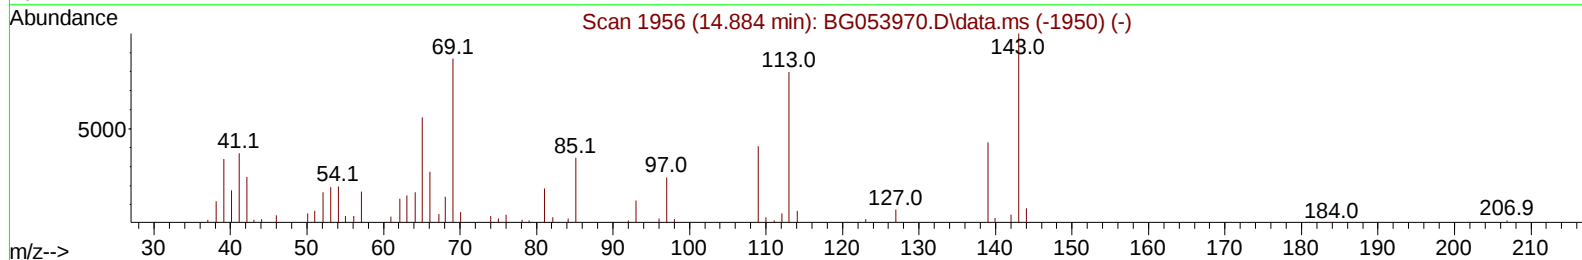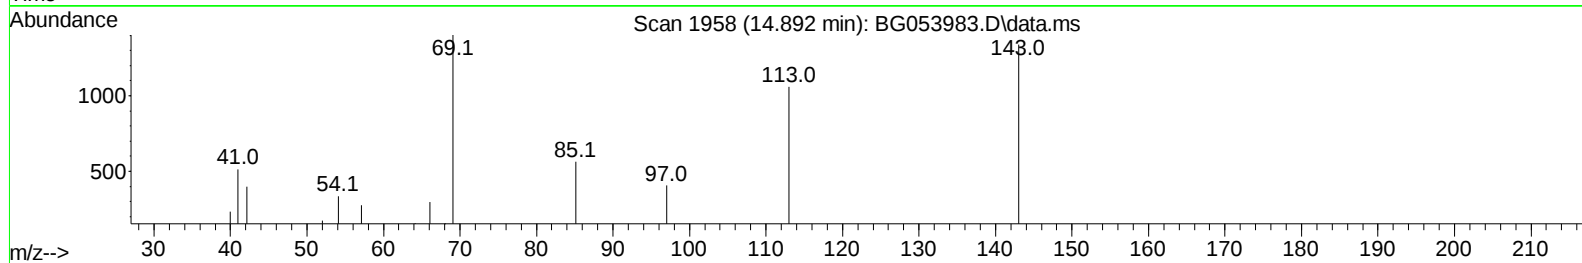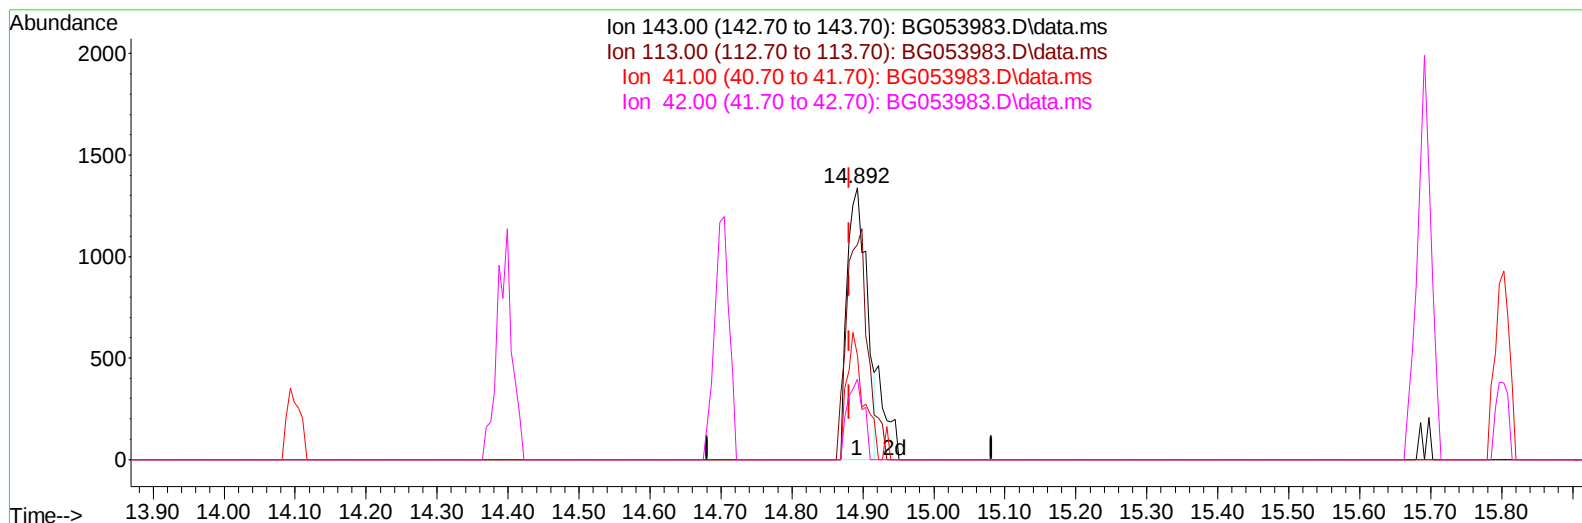

TIC: BG053983.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.892min (+ 0.011) 3.59 ng/u1

response 2575

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.90	79.15
41.00	51.40	38.42#
42.00	37.10	29.60#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053983.D
 Acq On : 21 Jun 2022 18:02
 Operator : CG/JU
 Sample : N3355-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EY0D3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 03:32:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.083	152	20907	20.000	ng/ul	0.00
20) Naphthalene-d8	10.885	136	84888	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.704	164	66634	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.442	188	182806	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.719	240	206738	20.000	ng/ul	# 0.00
88) Perylene-d12	24.980	264	208557	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.500	96	2019	4.595	ng/uL	0.00
4) Pyridine-d5	3.923	84	9291	7.774	ng/ul	0.00
7) Phenol-d5	7.231	99	7387	4.932	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.395	67	24426	27.035	ng/ul	0.00
11) 2-Chlorophenol-d4	7.612	132	24912	20.857	ng/ul	0.00
15) 4-Methylphenol-d8	8.776	113	15425	12.078	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	17713	28.112	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	19045	28.448	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.503	165	36722	24.792	ng/ul	0.00
31) 4-Chloroaniline-d4	11.014	131	42446	22.684	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	161423	30.794	ng/ul	0.00
49) Acenaphthylene-d8	14.399	160	163826	28.741	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	2961m	4.125	ng/ul	0.01
60) Fluorene-d10	15.691	176	145206	30.838	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.803	200	27687	27.764	ng/ul	0.00
73) Anthracene-d10	17.542	188	273094	33.079	ng/ul	0.00
81) Pyrene-d10	19.828	212	351677	32.626	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.751	264	350070	33.253	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053983.D
Acq On : 21 Jun 2022 18:02
Operator : CG/JU
Sample : N3355-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EY0D3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 03:32:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

