




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053989.D
Acq On : 21 Jun 2022 22:36
Operator : CG/JU
Sample : PB145688BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK688

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 00:01:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

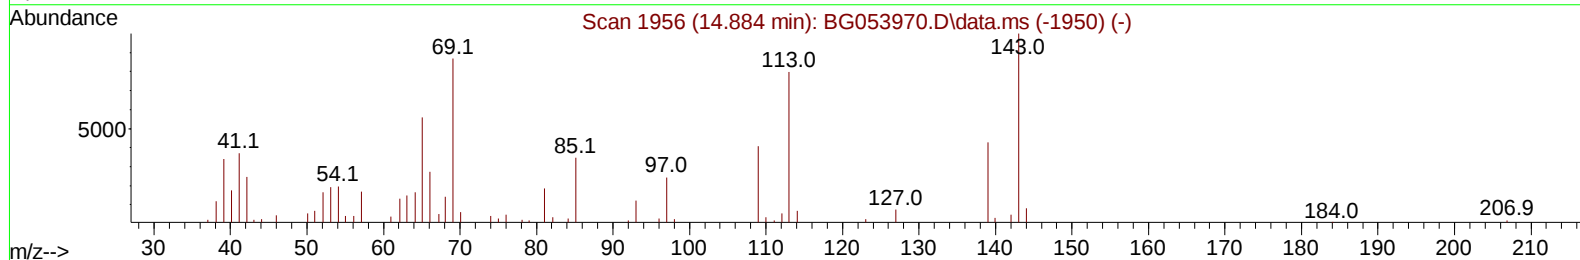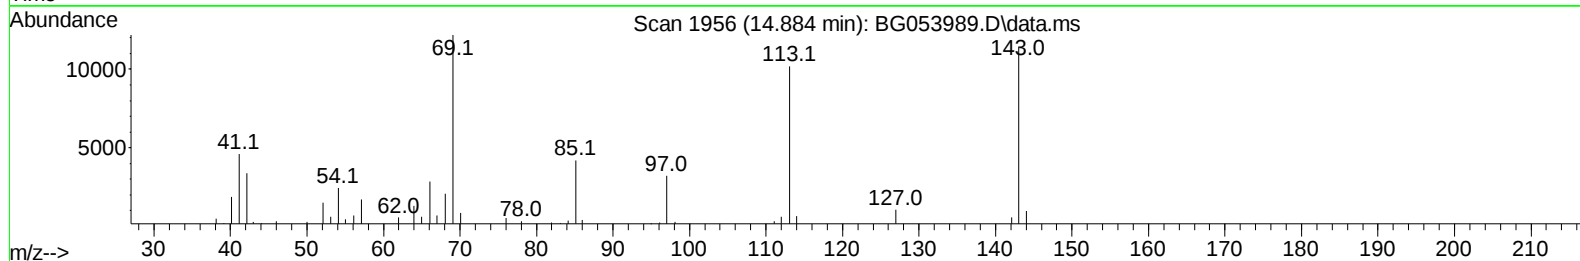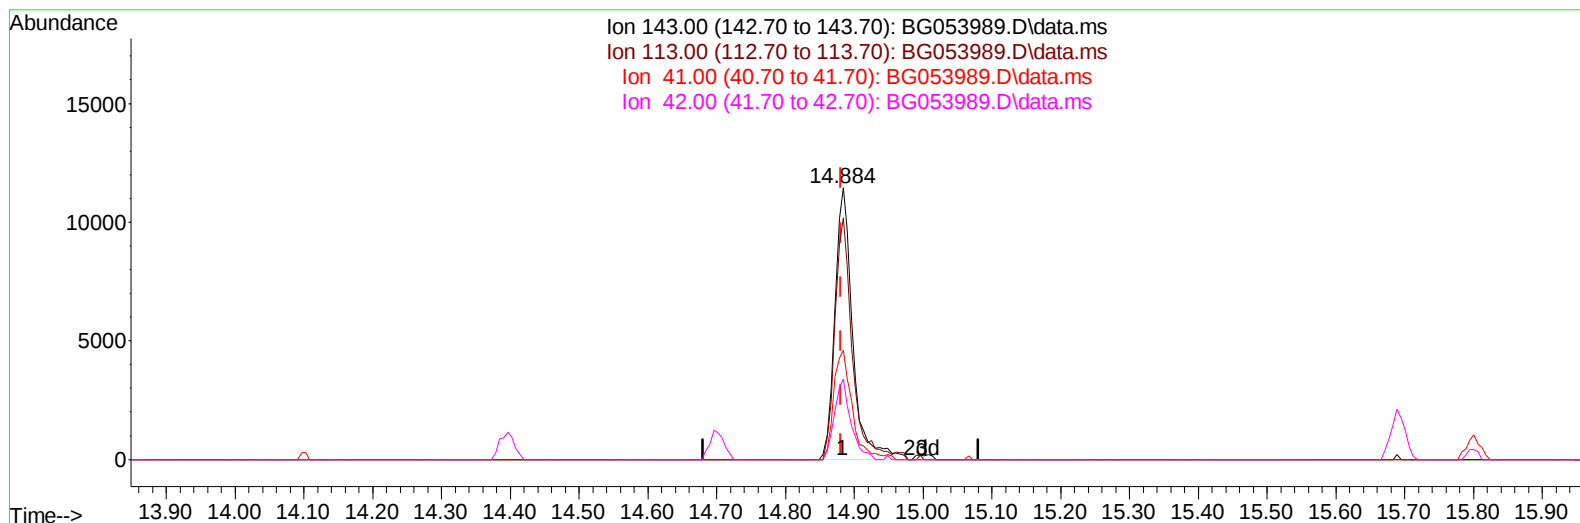

TIC: BG053989.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.884min (+ 0.003) 28.24 ng/u1****response 20380**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.90	88.96
41.00	51.40	40.24#
42.00	37.10	29.61#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053989.D
 Acq On : 21 Jun 2022 22:36
 Operator : CG/JU
 Sample : PB145688BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK688

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:01:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

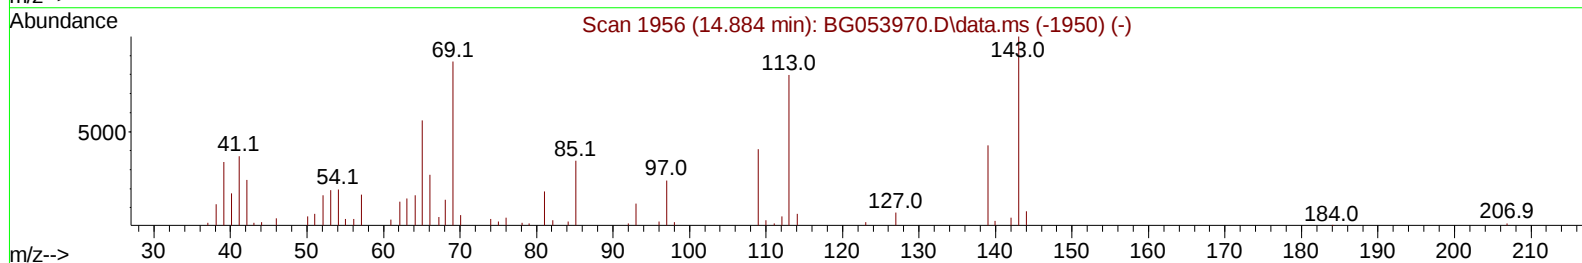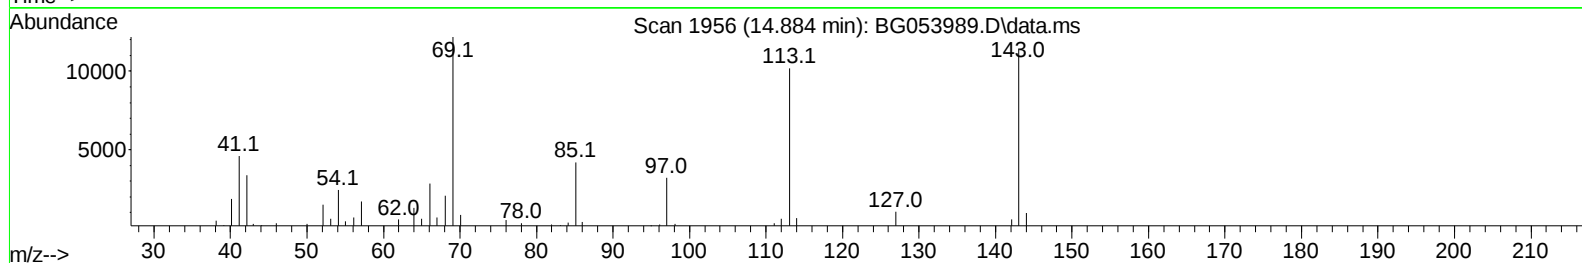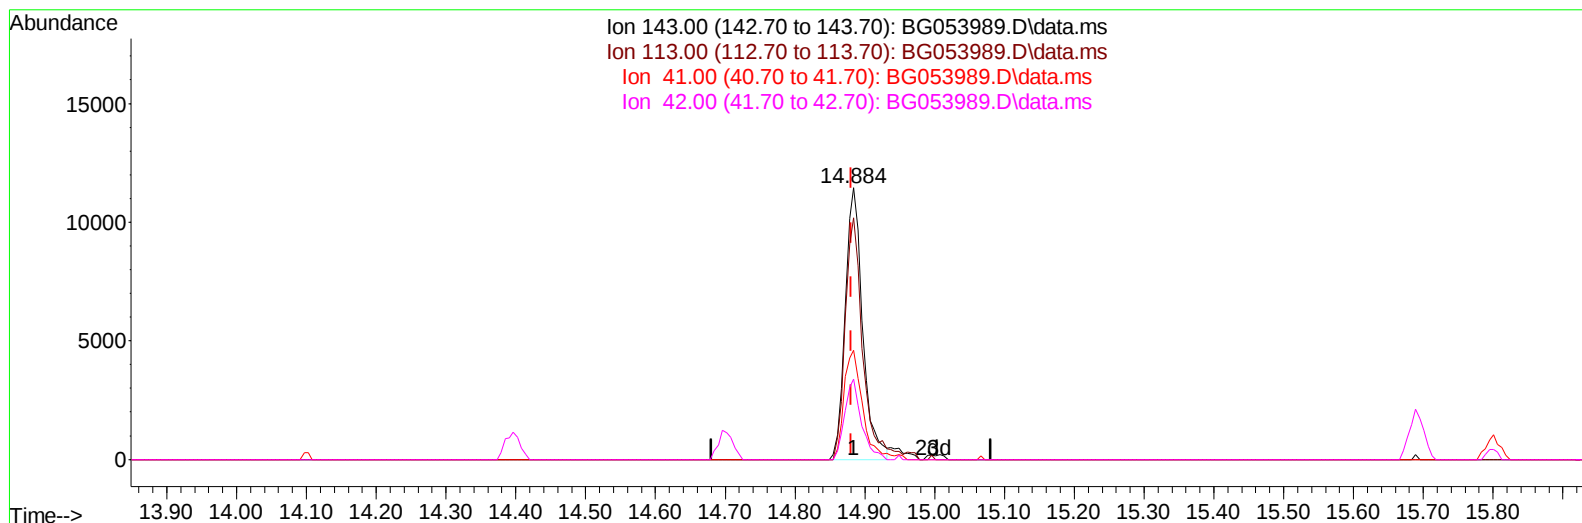

TIC: BG053989.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.884min (+ 0.003) 27.29 ng/ul m

response 19692

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.90	88.96
41.00	51.40	40.24#
42.00	37.10	29.61#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053989.D
 Acq On : 21 Jun 2022 22:36
 Operator : CG/JU
 Sample : PB145688BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK688

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 00:01:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.080	152	21887	20.000	ng/ul	0.00
20) Naphthalene-d8	10.883	136	87448	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.702	164	66994	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.446	188	181290	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.717	240	213156	20.000	ng/ul	# 0.00
88) Perylene-d12	24.978	264	212931	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.503	96	2718	5.909	ng/uL	0.00
4) Pyridine-d5	3.915	84	39142	31.284	ng/ul	0.00
7) Phenol-d5	7.228	99	49335	31.463	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	29558	31.250	ng/ul	0.00
11) 2-Chlorophenol-d4	7.610	132	40508	32.396	ng/ul	0.00
15) 4-Methylphenol-d8	8.779	113	40990	30.659	ng/ul	0.00
21) Nitrobenzene-d5	9.238	128	20666	31.839	ng/ul	0.00
24) 2-Nitrophenol-d4	9.966	143	23028	33.390	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.501	165	45248	29.654	ng/ul	0.00
31) 4-Chloroaniline-d4	11.012	131	57914	30.044	ng/ul	0.00
46) Dimethylphthalate-d6	14.103	166	165300	31.364	ng/ul	0.00
49) Acenaphthylene-d8	14.396	160	176488	30.796	ng/ul	0.00
54) 4-Nitrophenol-d4	14.884	143	19692m	27.288	ng/ul	0.00
60) Fluorene-d10	15.689	176	146841	31.018	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.801	200	25829	26.117	ng/ul	0.00
73) Anthracene-d10	17.540	188	263615	32.198	ng/ul	0.00
81) Pyrene-d10	19.825	212	345666	31.102	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.755	264	350811	32.639	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053989.D
Acq On : 21 Jun 2022 22:36
Operator : CG/JU
Sample : PB145688BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK688

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:01:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022

