

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053971.D
 Acq On : 21 Jun 2022 10:17
 Operator : CG/JU
 Sample : PB145611BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	15	20	26	rVB4	4457	7895	1.07%	0.126%
2	3.558	26	29	31	rBV2	772	1027	0.14%	0.016%
3	3.916	86	90	103	rBV	55005	95416	12.90%	1.517%
4	4.075	115	117	119	rVB2	960	760	0.10%	0.012%
5	4.416	173	175	178	rBV2	661	826	0.11%	0.013%
6	4.604	205	207	210	rBV	695	873	0.12%	0.014%
7	4.727	224	228	231	rVB2	713	816	0.11%	0.013%
8	5.127	293	296	302	rBV	538	984	0.13%	0.016%
9	6.983	607	612	614	rVB2	508	815	0.11%	0.013%
10	7.230	647	654	666	rVB2	70793	125553	16.97%	1.996%
11	7.395	675	682	695	rBV	52400	92205	12.46%	1.466%
12	7.606	711	718	727	rBV	69783	125049	16.90%	1.988%
13	8.076	790	798	806	rBB	58301	103595	14.00%	1.647%
14	8.775	911	917	926	rBV	87847	158061	21.37%	2.513%
15	9.234	987	995	1004	rBV	67733	125634	16.98%	1.997%
16	9.962	1112	1119	1126	rBV2	57218	104169	14.08%	1.656%
17	10.503	1204	1211	1222	rBB	91213	168873	22.83%	2.685%
18	10.885	1269	1276	1284	rBB	78724	148614	20.09%	2.363%
19	11.014	1291	1298	1310	rBV	89033	166754	22.54%	2.651%
20	12.471	1540	1546	1550	rBB2	1234	2051	0.28%	0.033%
21	14.099	1817	1823	1833	rBB	197316	298162	40.31%	4.740%
22	14.392	1866	1873	1883	rBB	197824	329708	44.57%	5.242%
23	14.698	1919	1925	1932	rBB	148677	241598	32.66%	3.841%
24	14.880	1950	1956	1970	rBV	70498	122079	16.50%	1.941%
25	15.691	2086	2094	2102	rBB	302025	463336	62.63%	7.366%
26	15.797	2107	2112	2120	rBV	67229	106617	14.41%	1.695%
27	15.932	2131	2135	2140	rVB	2694	3450	0.47%	0.055%
28	16.478	2225	2228	2230	rBB	1041	976	0.13%	0.016%
29	17.442	2386	2392	2402	rVB	217152	342845	46.35%	5.451%
30	17.542	2402	2409	2418	rBV	358587	562717	76.07%	8.946%
31	17.824	2453	2457	2460	rBV2	507	910	0.12%	0.014%
32	18.911	2639	2642	2645	rVB	739	798	0.11%	0.013%
33	18.958	2647	2650	2652	rBV	601	829	0.11%	0.013%
34	19.392	2720	2724	2728	rBV3	4836	7247	0.98%	0.115%
35	19.463	2732	2736	2740	rBV2	4439	6568	0.89%	0.104%
36	19.516	2744	2745	2748	rBV	608	765	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053971.D
 Acq On : 21 Jun 2022 10:17
 Operator : CG/JU
 Sample : PB145611BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.622	2760	2763	2765	rBV3	923	1092	0.15%	0.017%
38	19.827	2789	2798	2806	rBV	501452	722630	97.68%	11.488%
39	19.880	2806	2807	2811	rVV2	755	962	0.13%	0.015%
40	20.156	2850	2854	2856	rBV	760	1132	0.15%	0.018%
41	20.215	2861	2864	2865	rBV2	1152	1132	0.15%	0.018%
42	20.309	2877	2880	2882	rBV2	794	1071	0.14%	0.017%
43	20.744	2951	2954	2955	rBV2	868	933	0.13%	0.015%
44	20.791	2960	2962	2963	rBV2	1026	853	0.12%	0.014%
45	20.838	2968	2970	2972	rBV3	1293	972	0.13%	0.015%
46	20.985	2994	2995	2999	rBV3	1470	1558	0.21%	0.025%
47	21.073	3009	3010	3012	rVB	2263	857	0.12%	0.014%
48	21.243	3037	3039	3040	rBV2	1309	918	0.12%	0.015%
49	21.290	3045	3047	3048	rBV2	1464	937	0.13%	0.015%
50	21.719	3113	3120	3130	rVV	259419	426682	57.68%	6.783%
51	21.784	3130	3131	3136	rVB5	1877	1848	0.25%	0.029%
52	22.001	3167	3168	3170	rBV3	1561	898	0.12%	0.014%
53	22.236	3206	3208	3210	rBV2	1233	1053	0.14%	0.017%
54	22.612	3270	3272	3274	rBV2	1399	960	0.13%	0.015%
55	23.400	3404	3406	3408	rBV2	1674	1142	0.15%	0.018%
56	24.445	3582	3584	3585	rBV2	1321	840	0.11%	0.013%
57	24.569	3603	3605	3608	rVB4	1425	1130	0.15%	0.018%
58	24.757	3625	3637	3652	rVB2	253637	739764	100.00%	11.761%
59	24.980	3664	3675	3689	rVB2	148703	426701	57.68%	6.784%
60	25.192	3710	3711	3713	rBV2	1419	999	0.14%	0.016%
61	25.403	3745	3747	3749	rBV3	1347	805	0.11%	0.013%
62	25.526	3766	3768	3770	rVB3	1614	1142	0.15%	0.018%
63	25.991	3845	3847	3848	rBV2	1318	1003	0.14%	0.016%
64	26.020	3850	3852	3853	rBV2	1443	1254	0.17%	0.020%
65	26.267	3892	3894	3896	rVB3	1769	1411	0.19%	0.022%
66	26.608	3950	3952	3953	rBV2	1440	954	0.13%	0.015%
67	26.655	3958	3960	3963	rVV2	2023	1418	0.19%	0.023%
68	26.684	3963	3965	3967	rVB3	1511	1036	0.14%	0.016%
69	26.884	3997	3999	4003	rBV5	1727	2488	0.34%	0.040%
70	26.989	4015	4017	4018	rBV2	1379	764	0.10%	0.012%
71	27.524	4105	4108	4110	rBV2	2436	3698	0.50%	0.059%
72	27.559	4112	4114	4116	rVV2	2536	2294	0.31%	0.036%
73	27.859	4163	4165	4166	rBV	1248	877	0.12%	0.014%
74	27.877	4166	4168	4170	rVV3	1581	1242	0.17%	0.020%
75	29.022	4361	4363	4364	rBV2	1557	1126	0.15%	0.018%
76	29.481	4439	4441	4444	rBV3	1579	1395	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053971.D
Acq On : 21 Jun 2022 10:17
Operator : CG/JU
Sample : PB145611BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK611

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	29.604	4460	4462	4463	rBV2	1431	1111	0.15%	0.018%
78	29.663	4470	4472	4474	rBV3	1200	1055	0.14%	0.017%
79	30.462	4606	4608	4609	rBV2	1508	1211	0.16%	0.019%
80	30.491	4611	4613	4616	rBV3	1774	2181	0.29%	0.035%
81	30.756	4656	4658	4659	rBV2	1514	1210	0.16%	0.019%
82	31.055	4707	4709	4710	rBV2	1732	1337	0.18%	0.021%
83	31.754	4826	4828	4830	rBV2	1353	859	0.12%	0.014%
84	32.277	4915	4917	4919	rBV3	1556	1545	0.21%	0.025%
85	32.612	4972	4974	4976	rBV3	1287	1024	0.14%	0.016%


Sum of corrected areas: 6290079

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053971.D
Acq On : 21 Jun 2022 10:17
Operator : CG/JU
Sample : PB145611BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK611

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

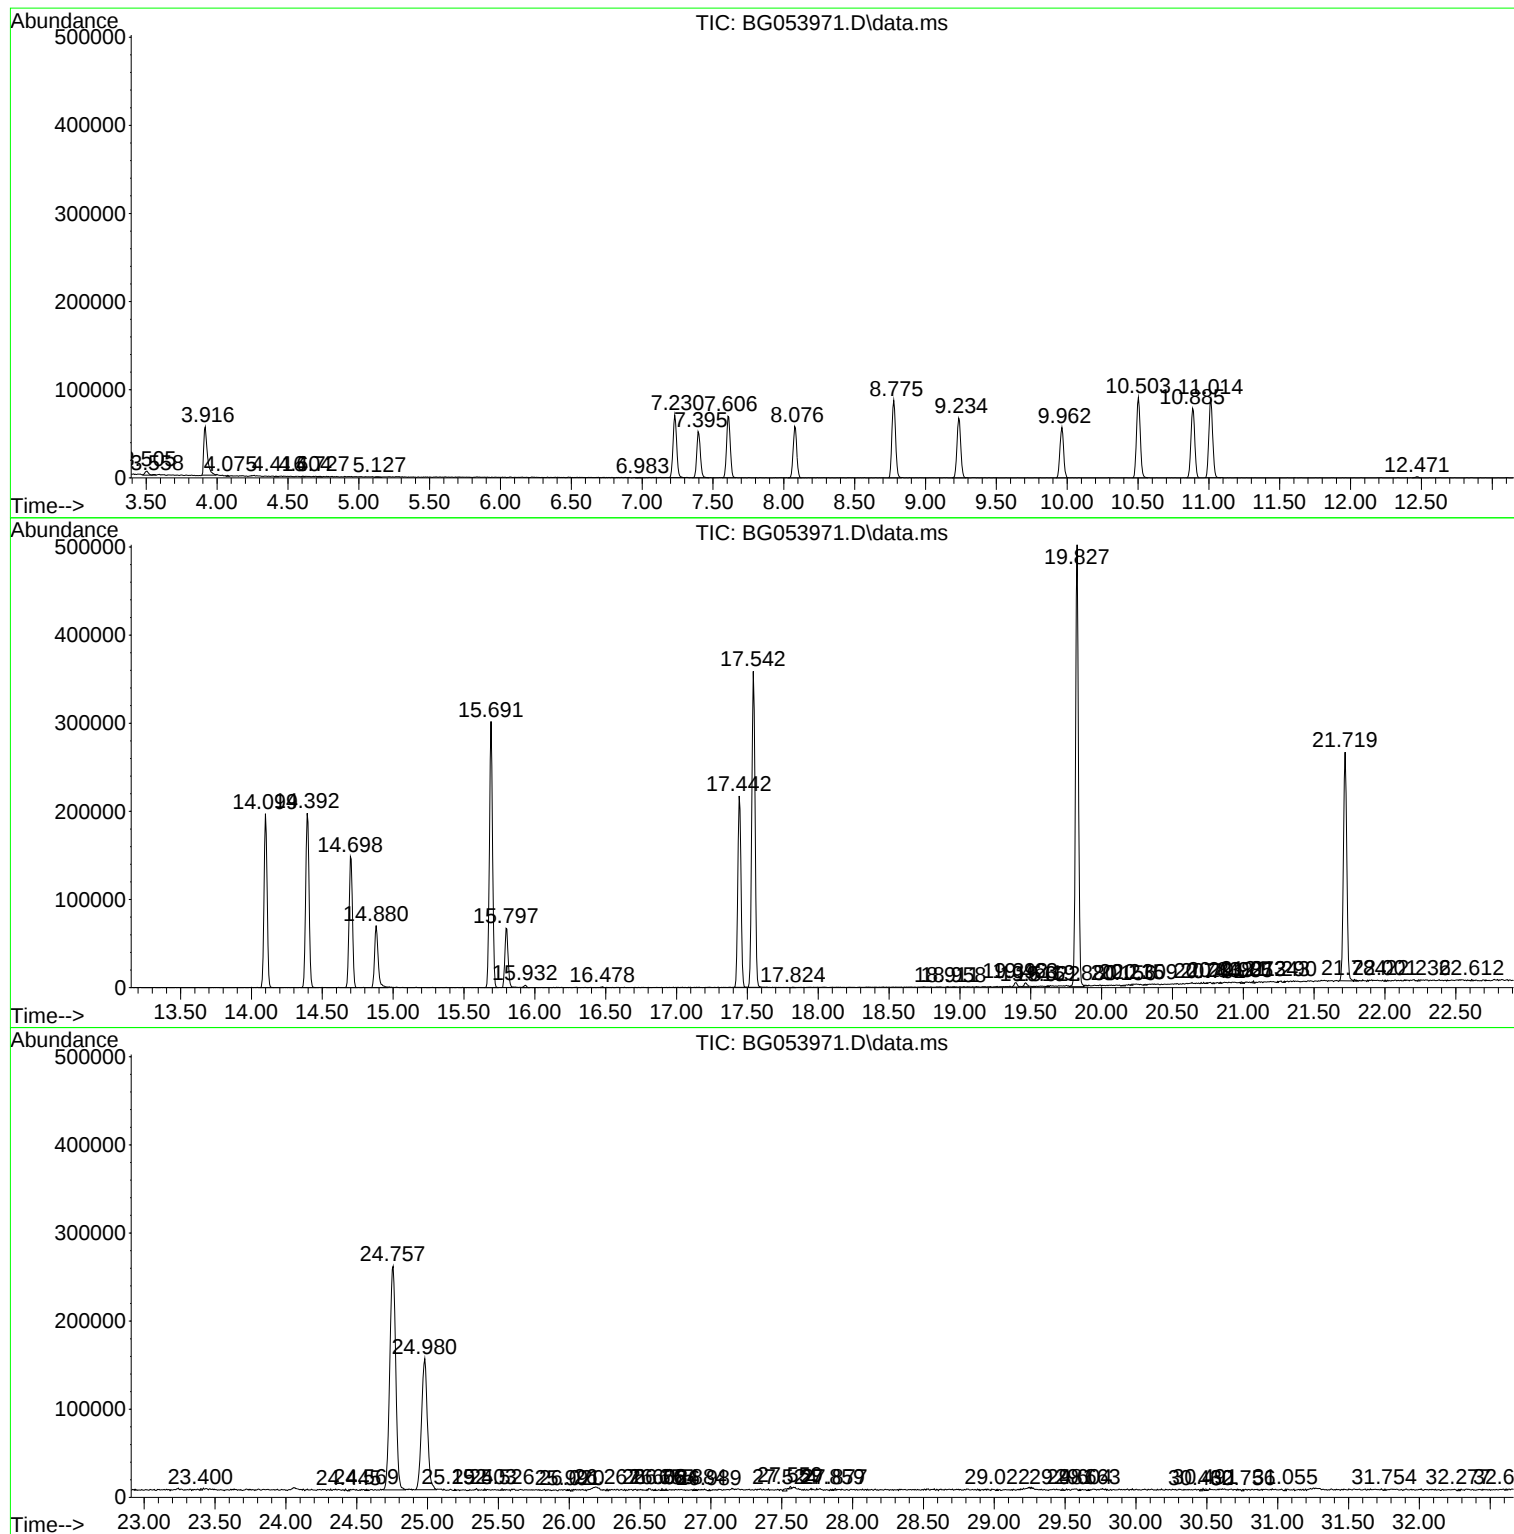

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053971.D
Acq On : 21 Jun 2022 10:17
Operator : CG/JU
Sample : PB145611BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK611

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053971.D
Acq On : 21 Jun 2022 10:17
Operator : CG/JU
Sample : PB145611BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK611

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------