

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053973.D
 Acq On : 21 Jun 2022 11:34
 Operator : CG/JU
 Sample : PB145591BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK591

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.499	16	19	29	rVB3	4319	7733	1.02%	0.122%
2	3.916	86	90	103	rBV	55821	101415	13.38%	1.594%
3	4.257	144	148	150	rBV3	980	1089	0.14%	0.017%
4	7.230	644	654	663	rBV	69778	125297	16.53%	1.970%
5	7.400	677	683	690	rBV	51501	91725	12.10%	1.442%
6	7.612	712	719	728	rVB	68218	125704	16.58%	1.976%
7	8.076	792	798	807	rBB	57062	101571	13.40%	1.597%
8	8.775	911	917	926	rBV	88533	160113	21.12%	2.517%
9	9.233	988	995	1006	rBB	67432	124434	16.41%	1.956%
10	9.962	1113	1119	1126	rBB2	57910	104290	13.76%	1.639%
11	10.502	1204	1211	1219	rBV	92803	166352	21.94%	2.615%
12	10.884	1269	1276	1285	rBB	79336	147418	19.44%	2.317%
13	11.014	1291	1298	1306	rBV	89445	164761	21.73%	2.590%
14	12.465	1542	1545	1550	rBB	1250	1800	0.24%	0.028%
15	14.098	1817	1823	1833	rBB	197234	292827	38.62%	4.603%
16	14.392	1866	1873	1881	rBV	195672	324591	42.81%	5.103%
17	14.703	1919	1926	1933	rBB	146995	238467	31.45%	3.749%
18	14.880	1950	1956	1972	rBV2	70275	121529	16.03%	1.910%
19	15.691	2087	2094	2103	rBB	310198	463713	61.16%	7.289%
20	15.796	2107	2112	2120	rBV	65212	106488	14.05%	1.674%
21	15.849	2120	2121	2125	rVB	1537	971	0.13%	0.015%
22	15.926	2131	2134	2139	rBV	2423	3120	0.41%	0.049%
23	16.472	2223	2227	2231	rBB3	764	1029	0.14%	0.016%
24	17.441	2386	2392	2400	rBV	214722	347854	45.88%	5.468%
25	17.541	2403	2409	2424	rVB	354069	562761	74.23%	8.847%
26	19.292	2704	2707	2710	rVB	912	1079	0.14%	0.017%
27	19.398	2718	2725	2730	rVV3	4876	8407	1.11%	0.132%
28	19.463	2732	2736	2742	rVB	4309	6564	0.87%	0.103%
29	19.680	2770	2773	2776	rBV2	933	1035	0.14%	0.016%
30	19.827	2791	2798	2809	rVB	489747	731683	96.51%	11.502%
31	19.974	2820	2823	2826	rBV2	987	1202	0.16%	0.019%
32	20.150	2850	2853	2855	rBV2	717	857	0.11%	0.013%
33	20.191	2859	2860	2861	rBV	1179	762	0.10%	0.012%
34	20.320	2880	2882	2886	rVB4	637	829	0.11%	0.013%
35	20.432	2900	2901	2903	rBV2	937	788	0.10%	0.012%
36	20.790	2961	2962	2964	rBV	1040	813	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053973.D
 Acq On : 21 Jun 2022 11:34
 Operator : CG/JU
 Sample : PB145591BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK591

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.843	2969	2971	2972	rBV2	1103	797	0.11%	0.013%
38	20.914	2981	2983	2986	rBV4	976	1408	0.19%	0.022%
39	21.055	3004	3007	3008	rBV2	1103	1110	0.15%	0.017%
40	21.454	3074	3075	3077	rBV2	2040	1064	0.14%	0.017%
41	21.578	3094	3096	3099	rVB3	2280	1653	0.22%	0.026%
42	21.719	3113	3120	3128	rBV2	266702	446377	58.88%	7.017%
43	21.830	3137	3139	3142	rBV3	1255	1351	0.18%	0.021%
44	22.248	3208	3210	3211	rBV2	1410	985	0.13%	0.015%
45	22.676	3282	3283	3285	rBV2	1618	1270	0.17%	0.020%
46	22.906	3321	3322	3324	rBV2	1455	1009	0.13%	0.016%
47	23.235	3376	3378	3385	rVB7	2889	4693	0.62%	0.074%
48	23.599	3438	3440	3441	rBV2	1573	1241	0.16%	0.020%
49	23.640	3445	3447	3448	rBV	1406	1048	0.14%	0.016%
50	23.781	3469	3471	3472	rBV2	1460	783	0.10%	0.012%
51	23.852	3481	3483	3486	rBV4	1519	2219	0.29%	0.035%
52	24.069	3514	3520	3525	rVB8	3117	7235	0.95%	0.114%
53	24.245	3548	3550	3553	rVB3	1708	1237	0.16%	0.019%
54	24.668	3620	3622	3623	rBV2	1296	931	0.12%	0.015%
55	24.756	3625	3637	3651	rVV2	260297	758174	100.00%	11.918%
56	24.980	3663	3675	3691	rBV2	148488	454132	59.90%	7.139%
57	25.649	3787	3789	3790	rBV2	1327	876	0.12%	0.014%
58	26.043	3854	3856	3859	rBV3	1621	1602	0.21%	0.025%
59	26.260	3892	3893	3895	rVB2	1688	886	0.12%	0.014%
60	26.284	3895	3897	3901	rBV4	1411	1474	0.19%	0.023%
61	26.960	4011	4012	4014	rBV2	1957	1428	0.19%	0.022%
62	26.983	4014	4016	4017	rVV	1390	838	0.11%	0.013%
63	27.347	4076	4078	4081	rBV4	1268	1223	0.16%	0.019%
64	27.500	4102	4104	4105	rBV	1615	1464	0.19%	0.023%
65	27.541	4109	4111	4112	rBV2	2077	1339	0.18%	0.021%
66	27.747	4144	4146	4149	rBV3	1684	2092	0.28%	0.033%
67	27.788	4151	4153	4155	rBV3	1269	955	0.13%	0.015%
68	27.917	4174	4175	4178	rBV3	1774	1351	0.18%	0.021%
69	28.752	4315	4317	4320	rBV4	1391	1398	0.18%	0.022%
70	29.445	4433	4435	4438	rBV4	1523	1711	0.23%	0.027%
71	29.486	4440	4442	4444	rVV3	1399	915	0.12%	0.014%
72	29.533	4448	4450	4453	rBV3	1365	1283	0.17%	0.020%
73	29.968	4522	4524	4526	rBV2	1736	1898	0.25%	0.030%
74	30.174	4557	4559	4560	rBV2	1325	834	0.11%	0.013%
75	30.720	4650	4652	4656	rBV4	1339	1768	0.23%	0.028%
76	30.837	4670	4672	4673	rBV2	1338	1073	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053973.D
Acq On : 21 Jun 2022 11:34
Operator : CG/JU
Sample : PB145591BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK591

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	31.037	4704	4706	4709	rVB3	1503	1190	0.16%	0.019%
78	31.102	4715	4717	4720	rBV2	1388	1322	0.17%	0.021%
79	31.155	4724	4726	4728	rBV3	1436	1269	0.17%	0.020%
80	31.930	4856	4858	4861	rVB4	1764	1420	0.19%	0.022%




Sum of corrected areas: 6361397

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053973.D
Acq On : 21 Jun 2022 11:34
Operator : CG/JU
Sample : PB145591BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK591

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

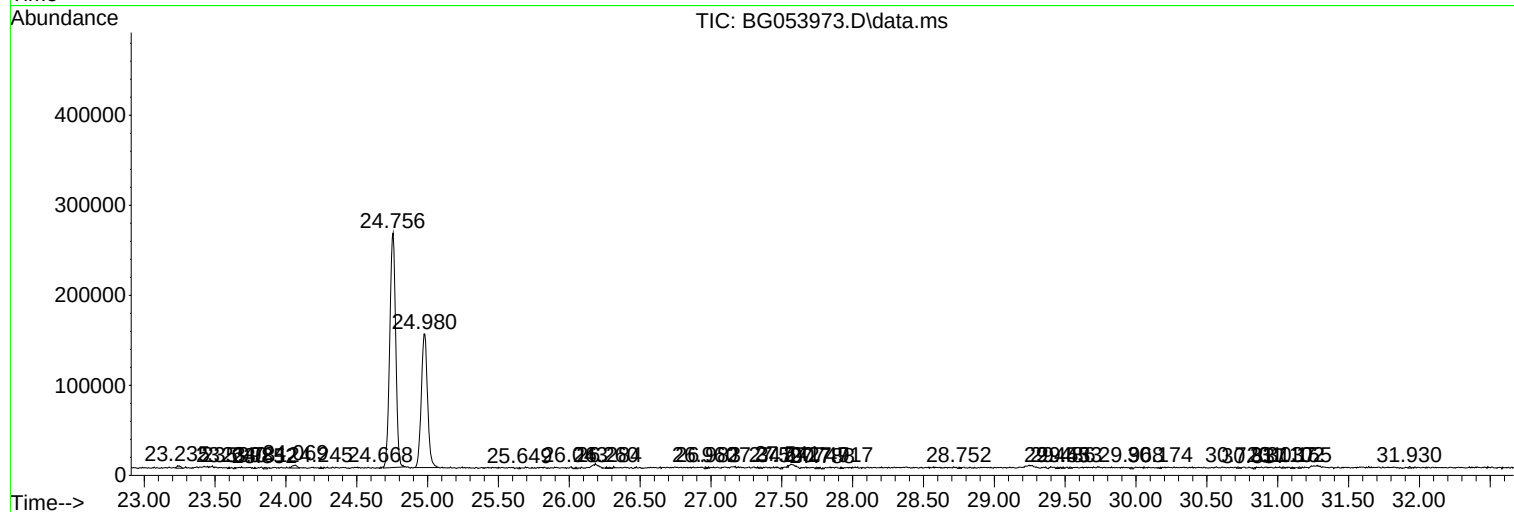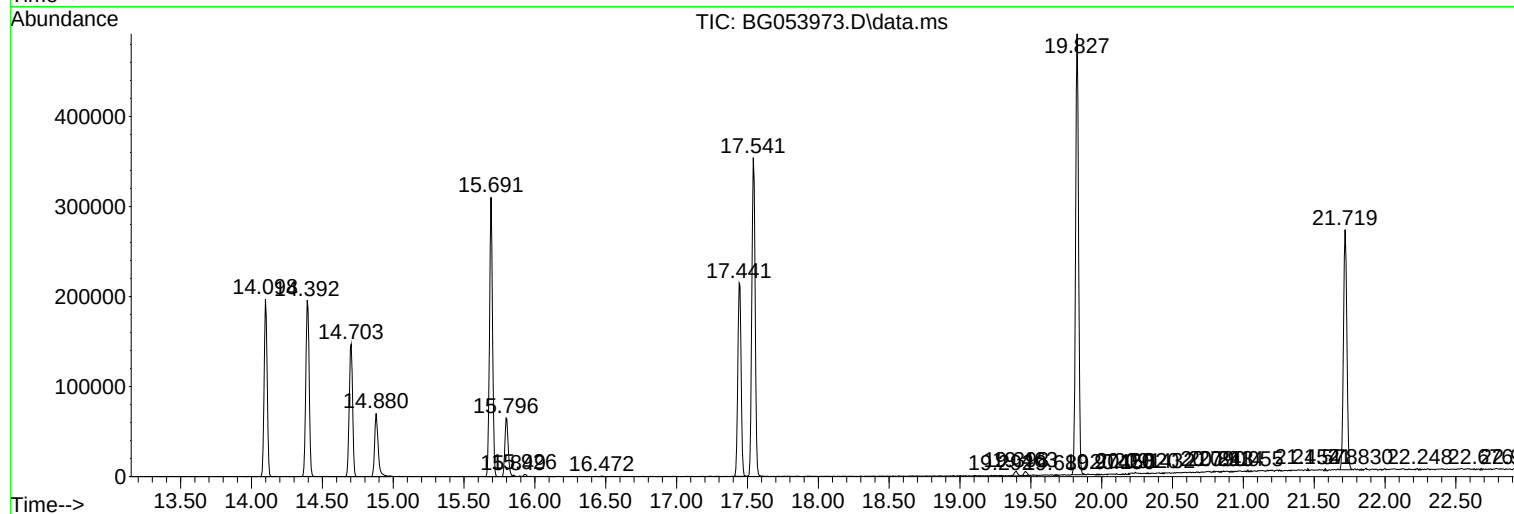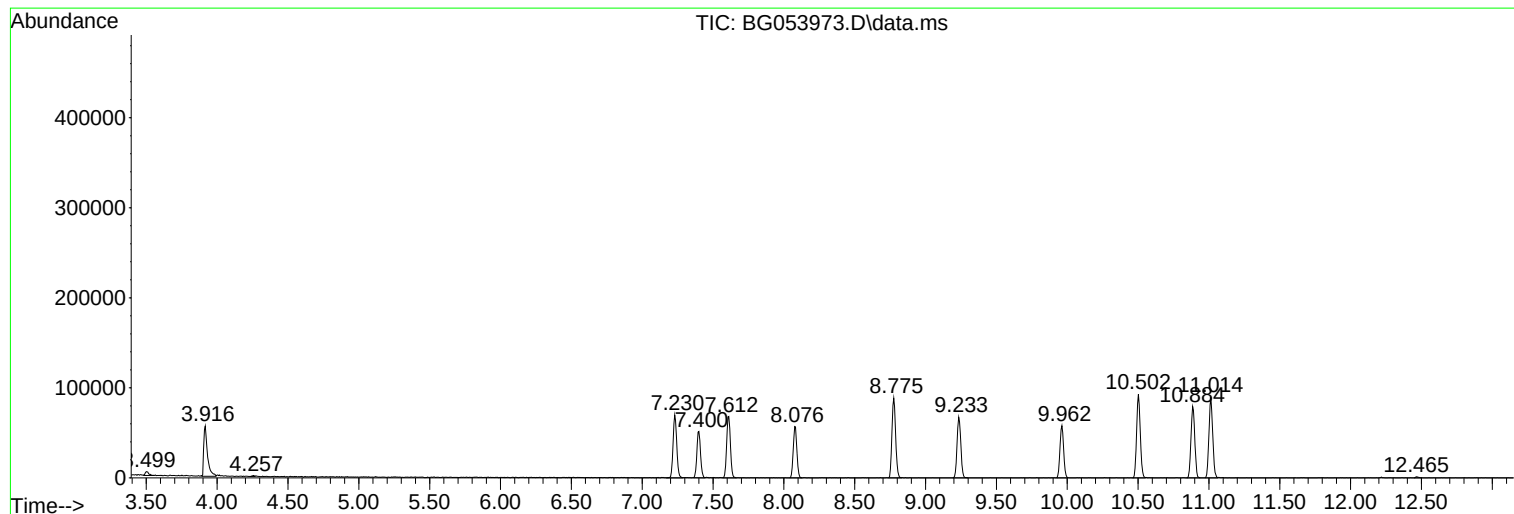

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053973.D
Acq On : 21 Jun 2022 11:34
Operator : CG/JU
Sample : PB145591BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK591

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053973.D
Acq On : 21 Jun 2022 11:34
Operator : CG/JU
Sample : PB145591BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK591

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc