

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053975.D
 Acq On : 21 Jun 2022 12:52
 Operator : CG/JU
 Sample : N3285-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4R3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.501	16	19	26	rVB3	4005	5681	0.62%	0.083%
2	3.771	63	65	70	rVB3	683	921	0.10%	0.013%
3	3.924	87	91	105	rBV	14109	26670	2.92%	0.390%
4	4.153	127	130	131	rBV2	1510	1381	0.15%	0.020%
5	4.258	145	148	151	rBV4	1395	1702	0.19%	0.025%
6	5.175	301	304	307	rVB3	1414	1908	0.21%	0.028%
7	7.231	648	654	662	rBB	19501	33323	3.65%	0.488%
8	7.396	675	682	692	rBV	63244	110944	12.14%	1.623%
9	7.607	710	718	728	rBB	66117	117140	12.82%	1.714%
10	8.078	790	798	807	rBB	60843	108360	11.86%	1.585%
11	8.777	911	917	926	rBB	53955	94718	10.37%	1.386%
12	9.235	988	995	1005	rBB	82160	151422	16.58%	2.215%
13	9.964	1112	1119	1126	rBV	65601	119196	13.05%	1.744%
14	10.504	1204	1211	1220	rBB	100862	186515	20.42%	2.729%
15	10.886	1268	1276	1285	rBB	84664	156330	17.11%	2.287%
16	11.015	1291	1298	1306	rBV	62730	118158	12.93%	1.729%
17	12.466	1540	1545	1549	rBB2	1515	2312	0.25%	0.034%
18	14.100	1816	1823	1830	rBV	237571	356160	38.99%	5.210%
19	14.394	1866	1873	1883	rVB	238680	391952	42.91%	5.734%
20	14.699	1919	1925	1932	rBB	154223	246272	26.96%	3.603%
21	14.887	1951	1957	1969	rBB2	13979	26570	2.91%	0.389%
22	15.034	1979	1982	1989	rBB3	2935	4495	0.49%	0.066%
23	15.692	2087	2094	2102	rBV	367798	567835	62.16%	8.307%
24	15.798	2106	2112	2122	rBV	95526	147007	16.09%	2.151%
25	15.933	2131	2135	2139	rVB	2890	4123	0.45%	0.060%
26	16.474	2222	2227	2232	rBB2	1275	1926	0.21%	0.028%
27	16.985	2309	2314	2318	rVB2	602	1084	0.12%	0.016%
28	17.443	2386	2392	2399	rVV	226749	347826	38.07%	5.089%
29	17.543	2401	2409	2419	rVV2	435453	680348	74.47%	9.953%
30	17.719	2436	2439	2444	rVB	1254	1349	0.15%	0.020%
31	18.401	2551	2555	2561	rVB2	866	1641	0.18%	0.024%
32	18.818	2621	2626	2632	rVB3	1415	2275	0.25%	0.033%
33	18.877	2632	2636	2639	rBV	767	1170	0.13%	0.017%
34	19.088	2664	2672	2674	rBV4	1030	1703	0.19%	0.025%
35	19.394	2720	2724	2730	rVB4	6667	10158	1.11%	0.149%
36	19.464	2730	2736	2740	rBV2	6099	9918	1.09%	0.145%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053975.D
 Acq On : 21 Jun 2022 12:52
 Operator : CG/JU
 Sample : N3285-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4R3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.828	2790	2798	2810	rBV	630951	909578	99.57%	13.307%
38	19.917	2812	2813	2816	rVV3	996	1149	0.13%	0.017%
39	20.110	2842	2846	2847	rBV3	1267	1111	0.12%	0.016%
40	20.187	2854	2859	2860	rBV3	1329	2217	0.24%	0.032%

41	20.222	2860	2865	2867	rBV3	1304	2397	0.26%	0.035%
42	20.304	2877	2879	2883	rVB2	750	954	0.10%	0.014%
43	20.434	2899	2901	2903	rVB3	1162	976	0.11%	0.014%
44	20.457	2903	2905	2907	rBV2	1045	1038	0.11%	0.015%
45	20.722	2948	2950	2954	rBV3	1407	1549	0.17%	0.023%

46	20.951	2987	2989	2992	rVB3	2378	1537	0.17%	0.022%
47	21.338	3052	3055	3058	rBV4	1160	1858	0.20%	0.027%
48	21.438	3070	3072	3075	rBV4	1521	2092	0.23%	0.031%
49	21.515	3083	3085	3087	rBV2	1517	1391	0.15%	0.020%
50	21.720	3113	3120	3129	rVB	262649	434594	47.57%	6.358%

51	21.808	3134	3135	3138	rBV3	1977	2083	0.23%	0.030%
52	21.920	3151	3154	3157	rVB4	1836	1839	0.20%	0.027%
53	22.531	3256	3258	3259	rBV2	2129	1051	0.12%	0.015%
54	23.236	3374	3378	3385	rVB7	4108	8775	0.96%	0.128%
55	23.301	3387	3389	3392	rVB4	1767	1702	0.19%	0.025%

56	23.424	3408	3410	3411	rBV2	1770	1126	0.12%	0.016%
57	24.059	3515	3518	3526	rVB5	6698	10613	1.16%	0.155%
58	24.411	3577	3578	3580	rBV2	1587	992	0.11%	0.015%
59	24.529	3597	3598	3600	rBV2	2168	1600	0.18%	0.023%
60	24.635	3614	3616	3619	rBV2	1578	1495	0.16%	0.022%

61	24.758	3624	3637	3650	rBV2	321979	913529	100.00%	13.365%
62	24.905	3660	3662	3663	rBV2	1509	1275	0.14%	0.019%
63	24.975	3664	3674	3690	rVB2	149099	454665	49.77%	6.652%
64	25.810	3814	3816	3818	rBV3	1587	1723	0.19%	0.025%
65	26.174	3873	3878	3880	rBV5	5605	9089	0.99%	0.133%

66	26.344	3905	3907	3911	rBV4	1664	2118	0.23%	0.031%
67	26.761	3976	3978	3980	rBV3	1297	949	0.10%	0.014%
68	26.944	4007	4009	4012	rBV3	1545	1632	0.18%	0.024%
69	27.243	4058	4060	4064	rBV4	1523	1994	0.22%	0.029%
70	27.907	4171	4173	4178	rBV5	1658	2099	0.23%	0.031%

71	28.841	4330	4332	4334	rVB3	1528	939	0.10%	0.014%
72	29.082	4371	4373	4374	rBV2	1946	1613	0.18%	0.024%
73	30.369	4590	4592	4594	rVB2	1595	989	0.11%	0.014%
74	30.393	4594	4596	4598	rBV3	1426	1466	0.16%	0.021%
75	30.592	4629	4630	4633	rBV3	1525	1323	0.14%	0.019%

76	30.757	4656	4658	4661	rVB3	1882	1149	0.13%	0.017%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053975.D
Acq On : 21 Jun 2022 12:52
Operator : CG/JU
Sample : N3285-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	32.267	4912	4915	4917	rBV3	1391	1822	0.20%	0.027%
78	32.549	4961	4963	4967	rVB4	1450	1603	0.18%	0.023%
79	32.584	4967	4969	4971	rBV2	1723	1254	0.14%	0.018%




Sum of corrected areas: 6835441

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053975.D
Acq On : 21 Jun 2022 12:52
Operator : CG/JU
Sample : N3285-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

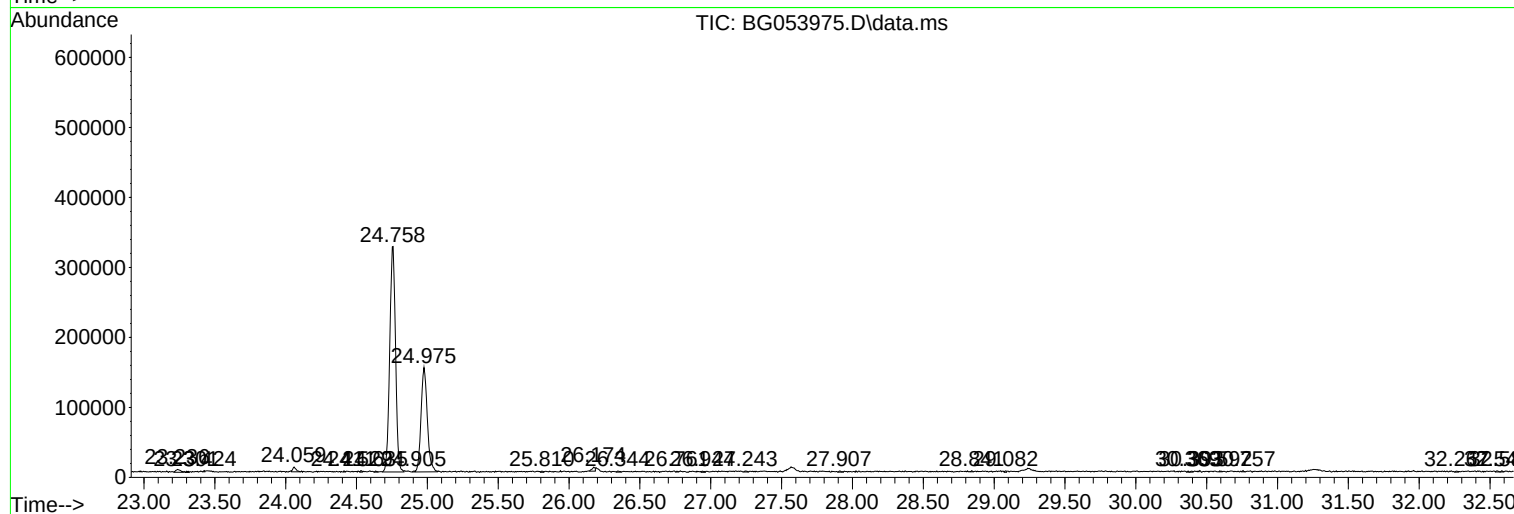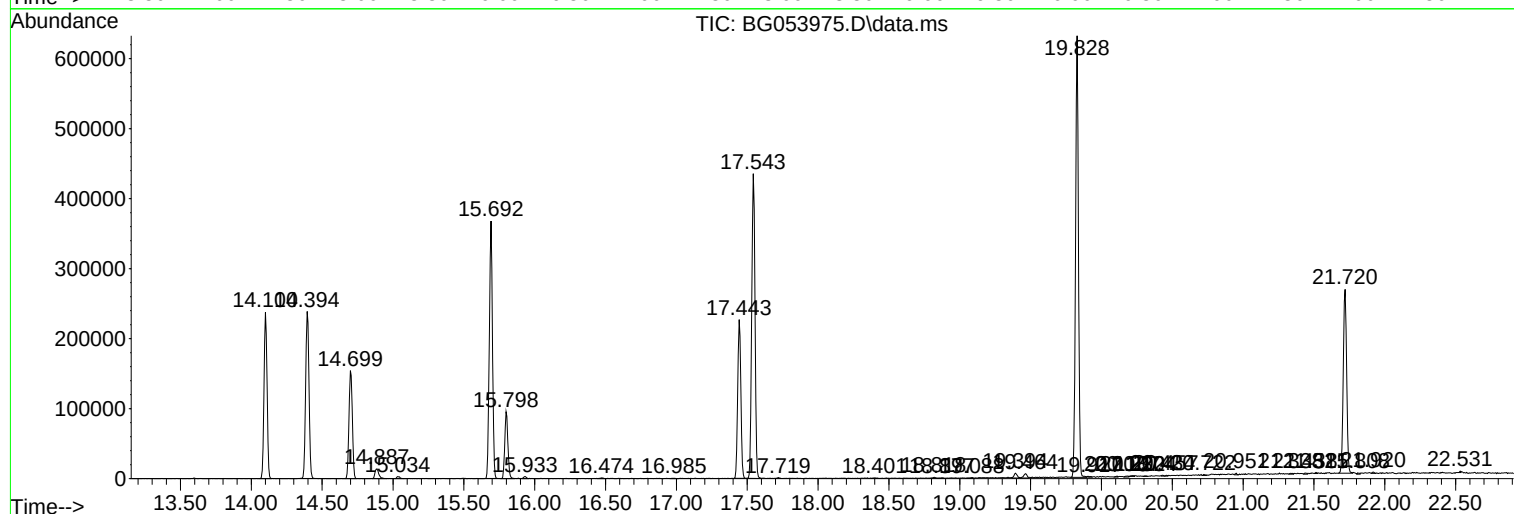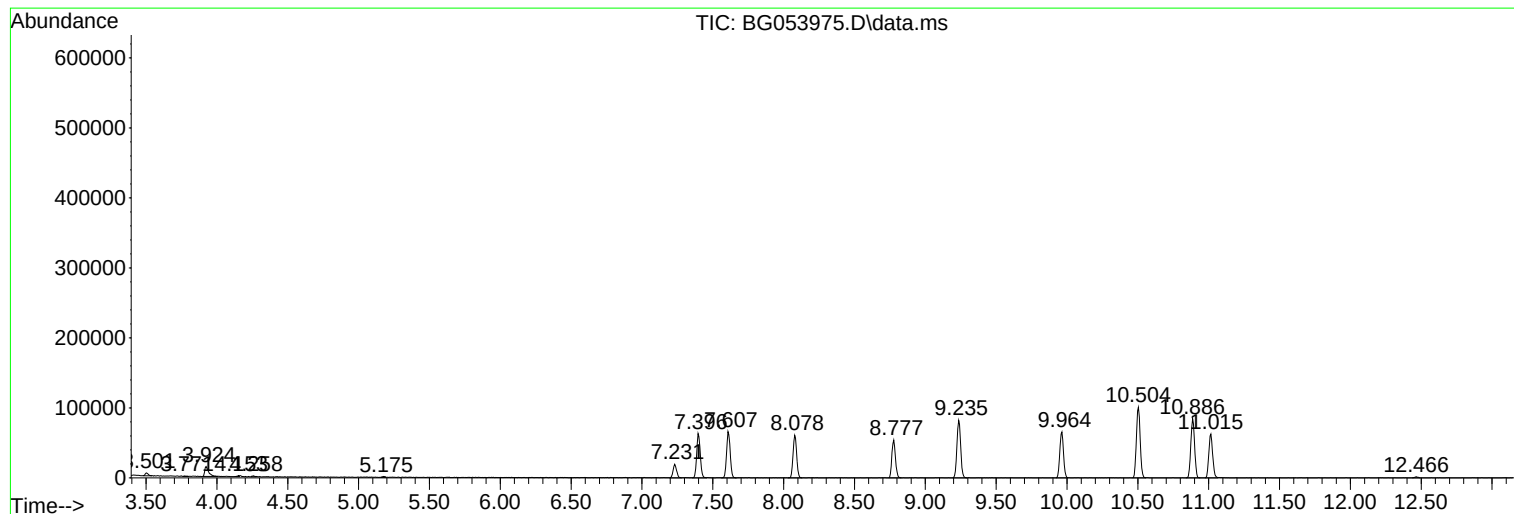

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053975.D
Acq On : 21 Jun 2022 12:52
Operator : CG/JU
Sample : N3285-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053975.D
Acq On : 21 Jun 2022 12:52
Operator : CG/JU
Sample : N3285-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc