

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053976.D
 Acq On : 21 Jun 2022 13:30
 Operator : CG/JU
 Sample : N3285-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.506	16	20	27	rVB2	4096	7029	0.82%	0.106%
2	3.917	88	90	100	rBV	16545	29829	3.48%	0.449%
3	4.164	129	132	135	rVB4	1793	2257	0.26%	0.034%
4	4.258	145	148	152	rVB3	1113	1809	0.21%	0.027%
5	5.145	293	299	300	rBV3	798	1478	0.17%	0.022%
6	6.021	441	448	451	rBV3	463	1045	0.12%	0.016%
7	7.231	648	654	661	rVB2	17388	30434	3.55%	0.458%
8	7.396	676	682	693	rBV	55440	98359	11.47%	1.480%
9	7.607	712	718	730	rVB2	59353	105321	12.29%	1.585%
10	8.077	791	798	806	rBV	62143	111390	12.99%	1.677%
11	8.776	909	917	927	rBB2	50064	86791	10.13%	1.306%
12	9.235	988	995	1004	rBV	72727	135914	15.86%	2.046%
13	9.963	1112	1119	1128	rBB	59073	106309	12.40%	1.600%
14	10.504	1204	1211	1221	rBB	91354	168132	19.61%	2.531%
15	10.886	1269	1276	1285	rBB	85829	160028	18.67%	2.409%
16	11.015	1291	1298	1307	rBV	57767	110218	12.86%	1.659%
17	12.466	1541	1545	1549	rBB	1650	2304	0.27%	0.035%
18	14.100	1817	1823	1830	rBV	229186	336201	39.22%	5.060%
19	14.393	1866	1873	1882	rVB	218668	364455	42.52%	5.485%
20	14.699	1919	1925	1934	rBB	152583	253811	29.61%	3.820%
21	14.881	1951	1956	1964	rBV2	13433	24288	2.83%	0.366%
22	15.040	1979	1983	1990	rBB2	3737	6047	0.71%	0.091%
23	15.504	2058	2062	2064	rBB	843	966	0.11%	0.015%
24	15.692	2087	2094	2103	rBB	333620	534211	62.32%	8.040%
25	15.798	2104	2112	2121	rBV	91336	140925	16.44%	2.121%
26	15.927	2131	2134	2140	rBB	2694	3939	0.46%	0.059%
27	16.473	2224	2227	2232	rBB	1158	1387	0.16%	0.021%
28	17.443	2386	2392	2400	rVB	235500	360756	42.09%	5.430%
29	17.543	2403	2409	2421	rVB	421656	653996	76.30%	9.843%
30	17.719	2435	2439	2443	rVB2	1377	1782	0.21%	0.027%
31	18.330	2539	2543	2552	rBV4	7731	11775	1.37%	0.177%
32	18.394	2552	2554	2557	rVV2	1082	1192	0.14%	0.018%
33	18.818	2623	2626	2630	rVV3	1197	1731	0.20%	0.026%
34	19.393	2720	2724	2731	rBV2	5884	9796	1.14%	0.147%
35	19.464	2731	2736	2742	rVB2	6193	9587	1.12%	0.144%
36	19.575	2751	2755	2756	rBV	838	919	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053976.D
 Acq On : 21 Jun 2022 13:30
 Operator : CG/JU
 Sample : N3285-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.605	2756	2760	2765	rVV2	2706	4137	0.48%	0.062%
38	19.746	2782	2784	2787	rBV3	1339	1247	0.15%	0.019%
39	19.828	2791	2798	2806	rVV	595825	857190	100.00%	12.902%
40	19.940	2814	2817	2819	rVB3	1332	1075	0.13%	0.016%
41	19.963	2819	2821	2823	rBV3	922	897	0.10%	0.014%
42	20.016	2827	2830	2833	rBV2	800	1088	0.13%	0.016%
43	20.228	2860	2866	2868	rBV4	2209	4589	0.54%	0.069%
44	20.357	2886	2888	2890	rBV2	1216	1055	0.12%	0.016%
45	20.480	2907	2909	2912	rBV3	1060	1323	0.15%	0.020%
46	20.551	2918	2921	2924	rBV3	1721	1931	0.23%	0.029%
47	20.892	2977	2979	2983	rVB5	1335	1437	0.17%	0.022%
48	20.921	2983	2984	2986	rBV2	1375	1022	0.12%	0.015%
49	20.962	2990	2991	2993	rBV2	1212	1096	0.13%	0.016%
50	21.038	3002	3004	3005	rBV2	1416	1194	0.14%	0.018%
51	21.273	3042	3044	3047	rBV4	1347	1267	0.15%	0.019%
52	21.356	3054	3058	3064	rBV3	20864	33237	3.88%	0.500%
53	21.473	3076	3078	3079	rBV2	1631	980	0.11%	0.015%
54	21.632	3103	3105	3106	rBV2	1739	1603	0.19%	0.024%
55	21.720	3113	3120	3130	rVB	265570	446566	52.10%	6.721%
56	21.920	3151	3154	3159	rVB6	2395	4071	0.47%	0.061%
57	21.961	3159	3161	3163	rBV3	1574	1181	0.14%	0.018%
58	22.108	3184	3186	3188	rVB3	1762	1289	0.15%	0.019%
59	22.178	3196	3198	3199	rBV2	1797	1176	0.14%	0.018%
60	22.907	3320	3322	3323	rVV2	1550	985	0.11%	0.015%
61	22.948	3327	3329	3332	rBV3	1355	1542	0.18%	0.023%
62	23.242	3375	3379	3384	rBV5	4116	5332	0.62%	0.080%
63	23.553	3431	3432	3435	rVB3	1488	960	0.11%	0.014%
64	23.624	3442	3444	3447	rVB3	1886	1364	0.16%	0.021%
65	24.058	3513	3518	3524	rBV6	6595	13796	1.61%	0.208%
66	24.399	3574	3576	3578	rBV3	1578	1476	0.17%	0.022%
67	24.440	3581	3583	3585	rVB3	1516	964	0.11%	0.015%
68	24.570	3603	3605	3607	rBV2	1223	1223	0.14%	0.018%
69	24.752	3625	3636	3651	rVB2	298023	857095	99.99%	12.900%
70	24.981	3662	3675	3692	rVB2	148997	461049	53.79%	6.939%
71	25.427	3749	3751	3752	rVB2	2089	1257	0.15%	0.019%
72	25.615	3781	3783	3785	rBV3	1425	1287	0.15%	0.019%
73	25.862	3823	3825	3827	rBV2	1456	1033	0.12%	0.016%
74	26.144	3871	3873	3874	rVV2	2643	2238	0.26%	0.034%
75	26.185	3875	3880	3892	rVB9	6659	19837	2.31%	0.299%
76	27.002	4018	4019	4023	rBV3	1403	1581	0.18%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053976.D
 Acq On : 21 Jun 2022 13:30
 Operator : CG/JU
 Sample : N3285-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW4R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	27.537	4108	4110	4111	rBV2	2381	1685	0.20%	0.025%
78	27.883	4167	4169	4170	rBV2	1248	921	0.11%	0.014%
79	28.083	4201	4203	4206	rBV4	1253	1604	0.19%	0.024%
80	28.306	4239	4241	4242	rBV	1510	1355	0.16%	0.020%
81	28.500	4273	4274	4276	rVB	2334	952	0.11%	0.014%
82	28.906	4341	4343	4346	rVB3	1583	1265	0.15%	0.019%
83	30.087	4543	4544	4551	rBV6	1597	3122	0.36%	0.047%
84	30.463	4606	4608	4609	rBV2	1411	1052	0.12%	0.016%
85	30.527	4617	4619	4623	rBV5	1612	2144	0.25%	0.032%
86	31.027	4703	4704	4707	rBV	1426	1767	0.21%	0.027%
87	31.573	4796	4797	4800	rVB3	1537	1345	0.16%	0.020%
88	31.890	4849	4851	4855	rBV5	1317	1155	0.13%	0.017%
89	31.973	4863	4865	4866	rBV2	1284	1133	0.13%	0.017%
90	32.002	4868	4870	4873	rBV3	1451	1761	0.21%	0.027%
91	32.360	4929	4931	4934	rBV3	1650	1676	0.20%	0.025%
92	32.625	4974	4976	4979	rBV	1399	991	0.12%	0.015%




Sum of corrected areas: 6644009

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053976.D
Acq On : 21 Jun 2022 13:30
Operator : CG/JU
Sample : N3285-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

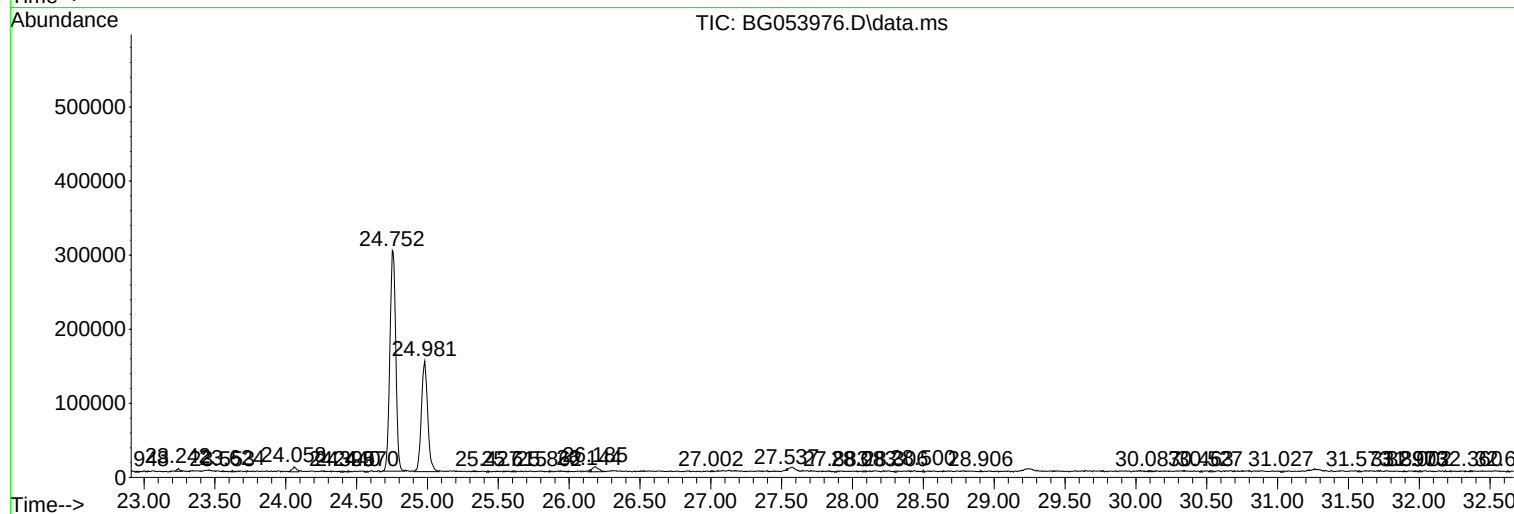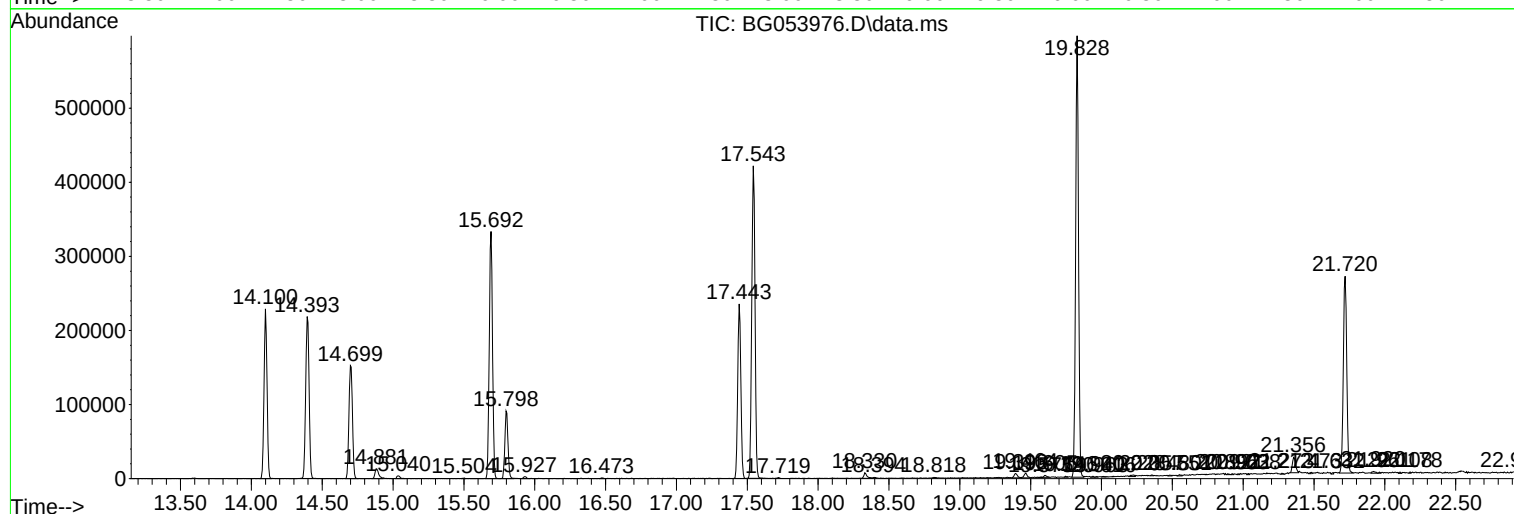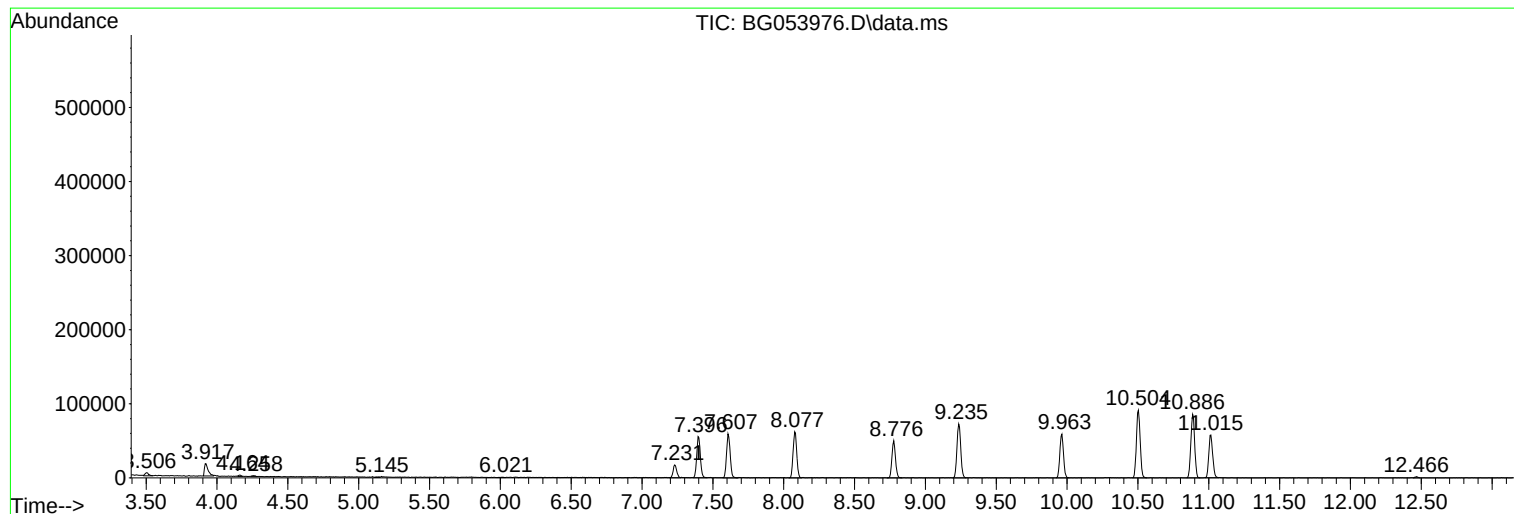

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053976.D
Acq On : 21 Jun 2022 13:30
Operator : CG/JU
Sample : N3285-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053976.D
Acq On : 21 Jun 2022 13:30
Operator : CG/JU
Sample : N3285-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW4R2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc