

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053986.D
 Acq On : 21 Jun 2022 20:39
 Operator : CG/JU
 Sample : PB145686BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.501	16	19	26	rVB3	5311	8748	1.06%	0.126%
2	3.918	86	90	104	rBV	61757	115344	13.99%	1.661%
3	4.264	146	149	152	rVB3	1268	1493	0.18%	0.022%
4	4.770	230	235	239	rBV3	597	1210	0.15%	0.017%
5	5.069	280	286	287	rVB2	620	1024	0.12%	0.015%
6	5.716	392	396	398	rVB2	680	882	0.11%	0.013%
7	5.745	398	401	404	rBV3	759	1085	0.13%	0.016%
8	5.921	427	431	435	rBV	678	1185	0.14%	0.017%
9	7.231	648	654	667	rBV	79447	143487	17.40%	2.067%
10	7.396	676	682	692	rBV	58291	103834	12.59%	1.495%
11	7.607	709	718	728	rVB	78527	143707	17.43%	2.070%
12	8.078	791	798	805	rBV	61654	105521	12.80%	1.520%
13	8.777	910	917	924	rBV	102545	183915	22.31%	2.649%
14	9.235	988	995	1005	rBB	77940	145137	17.60%	2.090%
15	9.964	1112	1119	1127	rBB2	66429	121212	14.70%	1.746%
16	10.504	1204	1211	1220	rBV	106196	192283	23.32%	2.769%
17	10.886	1269	1276	1284	rBV	83986	154851	18.78%	2.230%
18	11.015	1291	1298	1306	rBV	99324	191941	23.28%	2.764%
19	12.466	1540	1545	1550	rBB2	1089	1995	0.24%	0.029%
20	14.100	1817	1823	1830	rBV	228076	337201	40.90%	4.857%
21	14.394	1866	1873	1882	rBV	232590	379580	46.04%	5.467%
22	14.699	1918	1925	1932	rBB	156926	248877	30.19%	3.585%
23	14.881	1951	1956	1970	rBV	78362	133811	16.23%	1.927%
24	15.692	2087	2094	2102	rBB	341734	526874	63.91%	7.588%
25	15.798	2107	2112	2123	rBV	82690	129698	15.73%	1.868%
26	15.933	2132	2135	2139	rVB3	2835	3518	0.43%	0.051%
27	16.474	2223	2227	2230	rBB2	1113	1126	0.14%	0.016%
28	17.443	2385	2392	2399	rBV	235696	357227	43.33%	5.145%
29	17.543	2401	2409	2423	rBV	402933	623597	75.64%	8.982%
30	19.347	2713	2716	2718	rVV2	809	1018	0.12%	0.015%
31	19.394	2720	2724	2730	rVV4	5305	8463	1.03%	0.122%
32	19.464	2730	2736	2742	rVV2	4809	8202	0.99%	0.118%
33	19.523	2744	2746	2749	rVV3	793	1010	0.12%	0.015%
34	19.699	2773	2776	2777	rVV	882	966	0.12%	0.014%
35	19.828	2790	2798	2808	rBV	532967	790486	95.88%	11.385%
36	20.169	2851	2856	2857	rBV3	1417	1871	0.23%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053986.D
 Acq On : 21 Jun 2022 20:39
 Operator : CG/JU
 Sample : PB145686BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.187	2857	2859	2861	rBV2	1210	1323	0.16%	0.019%
38	20.216	2861	2864	2866	rBV4	1940	2732	0.33%	0.039%
39	20.710	2946	2948	2950	rBV3	981	857	0.10%	0.012%
40	20.857	2970	2973	2975	rBV4	962	1232	0.15%	0.018%
41	21.250	3038	3040	3042	rBV3	1330	1138	0.14%	0.016%
42	21.380	3060	3062	3063	rBV2	1445	1273	0.15%	0.018%
43	21.573	3093	3095	3101	rVB7	1487	1950	0.24%	0.028%
44	21.720	3113	3120	3128	rVB	256198	440518	53.43%	6.345%
45	21.967	3159	3162	3164	rBV3	1405	1984	0.24%	0.029%
46	22.055	3176	3177	3180	rBV2	1577	1539	0.19%	0.022%
47	22.143	3191	3192	3195	rBV3	1287	1256	0.15%	0.018%
48	22.190	3198	3200	3202	rBV3	1235	1048	0.13%	0.015%
49	22.267	3211	3213	3215	rBV2	1481	1152	0.14%	0.017%
50	22.484	3248	3250	3251	rBV2	1348	986	0.12%	0.014%
51	22.502	3251	3253	3254	rBV2	1523	1006	0.12%	0.014%
52	22.837	3308	3310	3311	rBV2	1215	1014	0.12%	0.015%
53	23.048	3344	3346	3347	rBV2	1319	1064	0.13%	0.015%
54	24.012	3509	3510	3513	rBV3	1455	1577	0.19%	0.023%
55	24.047	3513	3516	3517	rBV3	1616	1689	0.20%	0.024%
56	24.364	3568	3570	3572	rBV3	1267	1182	0.14%	0.017%
57	24.635	3613	3616	3617	rBV3	1699	1728	0.21%	0.025%
58	24.752	3624	3636	3648	rBV2	285012	824458	100.00%	11.874%
59	24.975	3664	3674	3686	rBV	153802	442463	53.67%	6.373%
60	25.087	3691	3693	3694	rBV2	1632	960	0.12%	0.014%
61	25.140	3700	3702	3704	rBV2	1228	1088	0.13%	0.016%
62	26.103	3865	3866	3870	rBV4	1727	1797	0.22%	0.026%
63	26.174	3872	3878	3879	rBV5	2393	4184	0.51%	0.060%
64	26.268	3892	3894	3897	rBV2	1318	999	0.12%	0.014%
65	26.568	3943	3945	3949	rBV5	1277	1358	0.16%	0.020%
66	27.085	4031	4033	4034	rBV	1562	983	0.12%	0.014%
67	27.655	4128	4130	4134	rVB4	1469	1533	0.19%	0.022%
68	27.690	4134	4136	4138	rBV3	1406	946	0.11%	0.014%
69	27.907	4171	4173	4175	rBV3	1555	971	0.12%	0.014%
70	28.031	4192	4194	4196	rBV3	1250	1031	0.13%	0.015%
71	29.347	4416	4418	4419	rBV	1407	886	0.11%	0.013%
72	29.811	4495	4497	4498	rBV2	1770	1242	0.15%	0.018%
73	30.052	4536	4538	4539	rBV2	1198	929	0.11%	0.013%
74	30.751	4655	4657	4660	rBV4	1424	1520	0.18%	0.022%
75	31.344	4754	4758	4759	rBV3	1464	2088	0.25%	0.030%
76	31.509	4785	4786	4788	rBV2	1686	1415	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053986.D
Acq On : 21 Jun 2022 20:39
Operator : CG/JU
Sample : PB145686BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK686

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	31.762	4828	4829	4833	rBV3	1242	1010	0.12%	0.015%
78	31.838	4840	4842	4843	rBV2	1555	1193	0.14%	0.017%
79	32.055	4877	4879	4881	rBV2	2282	2254	0.27%	0.032%
80	32.149	4894	4895	4898	rBV2	1754	1621	0.20%	0.023%
81	32.179	4898	4900	4901	rBV2	1670	1015	0.12%	0.015%
82	32.232	4907	4909	4913	rBV3	1479	1274	0.15%	0.018%
83	32.390	4935	4936	4941	rBV4	1492	2024	0.25%	0.029%
84	32.431	4941	4943	4944	rBV2	1499	1245	0.15%	0.018%




Sum of corrected areas: 6943114

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053986.D
Acq On : 21 Jun 2022 20:39
Operator : CG/JU
Sample : PB145686BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

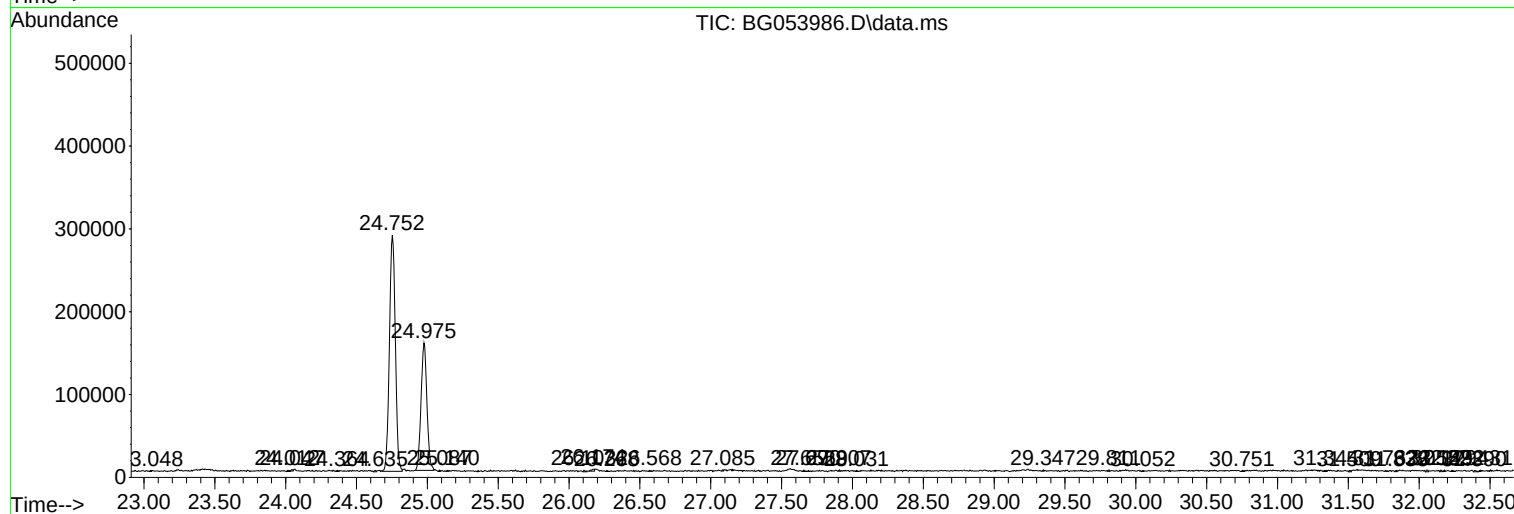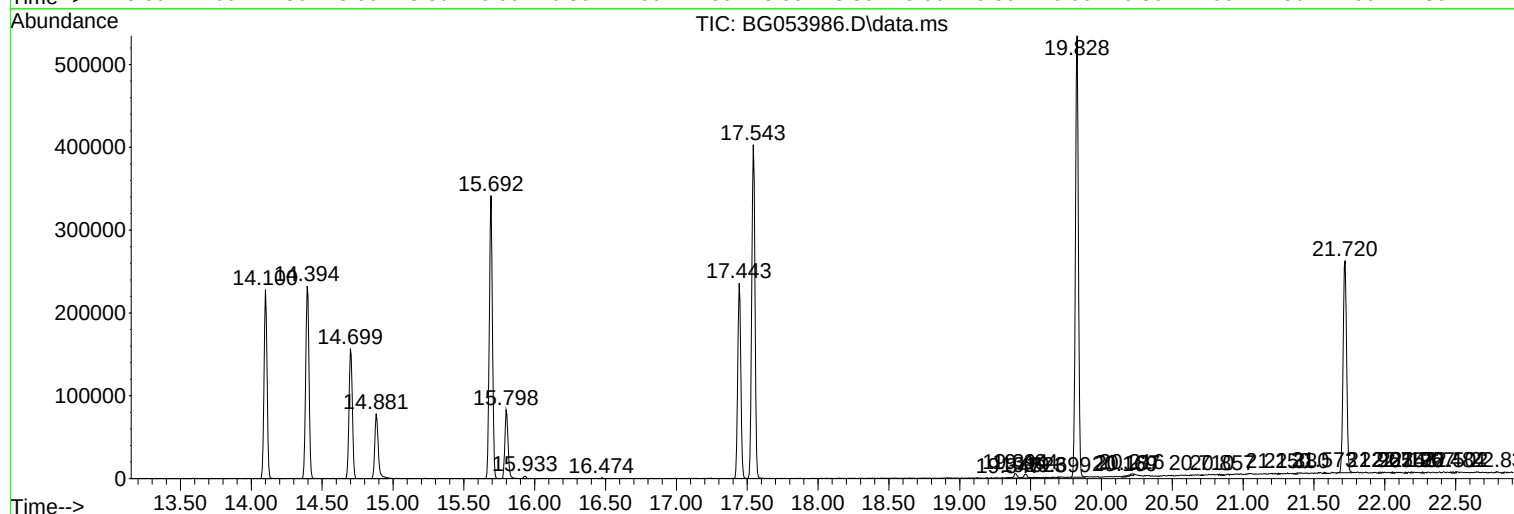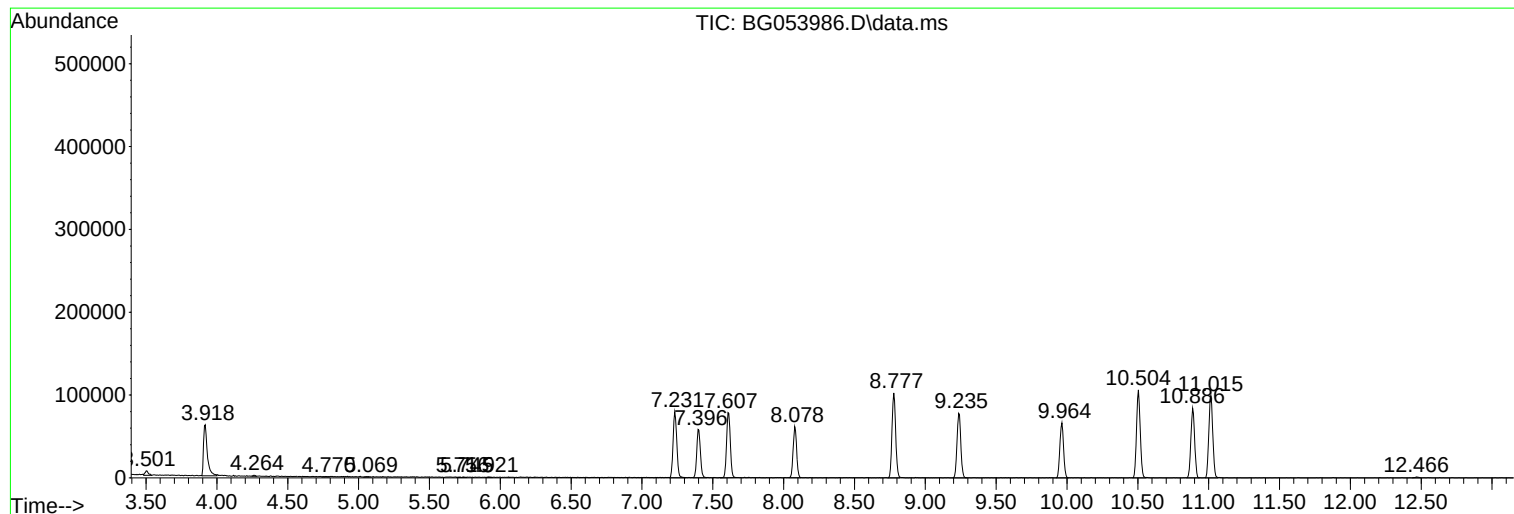

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053986.D
Acq On : 21 Jun 2022 20:39
Operator : CG/JU
Sample : PB145686BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053986.D
Acq On : 21 Jun 2022 20:39
Operator : CG/JU
Sample : PB145686BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc