

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053987.D
 Acq On : 21 Jun 2022 21:18
 Operator : CG/JU
 Sample : N3389-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.441	8	9	13	rVB3	964	755	0.17%	0.042%
2	3.547	26	27	31	rBV3	604	707	0.16%	0.039%
3	3.940	93	94	97	rBV2	651	605	0.14%	0.034%
4	4.034	108	110	114	rVB2	733	738	0.17%	0.041%
5	4.075	114	117	119	rVB2	631	825	0.19%	0.046%
6	4.105	119	122	125	rBV3	757	982	0.22%	0.055%
7	4.252	144	147	148	rVV2	1185	925	0.21%	0.051%
8	4.422	174	176	178	rBV2	731	767	0.17%	0.043%
9	4.563	196	200	202	rVB3	722	716	0.16%	0.040%
10	4.916	257	260	264	rBV	449	705	0.16%	0.039%
11	5.051	282	283	287	rVB	680	530	0.12%	0.029%
12	5.121	292	295	299	rVV2	439	713	0.16%	0.040%
13	5.168	301	303	309	rVB3	773	847	0.19%	0.047%
14	5.515	358	362	364	rBV2	604	728	0.16%	0.040%
15	5.591	369	375	377	rBV3	534	723	0.16%	0.040%
16	5.944	432	435	436	rBV2	595	619	0.14%	0.034%
17	6.014	445	447	449	rBV	619	592	0.13%	0.033%
18	6.155	468	471	473	rBV	637	645	0.15%	0.036%
19	6.367	506	507	512	rVB2	444	563	0.13%	0.031%
20	6.426	514	517	520	rVB2	560	682	0.15%	0.038%
21	6.808	578	582	586	rVB2	586	943	0.21%	0.052%
22	6.990	610	613	616	rBV	565	735	0.17%	0.041%
23	8.000	780	785	787	rBB	379	542	0.12%	0.030%
24	8.083	791	799	807	rBB	58068	101505	22.96%	5.642%
25	10.891	1269	1277	1286	rBV	75469	145247	32.85%	8.073%
26	14.698	1919	1925	1934	rBV	146026	241114	54.53%	13.401%
27	17.442	2384	2392	2402	rVV	217032	341829	77.31%	18.999%
28	17.507	2402	2403	2407	rVV	829	862	0.19%	0.048%
29	17.548	2407	2410	2413	rVV2	516	611	0.14%	0.034%
30	18.864	2630	2634	2636	rVV3	739	887	0.20%	0.049%
31	18.958	2647	2650	2652	rBV	460	567	0.13%	0.032%
32	19.111	2674	2676	2678	rBV	880	693	0.16%	0.039%
33	19.134	2678	2680	2685	rVB	563	926	0.21%	0.051%
34	19.240	2697	2698	2702	rBV	551	533	0.12%	0.030%
35	19.293	2702	2707	2709	rBV2	706	821	0.19%	0.046%
36	19.405	2724	2726	2729	rVB2	723	751	0.17%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053987.D
 Acq On : 21 Jun 2022 21:18
 Operator : CG/JU
 Sample : N3389-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.481	2736	2739	2743	rVB	705	763	0.17%	0.042%
38	19.634	2764	2765	2770	rVB2	843	1139	0.26%	0.063%
39	19.675	2770	2772	2776	rBV2	794	1035	0.23%	0.058%
40	19.769	2786	2788	2790	rBV2	461	622	0.14%	0.035%
41	19.833	2794	2799	2800	rBV	587	792	0.18%	0.044%
42	19.945	2814	2818	2820	rBV3	802	1065	0.24%	0.059%
43	19.974	2820	2823	2825	rBV3	804	833	0.19%	0.046%
44	20.010	2827	2829	2833	rVB2	795	744	0.17%	0.041%
45	20.051	2833	2836	2840	rBV2	888	1499	0.34%	0.083%
46	20.204	2860	2862	2863	rBV	592	545	0.12%	0.030%
47	20.221	2863	2865	2867	rVB3	720	659	0.15%	0.037%
48	20.368	2886	2890	2891	rBV3	923	1083	0.24%	0.060%
49	20.539	2917	2919	2920	rBV	805	604	0.14%	0.034%
50	20.556	2920	2922	2923	rVB2	1436	717	0.16%	0.040%
51	20.591	2923	2928	2931	rBV5	1114	2065	0.47%	0.115%
52	20.650	2936	2938	2940	rBV2	849	661	0.15%	0.037%
53	20.809	2963	2965	2966	rBV2	964	686	0.16%	0.038%
54	20.850	2971	2972	2976	rVV3	1036	980	0.22%	0.054%
55	21.108	3014	3016	3019	rBV3	1628	2025	0.46%	0.113%
56	21.261	3039	3042	3043	rBV3	1456	1655	0.37%	0.092%
57	21.320	3051	3052	3053	rBV	1188	557	0.13%	0.031%
58	21.520	3084	3086	3089	rBV4	1207	936	0.21%	0.052%
59	21.719	3113	3120	3132	rBV	259824	442174	100.00%	24.576%
60	21.796	3132	3133	3135	rVB2	1855	719	0.16%	0.040%
61	22.113	3185	3187	3189	rBV2	1147	721	0.16%	0.040%
62	22.583	3266	3267	3269	rBV2	1215	949	0.21%	0.053%
63	22.671	3281	3282	3283	rBV	1301	560	0.13%	0.031%
64	23.517	3424	3426	3430	rVB4	2027	1930	0.44%	0.107%
65	23.588	3434	3438	3440	rBV4	1767	2270	0.51%	0.126%
66	23.676	3452	3453	3456	rBV3	1251	839	0.19%	0.047%
67	23.917	3492	3494	3495	rBV	1390	693	0.16%	0.039%
68	23.935	3495	3497	3498	rBV2	1362	977	0.22%	0.054%
69	23.993	3505	3507	3510	rBV3	1219	710	0.16%	0.039%
70	24.064	3515	3519	3520	rBV4	1636	1474	0.33%	0.082%
71	24.810	3643	3646	3647	rBV3	1340	1056	0.24%	0.059%
72	24.974	3662	3674	3690	rBV2	144244	440233	99.56%	24.468%
73	26.056	3856	3858	3860	rBV3	1489	1037	0.23%	0.058%
74	26.279	3894	3896	3897	rVB2	1894	1053	0.24%	0.059%
75	26.379	3911	3913	3914	rVB2	1791	931	0.21%	0.052%
76	26.520	3935	3937	3938	rBV2	1287	786	0.18%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053987.D
 Acq On : 21 Jun 2022 21:18
 Operator : CG/JU
 Sample : N3389-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	26.602	3949	3951	3952	rVB2	1289	567	0.13%	0.032%
78	27.372	4080	4082	4083	rBV2	1210	981	0.22%	0.055%
79	27.419	4089	4090	4094	rVV3	1498	1395	0.32%	0.078%
80	27.454	4094	4096	4097	rVB2	2288	1082	0.24%	0.060%
81	28.018	4190	4192	4193	rBV2	2255	1320	0.30%	0.073%
82	28.083	4201	4203	4204	rVB2	1445	823	0.19%	0.046%
83	28.300	4238	4240	4241	rBV	1233	691	0.16%	0.038%
84	28.582	4286	4288	4290	rBV3	1486	1551	0.35%	0.086%
85	28.688	4304	4306	4307	rBV2	1216	910	0.21%	0.051%
86	29.052	4366	4368	4369	rVB2	1472	854	0.19%	0.047%
87	29.093	4373	4375	4376	rBV2	1189	802	0.18%	0.045%
88	29.140	4381	4383	4385	rVB2	1468	1111	0.25%	0.062%
89	29.287	4406	4408	4411	rVB3	1632	1459	0.33%	0.081%
90	29.399	4425	4427	4428	rBV2	1379	1239	0.28%	0.069%
91	29.481	4440	4441	4443	rBV2	1762	1081	0.24%	0.060%
92	29.775	4490	4491	4495	rBV3	1418	1751	0.40%	0.097%
93	30.210	4563	4565	4566	rBV2	1292	885	0.20%	0.049%
94	30.809	4665	4667	4669	rBV3	1763	1466	0.33%	0.081%
95	31.150	4723	4725	4726	rBV2	1171	671	0.15%	0.037%
96	31.661	4811	4812	4816	rVB3	1319	817	0.18%	0.045%
97	31.996	4867	4869	4872	rVB4	1498	1066	0.24%	0.059%
98	32.148	4893	4895	4898	rBV4	1592	1328	0.30%	0.074%
99	32.289	4917	4919	4920	rBV	1378	914	0.21%	0.051%
100	32.325	4923	4925	4926	rBV	1184	746	0.17%	0.041%




Sum of corrected areas: 1799220

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053987.D
Acq On : 21 Jun 2022 21:18
Operator : CG/JU
Sample : N3389-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

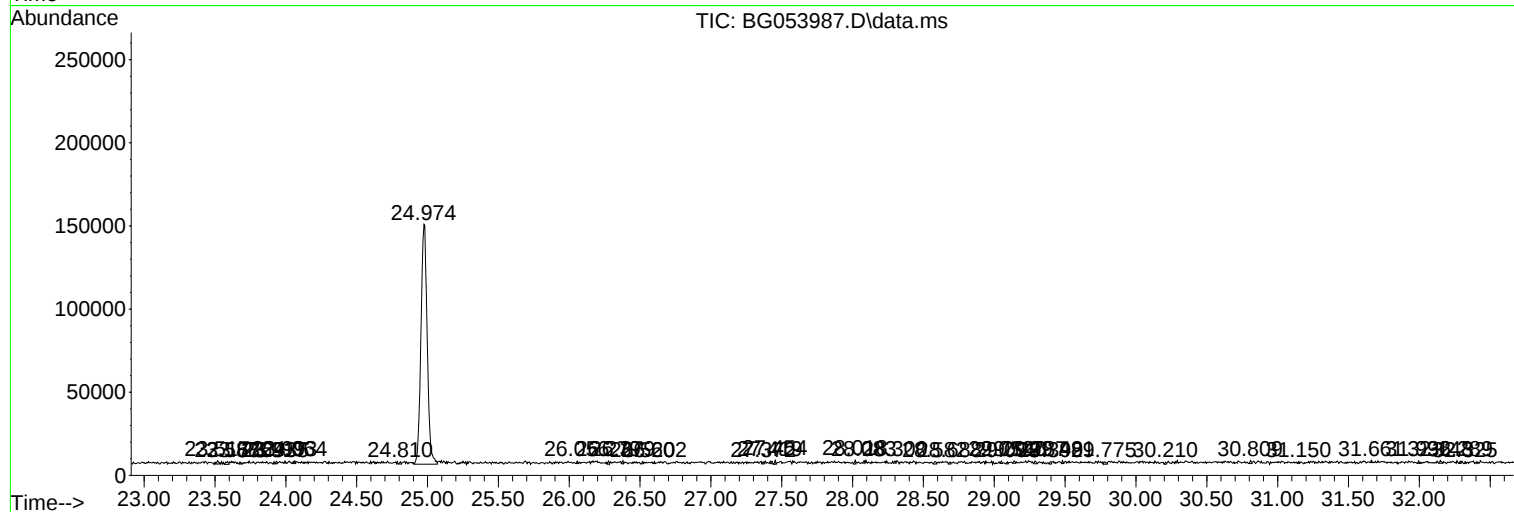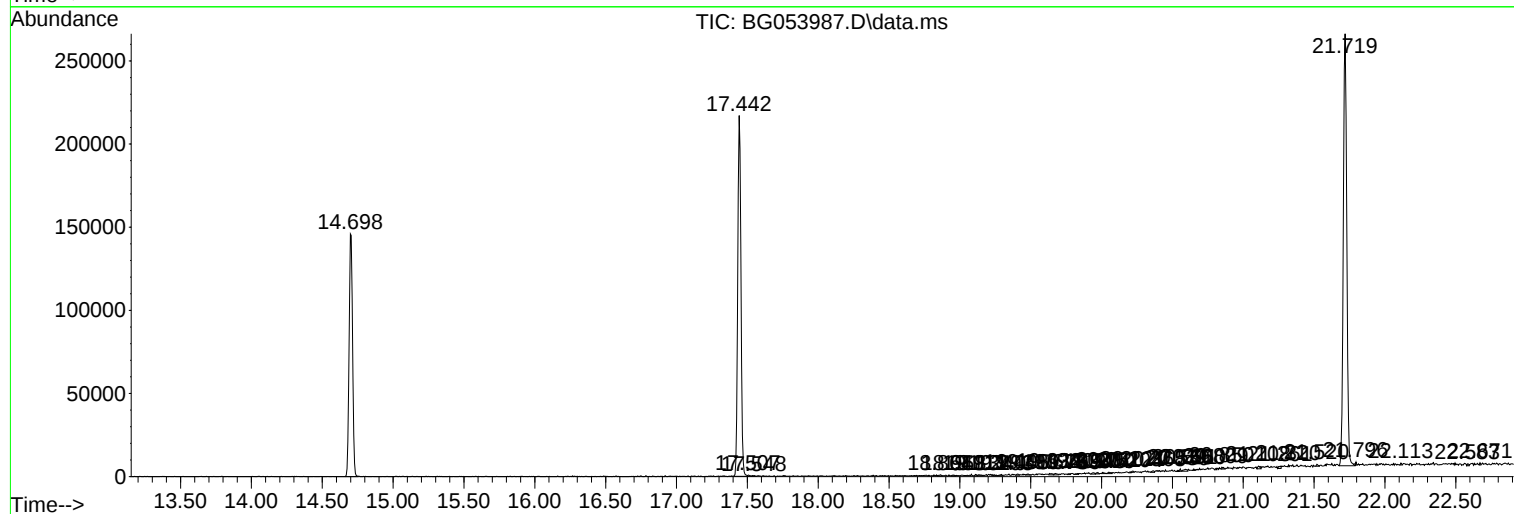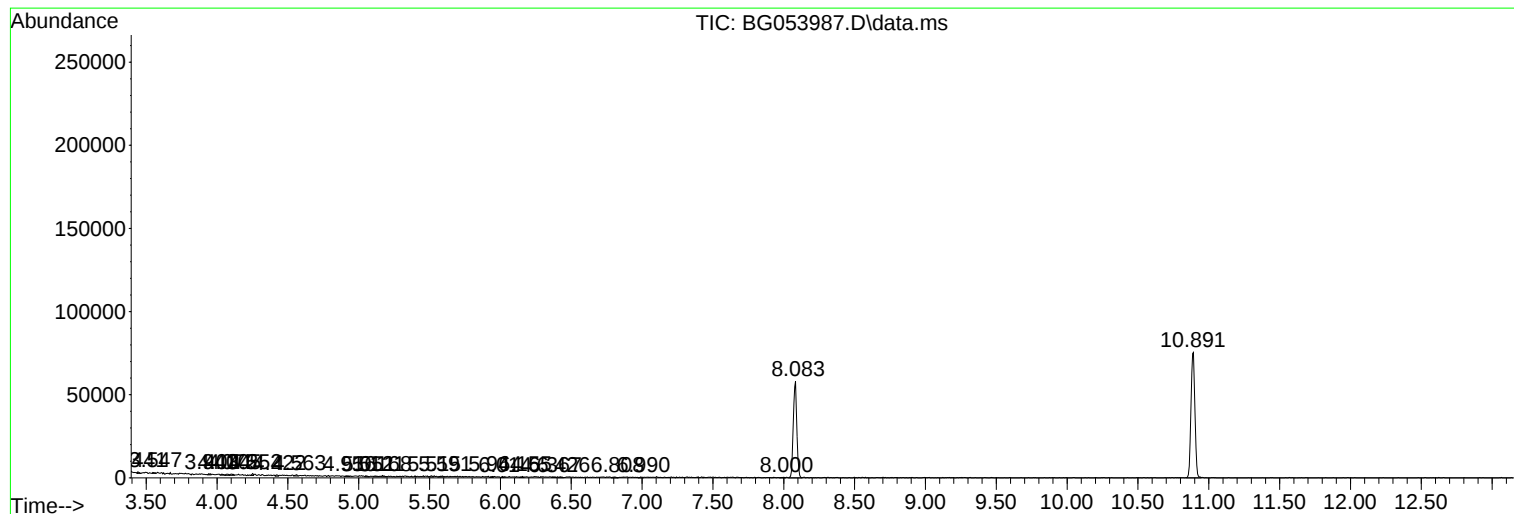

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053987.D
Acq On : 21 Jun 2022 21:18
Operator : CG/JU
Sample : N3389-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053987.D
Acq On : 21 Jun 2022 21:18
Operator : CG/JU
Sample : N3389-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc