

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053989.D
 Acq On : 21 Jun 2022 22:36
 Operator : CG/JU
 Sample : PB145688BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.503	16	19	27	rVB5	5536	9167	1.12%	0.129%
2	3.879	81	83	85	rBV2	827	836	0.10%	0.012%
3	3.915	85	89	103	rVV	65034	116269	14.21%	1.636%
4	6.188	473	476	483	rBV3	628	1097	0.13%	0.015%
5	7.234	646	654	665	rBV	78591	143917	17.59%	2.025%
6	7.399	675	682	692	rVB	60436	103332	12.63%	1.454%
7	7.610	711	718	726	rBV	81967	143592	17.55%	2.021%
8	8.080	791	798	806	rBV	69010	122002	14.91%	1.717%
9	8.779	910	917	928	rVB	103337	183588	22.44%	2.583%
10	9.238	988	995	1008	rBB	78488	144844	17.70%	2.038%
11	9.960	1112	1118	1127	rVB	65563	118443	14.48%	1.667%
12	10.501	1203	1210	1222	rBV	100047	189620	23.18%	2.668%
13	10.883	1268	1275	1283	rBV	91588	174228	21.30%	2.452%
14	11.012	1290	1297	1311	rBB	99273	186473	22.79%	2.624%
15	12.469	1541	1545	1549	rBB2	1345	1987	0.24%	0.028%
16	14.103	1816	1823	1834	rBB	217043	324050	39.61%	4.560%
17	14.396	1865	1873	1885	rBB	233857	365533	44.68%	5.144%
18	14.702	1918	1925	1932	rBB	171326	273833	33.47%	3.853%
19	14.884	1950	1956	1966	rBV	75901	127195	15.55%	1.790%
20	15.689	2087	2093	2102	rBB	316682	508020	62.10%	7.149%
21	15.801	2107	2112	2124	rBV	79315	122007	14.91%	1.717%
22	15.930	2130	2134	2138	rVB3	2750	3498	0.43%	0.049%
23	16.476	2223	2227	2231	rBV2	954	1480	0.18%	0.021%
24	17.446	2385	2392	2399	rBV	251563	390246	47.70%	5.491%
25	17.546	2402	2409	2420	rBV	374852	612523	74.87%	8.619%
26	17.869	2458	2464	2468	rBV	332	920	0.11%	0.013%
27	19.391	2720	2723	2728	rVV3	5446	7649	0.93%	0.108%
28	19.461	2730	2735	2741	rVV3	4812	7592	0.93%	0.107%
29	19.561	2751	2752	2757	rBV	859	1367	0.17%	0.019%
30	19.725	2779	2780	2784	rVB3	794	820	0.10%	0.012%
31	19.825	2790	2797	2806	rBV	515888	792301	96.85%	11.149%
32	19.902	2806	2810	2817	rVB2	1095	2057	0.25%	0.029%
33	20.090	2839	2842	2843	rBV3	1056	839	0.10%	0.012%
34	20.301	2877	2878	2882	rVB2	965	828	0.10%	0.012%
35	20.342	2882	2885	2886	rBV3	830	859	0.10%	0.012%
36	20.648	2935	2937	2938	rBV	1219	881	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053989.D
 Acq On : 21 Jun 2022 22:36
 Operator : CG/JU
 Sample : PB145688BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	21.077	3009	3010	3012	rBV2	1214	1041	0.13%	0.015%
38	21.141	3017	3021	3022	rVV3	1075	1451	0.18%	0.020%
39	21.183	3025	3028	3031	rBV2	1844	1924	0.24%	0.027%
40	21.306	3047	3049	3051	rBV2	1509	1532	0.19%	0.022%
41	21.488	3078	3080	3081	rBV2	1238	1096	0.13%	0.015%
42	21.541	3087	3089	3090	rBV2	1842	845	0.10%	0.012%
43	21.670	3109	3111	3112	rBV2	1099	1002	0.12%	0.014%
44	21.717	3112	3119	3131	rVB2	295090	504772	61.70%	7.103%
45	21.811	3131	3135	3138	rBV5	1587	2759	0.34%	0.039%
46	22.176	3195	3197	3199	rBV	1204	963	0.12%	0.014%
47	22.546	3258	3260	3261	rVB2	1658	1066	0.13%	0.015%
48	22.575	3261	3265	3266	rBV4	1227	1340	0.16%	0.019%
49	22.704	3285	3287	3289	rVB2	1637	914	0.11%	0.013%
50	22.757	3294	3296	3298	rBV2	1438	1247	0.15%	0.018%
51	23.850	3481	3482	3483	rVB	2816	993	0.12%	0.014%
52	23.879	3485	3487	3490	rVB4	1485	1357	0.17%	0.019%
53	23.909	3490	3492	3494	rBV3	1261	1325	0.16%	0.019%
54	23.926	3494	3495	3498	rVB3	1946	1296	0.16%	0.018%
55	24.062	3512	3518	3521	rBV6	4748	8261	1.01%	0.116%
56	24.755	3625	3636	3650	rVB2	291036	818111	100.00%	11.512%
57	24.978	3663	3674	3690	rVB2	164208	507852	62.08%	7.146%
58	25.401	3744	3746	3748	rBV2	1132	1008	0.12%	0.014%
59	25.554	3771	3772	3775	rVB2	1382	900	0.11%	0.013%
60	25.636	3784	3786	3787	rBV	1276	888	0.11%	0.012%
61	25.795	3810	3813	3816	rBV5	1285	2077	0.25%	0.029%
62	25.824	3816	3818	3819	rBV2	1420	1024	0.13%	0.014%
63	25.953	3838	3840	3842	rBV2	1618	1185	0.14%	0.017%
64	26.183	3874	3879	3887	rVB7	5146	13280	1.62%	0.187%
65	26.277	3892	3895	3898	rBV4	1703	2974	0.36%	0.042%
66	26.753	3974	3976	3977	rBV2	1460	839	0.10%	0.012%
67	27.035	4021	4024	4028	rBV5	1315	2235	0.27%	0.031%
68	27.146	4041	4043	4045	rBV3	1206	1037	0.13%	0.015%
69	27.563	4108	4114	4116	rBV7	3582	7200	0.88%	0.101%
70	27.922	4173	4175	4177	rBV	1420	1259	0.15%	0.018%
71	28.074	4197	4201	4202	rBV3	1560	2180	0.27%	0.031%
72	28.509	4273	4275	4277	rBV3	1207	1131	0.14%	0.016%
73	28.956	4349	4351	4354	rBV3	1110	978	0.12%	0.014%
74	29.132	4378	4381	4383	rBV4	1687	2193	0.27%	0.031%
75	29.226	4395	4397	4400	rBV4	1694	2122	0.26%	0.030%
76	29.443	4432	4434	4435	rBV	1222	821	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053989.D
Acq On : 21 Jun 2022 22:36
Operator : CG/JU
Sample : PB145688BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK688

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	29.661	4469	4471	4472	rBV	1285	838	0.10%	0.012%
78	29.820	4495	4498	4499	rBV3	1609	1694	0.21%	0.024%
79	30.107	4545	4547	4549	rVB3	1355	1156	0.14%	0.016%
80	30.131	4549	4551	4552	rBV2	1248	936	0.11%	0.013%
81	30.149	4552	4554	4555	rVB2	1454	943	0.12%	0.013%
82	30.730	4652	4653	4654	rBV	1612	851	0.10%	0.012%
83	31.083	4712	4713	4717	rBV4	1393	1588	0.19%	0.022%
84	31.523	4784	4788	4789	rBV4	1392	1908	0.23%	0.027%
85	31.659	4809	4811	4813	rBV3	1615	1284	0.16%	0.018%
86	32.099	4884	4886	4887	rVB2	1623	1127	0.14%	0.016%
87	32.123	4887	4890	4892	rBV4	1656	2092	0.26%	0.029%
88	32.252	4908	4912	4914	rBV5	1258	1624	0.20%	0.023%




Sum of corrected areas: 7106412

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053989.D
Acq On : 21 Jun 2022 22:36
Operator : CG/JU
Sample : PB145688BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK688

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

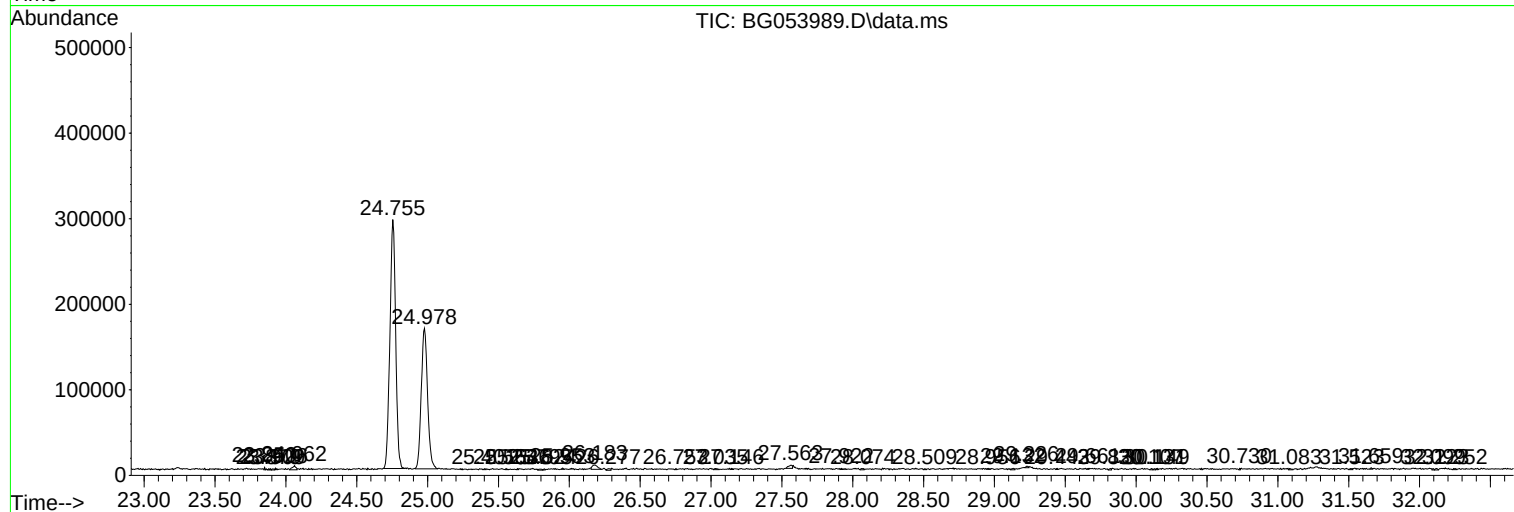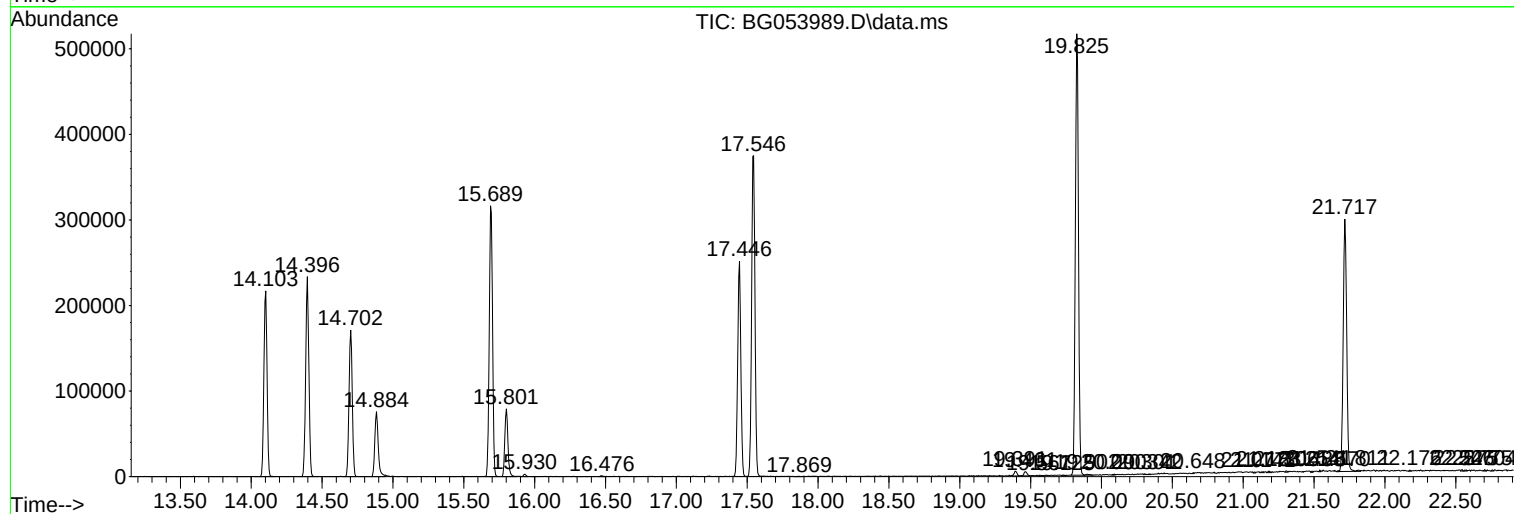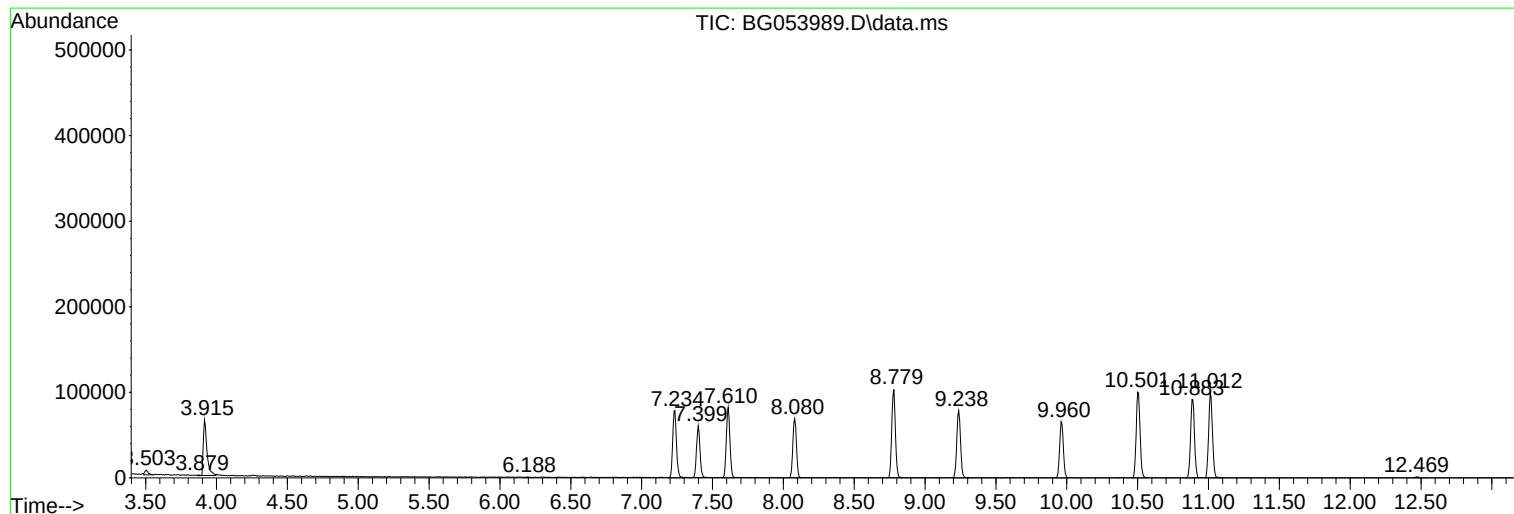

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053989.D
Acq On : 21 Jun 2022 22:36
Operator : CG/JU
Sample : PB145688BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK688

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053989.D
Acq On : 21 Jun 2022 22:36
Operator : CG/JU
Sample : PB145688BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK688

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc