

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053990.D
 Acq On : 21 Jun 2022 23:15
 Operator : CG/JU
 Sample : N3400-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.508	16	20	24	rBV3	3701	5367	0.67%	0.080%
2	3.919	87	90	103	rBV	19651	35101	4.39%	0.523%
3	4.260	145	148	155	rVB4	1351	2137	0.27%	0.032%
4	5.170	299	303	308	rBV3	975	1852	0.23%	0.028%
5	5.635	379	382	387	rBV2	709	1327	0.17%	0.020%
6	7.233	649	654	662	rVB2	16541	29756	3.72%	0.443%
7	7.397	676	682	690	rBV	49613	86754	10.84%	1.292%
8	7.462	690	693	698	rBV	1164	1710	0.21%	0.025%
9	7.609	712	718	727	rVB	55169	94756	11.84%	1.412%
10	8.079	791	798	807	rBV	69390	123855	15.48%	1.845%
11	8.778	911	917	927	rBB	45160	82791	10.35%	1.233%
12	9.236	988	995	1005	rBB	65793	122992	15.37%	1.832%
13	9.671	1065	1069	1074	rBB2	979	1431	0.18%	0.021%
14	9.965	1112	1119	1127	rBB	53709	97251	12.16%	1.449%
15	10.505	1204	1211	1222	rBV	82241	153698	19.21%	2.290%
16	10.887	1268	1276	1284	rBB	96571	178707	22.34%	2.662%
17	11.011	1291	1297	1307	rBV	72948	140031	17.50%	2.086%
18	12.468	1541	1545	1549	rBB2	1273	1982	0.25%	0.030%
19	14.101	1816	1823	1830	rBV	198361	291472	36.43%	4.342%
20	14.395	1866	1873	1881	rBV	202382	327671	40.96%	4.882%
21	14.700	1918	1925	1932	rBB	177719	279649	34.95%	4.166%
22	14.883	1952	1956	1969	rBB	12503	23159	2.89%	0.345%
23	15.435	2045	2050	2054	rBB	4783	6363	0.80%	0.095%
24	15.693	2087	2094	2102	rVB	299090	472366	59.04%	7.037%
25	15.799	2107	2112	2119	rBV	78761	123144	15.39%	1.835%
26	15.934	2129	2135	2138	rBB	2788	3643	0.46%	0.054%
27	16.475	2224	2227	2230	rBB	913	1040	0.13%	0.015%
28	17.227	2352	2355	2360	rBB	689	1195	0.15%	0.018%
29	17.444	2385	2392	2400	rBV	262943	403593	50.45%	6.013%
30	17.544	2402	2409	2422	rVB	372139	596350	74.54%	8.885%
31	18.331	2540	2543	2549	rBV2	15798	22570	2.82%	0.336%
32	19.342	2711	2715	2719	rBV	771	1102	0.14%	0.016%
33	19.395	2719	2724	2731	rVV3	5436	8763	1.10%	0.131%
34	19.459	2731	2735	2742	rBV	4903	8489	1.06%	0.126%
35	19.601	2754	2759	2767	rBV4	8105	13690	1.71%	0.204%
36	19.730	2778	2781	2782	rBV2	1320	1529	0.19%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053990.D
 Acq On : 21 Jun 2022 23:15
 Operator : CG/JU
 Sample : N3400-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.742	2782	2783	2789	rVV4	2338	3458	0.43%	0.052%
38	19.830	2791	2798	2808	rVV	520594	794638	99.33%	11.839%
39	19.912	2811	2812	2816	rBV	1048	1399	0.17%	0.021%
40	20.153	2851	2853	2854	rBV2	1241	1135	0.14%	0.017%
41	20.306	2877	2879	2880	rBV2	1405	1343	0.17%	0.020%
42	20.323	2880	2882	2883	rBV	1513	1120	0.14%	0.017%
43	20.423	2897	2899	2902	rBV4	1000	1404	0.18%	0.021%
44	20.452	2902	2904	2907	rVB4	1400	1168	0.15%	0.017%
45	20.494	2907	2911	2913	rBV5	2424	3641	0.46%	0.054%
46	20.541	2917	2919	2920	rBV2	1548	1207	0.15%	0.018%
47	20.570	2923	2924	2927	rVV3	1689	1010	0.13%	0.015%
48	20.787	2959	2961	2964	rVB4	1810	1948	0.24%	0.029%
49	20.823	2964	2967	2968	rBV3	1323	1414	0.18%	0.021%
50	20.846	2970	2971	2975	rVV4	3961	4390	0.55%	0.065%
51	20.887	2976	2978	2981	rVB4	1726	1543	0.19%	0.023%
52	21.052	3004	3006	3007	rBV2	1371	1244	0.16%	0.019%
53	21.357	3052	3058	3068	rBV	38815	72430	9.05%	1.079%
54	21.716	3113	3119	3128	rVB	295625	505093	63.13%	7.525%
55	22.192	3198	3200	3201	rBV2	2081	1534	0.19%	0.023%
56	22.227	3204	3206	3212	rVB5	5938	7914	0.99%	0.118%
57	22.380	3226	3232	3236	rBV5	10246	21755	2.72%	0.324%
58	22.521	3251	3256	3257	rBV3	6549	8989	1.12%	0.134%
59	22.662	3278	3280	3285	rBV4	3437	4612	0.58%	0.069%
60	22.709	3285	3288	3292	rVB4	6567	10058	1.26%	0.150%
61	22.891	3314	3319	3321	rBV5	4586	7268	0.91%	0.108%
62	23.114	3355	3357	3359	rBV3	1941	1795	0.22%	0.027%
63	23.237	3373	3378	3386	rVB2	17937	34910	4.36%	0.520%
64	23.878	3485	3487	3488	rBV2	1940	1870	0.23%	0.028%
65	23.919	3492	3494	3497	rVB4	2632	2625	0.33%	0.039%
66	24.060	3513	3518	3523	rVB4	8356	14618	1.83%	0.218%
67	24.442	3576	3583	3586	rBV7	6502	15797	1.97%	0.235%
68	24.612	3610	3612	3614	rBV3	1325	1030	0.13%	0.015%
69	24.753	3625	3636	3653	rVB2	282603	800027	100.00%	11.919%
70	24.977	3663	3674	3688	rVB2	172171	521585	65.20%	7.771%
71	26.005	3848	3849	3853	rBV4	1451	1582	0.20%	0.024%
72	26.175	3871	3878	3890	rVB5	11472	35718	4.46%	0.532%
73	26.404	3916	3917	3920	rBV3	2145	1766	0.22%	0.026%
74	26.469	3925	3928	3929	rBV3	1703	1309	0.16%	0.020%
75	26.492	3929	3932	3936	rBV6	1910	3019	0.38%	0.045%
76	26.845	3990	3992	3995	rBV4	1380	1415	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053990.D
 Acq On : 21 Jun 2022 23:15
 Operator : CG/JU
 Sample : N3400-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	27.051	4025	4027	4028	rBV2	2059	1315	0.16%	0.020%
78	27.186	4048	4050	4051	rBV2	1759	1205	0.15%	0.018%
79	27.203	4051	4053	4054	rBV2	1419	1111	0.14%	0.017%
80	27.568	4106	4115	4126	rBV9	7607	28786	3.60%	0.429%
81	27.668	4130	4132	4134	rBV2	1437	1564	0.20%	0.023%
82	27.891	4168	4170	4172	rVB2	1836	1238	0.15%	0.018%
83	28.226	4225	4227	4229	rBV3	1262	1023	0.13%	0.015%
84	28.690	4304	4306	4308	rBV2	1344	1226	0.15%	0.018%
85	28.931	4344	4347	4349	rBV4	1292	1575	0.20%	0.023%
86	29.025	4360	4363	4364	rVV3	1505	1246	0.16%	0.019%
87	29.360	4418	4420	4422	rVB3	1884	1338	0.17%	0.020%
88	29.759	4486	4488	4491	rVB3	1859	1466	0.18%	0.022%
89	30.194	4561	4562	4565	rVB3	1545	1029	0.13%	0.015%
90	30.347	4587	4588	4591	rVB3	1593	1091	0.14%	0.016%
91	30.376	4591	4593	4594	rBV2	1470	1104	0.14%	0.016%
92	30.805	4665	4666	4668	rBV2	1681	1356	0.17%	0.020%
93	30.846	4671	4673	4675	rVB3	1714	1063	0.13%	0.016%
94	30.975	4693	4695	4697	rBV3	1296	1153	0.14%	0.017%
95	31.246	4735	4741	4743	rBV6	3190	6349	0.79%	0.095%
96	31.457	4775	4777	4781	rBV4	1613	1852	0.23%	0.028%
97	31.751	4825	4827	4830	rBV2	1642	1542	0.19%	0.023%
98	31.810	4835	4837	4839	rVB2	1668	1356	0.17%	0.020%
99	32.203	4902	4904	4907	rBV2	1402	1451	0.18%	0.022%
100	32.303	4919	4921	4926	rBV4	1403	1729	0.22%	0.026%




Sum of corrected areas: 6712235

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053990.D
Acq On : 21 Jun 2022 23:15
Operator : CG/JU
Sample : N3400-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

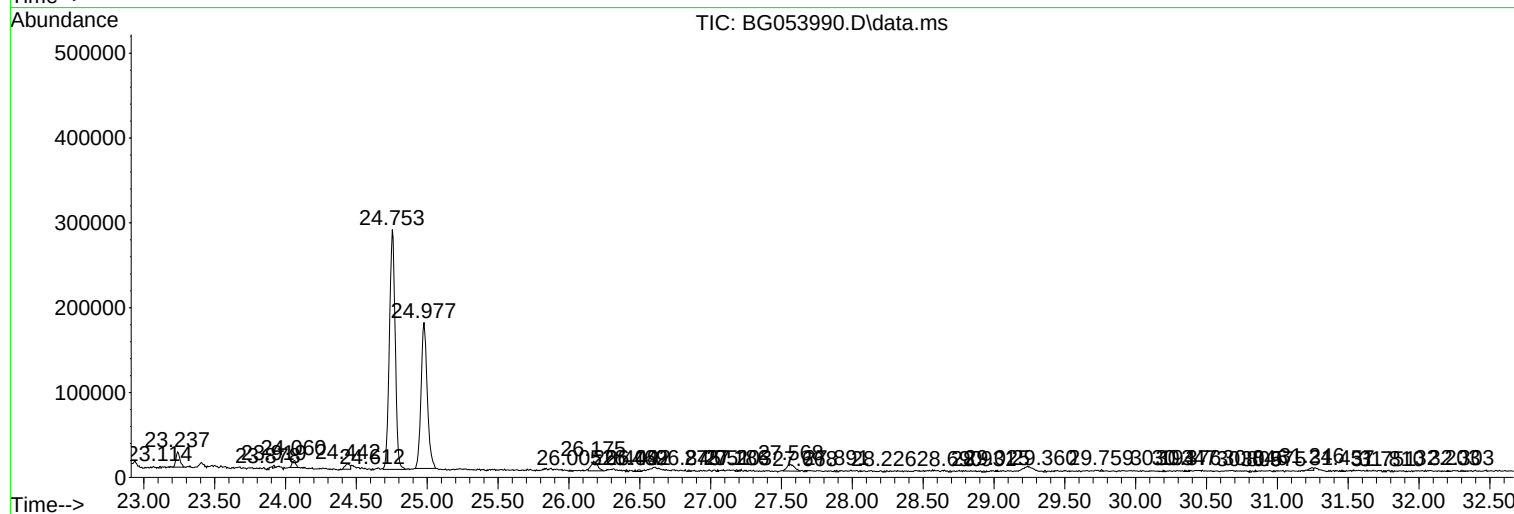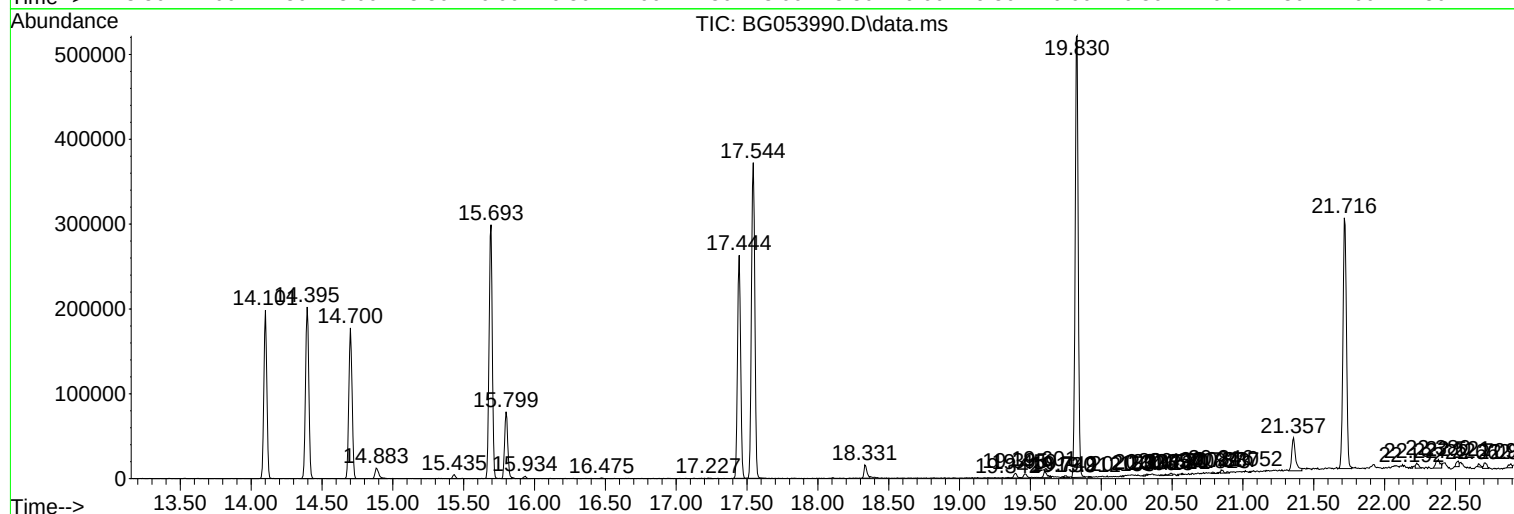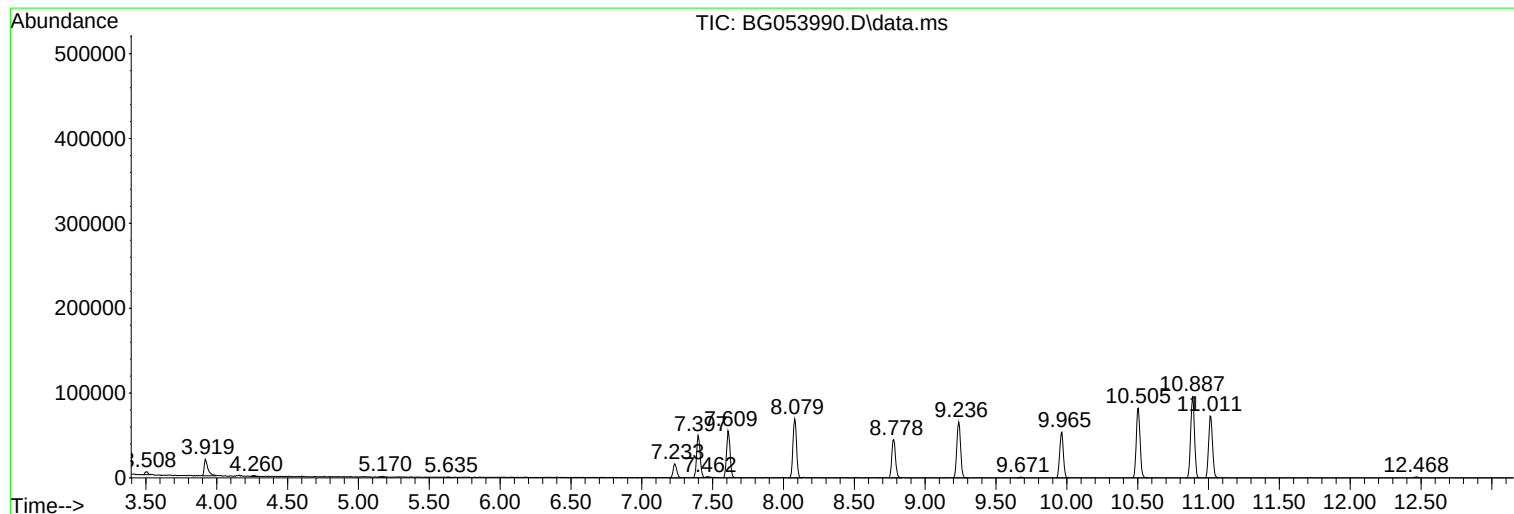

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053990.D
Acq On : 21 Jun 2022 23:15
Operator : CG/JU
Sample : N3400-03
Misc :
ALS Vial : 23 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.357	2.87 ng/ul	72430	Chrysene-d12	21.716	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Tricosene	322	C23H46	018835-32-0	94
2	Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	94
3	Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
4	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	93
5	Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91

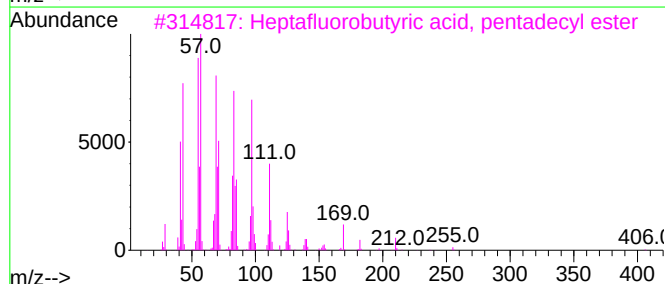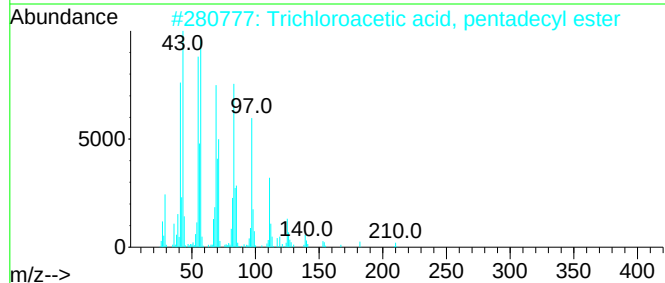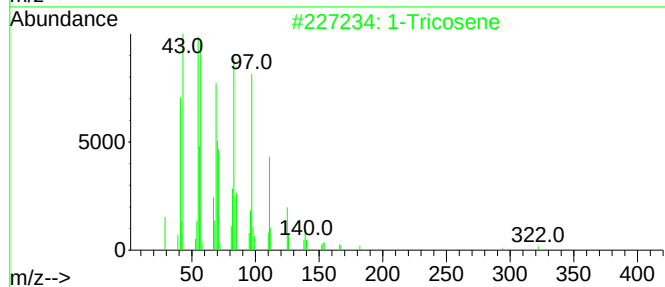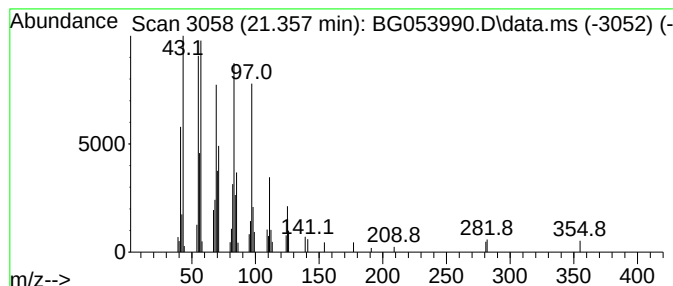

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053990.D
Acq On : 21 Jun 2022 23:15
Operator : CG/JU
Sample : N3400-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.357	2.9	ng/u1	72430	5	21.716	505093	20.0