

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053993.D
 Acq On : 22 Jun 2022 1:12
 Operator : CG/JU
 Sample : N3355-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EY0D3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.479	10	15	27	rVB5	11694	28249	3.11%	0.400%
2	3.896	82	86	88	rBV3	803	1018	0.11%	0.014%
3	3.926	88	91	102	rVB2	6025	10755	1.18%	0.152%
4	4.155	127	130	138	rVB3	1699	3247	0.36%	0.046%
5	4.255	143	147	152	rBV4	1070	1819	0.20%	0.026%
6	4.525	190	193	196	rBV3	735	1013	0.11%	0.014%
7	5.177	300	304	307	rVB3	1420	1909	0.21%	0.027%
8	7.234	644	654	661	rVV2	18509	33158	3.65%	0.470%
9	7.398	676	682	693	rBV	60124	107006	11.78%	1.515%
10	7.610	711	718	726	rBV	66022	114382	12.59%	1.620%
11	8.080	791	798	808	rVB	72019	123712	13.62%	1.752%
12	8.779	910	917	926	rBV	54147	96951	10.67%	1.373%
13	9.237	988	995	1005	rBV	82972	148737	16.37%	2.106%
14	9.966	1111	1119	1127	rBB	65106	120853	13.30%	1.712%
15	10.500	1204	1210	1222	rBV	97867	185360	20.40%	2.625%
16	10.888	1268	1276	1284	rBB	96651	177333	19.52%	2.511%
17	11.017	1291	1298	1309	rBB	57453	108284	11.92%	1.534%
18	12.469	1541	1545	1549	rBB2	1488	2117	0.23%	0.030%
19	13.597	1733	1737	1740	rBB	1487	1623	0.18%	0.023%
20	14.102	1816	1823	1831	rBV	223868	345499	38.03%	4.893%
21	14.396	1865	1873	1881	rBV	237694	385213	42.40%	5.455%
22	14.701	1918	1925	1932	rBB2	173196	277461	30.54%	3.929%
23	14.883	1952	1956	1966	rBV3	12297	22096	2.43%	0.313%
24	15.694	2086	2094	2103	rBB	341606	549560	60.48%	7.783%
25	15.800	2107	2112	2122	rVV	90651	138454	15.24%	1.961%
26	15.935	2130	2135	2138	rVB	3119	3844	0.42%	0.054%
27	17.445	2385	2392	2399	rVV	258910	393745	43.34%	5.576%
28	17.545	2401	2409	2419	rBV	416100	655369	72.13%	9.281%
29	18.332	2539	2543	2547	rBV2	3915	4863	0.54%	0.069%
30	19.390	2719	2723	2728	rBV3	6055	8667	0.95%	0.123%
31	19.460	2728	2735	2742	rBV2	5363	8690	0.96%	0.123%
32	19.607	2756	2760	2763	rBV5	2539	2702	0.30%	0.038%
33	19.748	2780	2784	2787	rBV5	1170	1405	0.15%	0.020%
34	19.825	2791	2797	2806	rBV	570783	874133	96.21%	12.379%
35	20.118	2842	2847	2851	rBV3	932	1408	0.15%	0.020%
36	20.201	2858	2861	2863	rVV3	1007	1408	0.15%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053993.D
 Acq On : 22 Jun 2022 1:12
 Operator : CG/JU
 Sample : N3355-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EY0D3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.224	2863	2865	2867	rVV2	1547	1520	0.17%	0.022%
38	20.424	2894	2899	2900	rBV3	879	1446	0.16%	0.020%
39	20.530	2913	2917	2920	rBV4	1329	2018	0.22%	0.029%
40	20.788	2959	2961	2966	rVB6	1748	1888	0.21%	0.027%
41	20.853	2971	2972	2976	rVV3	1583	1396	0.15%	0.020%
42	21.047	3003	3005	3007	rBV3	950	1008	0.11%	0.014%
43	21.323	3050	3052	3053	rBV2	1408	1157	0.13%	0.016%
44	21.358	3053	3058	3063	rVV7	7579	13378	1.47%	0.189%
45	21.605	3096	3100	3103	rVB5	1557	2629	0.29%	0.037%
46	21.640	3103	3106	3108	rBV2	1968	1810	0.20%	0.026%
47	21.717	3112	3119	3132	rVV2	307699	521256	57.37%	7.382%
48	22.533	3256	3258	3259	rBV2	1834	1211	0.13%	0.017%
49	22.745	3292	3294	3296	rBV3	1484	1179	0.13%	0.017%
50	23.238	3372	3378	3384	rVB5	5273	11622	1.28%	0.165%
51	23.620	3441	3443	3445	rBV3	1628	1321	0.15%	0.019%
52	24.061	3511	3518	3524	rBV2	7287	16311	1.80%	0.231%
53	24.202	3540	3542	3545	rBV3	1050	1067	0.12%	0.015%
54	24.331	3562	3564	3565	rBV2	1685	1498	0.16%	0.021%
55	24.507	3592	3594	3596	rBV2	1233	1282	0.14%	0.018%
56	24.754	3625	3636	3650	rBV2	313175	908594	100.00%	12.867%
57	24.977	3663	3674	3693	rVB	177929	541110	59.55%	7.663%
58	25.095	3693	3694	3696	rBV	1660	992	0.11%	0.014%
59	25.324	3731	3733	3735	rBV2	1175	1074	0.12%	0.015%
60	25.688	3794	3795	3797	rBV2	1448	1373	0.15%	0.019%
61	25.712	3797	3799	3802	rVB4	1860	1484	0.16%	0.021%
62	26.182	3873	3879	3889	rVB6	8405	24497	2.70%	0.347%
63	26.294	3895	3898	3901	rBV3	1251	1987	0.22%	0.028%
64	26.358	3907	3909	3910	rBV	1419	923	0.10%	0.013%
65	26.411	3916	3918	3920	rBV2	1208	910	0.10%	0.013%
66	26.764	3976	3978	3982	rBV4	1596	2034	0.22%	0.029%
67	26.799	3982	3984	3985	rBV2	1235	1039	0.11%	0.015%
68	27.563	4107	4114	4116	rBV6	6145	14747	1.62%	0.209%
69	27.874	4165	4167	4171	rBV4	1426	1750	0.19%	0.025%
70	27.986	4184	4186	4189	rBV4	1157	1325	0.15%	0.019%
71	28.556	4281	4283	4285	rBV3	1139	1159	0.13%	0.016%
72	28.732	4309	4313	4315	rBV4	1595	2441	0.27%	0.035%
73	28.791	4321	4323	4324	rBV2	1512	1272	0.14%	0.018%
74	28.943	4347	4349	4351	rBV3	1166	1017	0.11%	0.014%
75	29.126	4378	4380	4383	rBV3	1833	2064	0.23%	0.029%
76	29.155	4383	4385	4386	rBV	1186	1049	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053993.D
 Acq On : 22 Jun 2022 1:12
 Operator : CG/JU
 Sample : N3355-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EY0D3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	29.237	4393	4399	4400	rBV4	3244	5263	0.58%	0.075%
78	29.425	4428	4431	4434	rBV3	1807	2202	0.24%	0.031%
79	29.631	4464	4466	4467	rBV2	1206	913	0.10%	0.013%
80	29.795	4492	4494	4497	rBV4	1713	1433	0.16%	0.020%
81	30.118	4547	4549	4551	rVB3	1396	1179	0.13%	0.017%
82	30.148	4551	4554	4555	rBV3	1196	1273	0.14%	0.018%
83	30.271	4573	4575	4578	rBV4	1322	1580	0.17%	0.022%
84	30.700	4646	4648	4651	rVB3	1658	1453	0.16%	0.021%
85	31.628	4804	4806	4809	rVB2	1343	1073	0.12%	0.015%
86	31.764	4823	4829	4831	rBV3	1213	2116	0.23%	0.030%
87	31.922	4854	4856	4858	rBV3	1205	1032	0.11%	0.015%
88	32.275	4914	4916	4920	rBV4	1578	1819	0.20%	0.026%




Sum of corrected areas: 7061217

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053993.D
Acq On : 22 Jun 2022 1:12
Operator : CG/JU
Sample : N3355-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EY0D3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

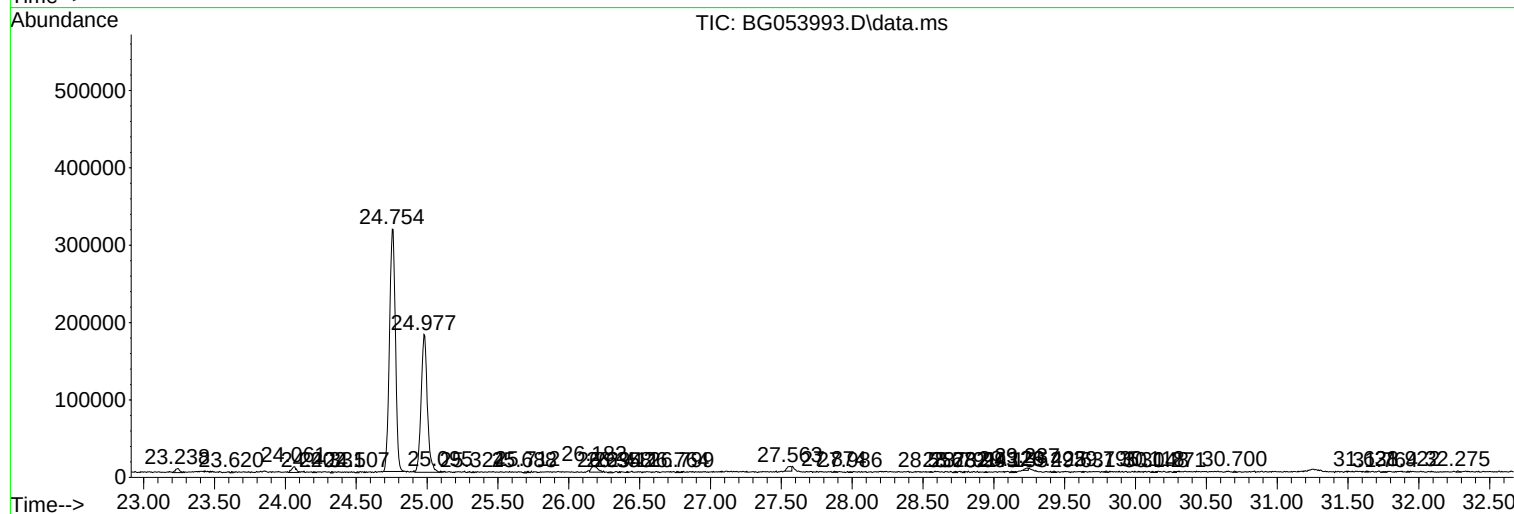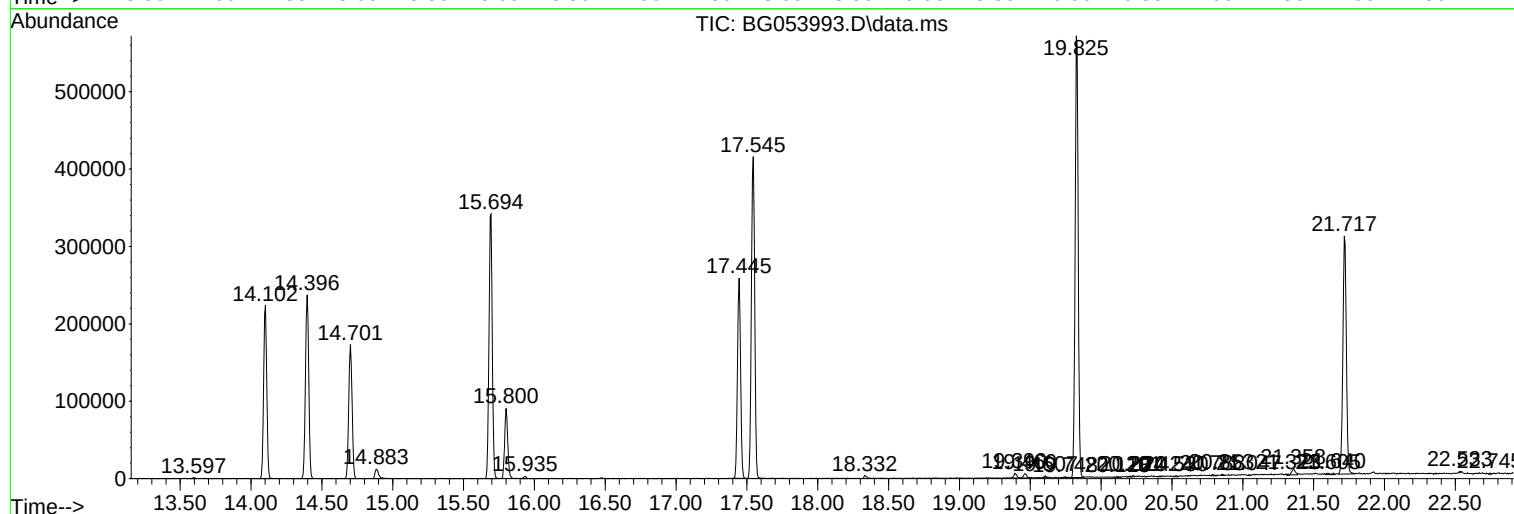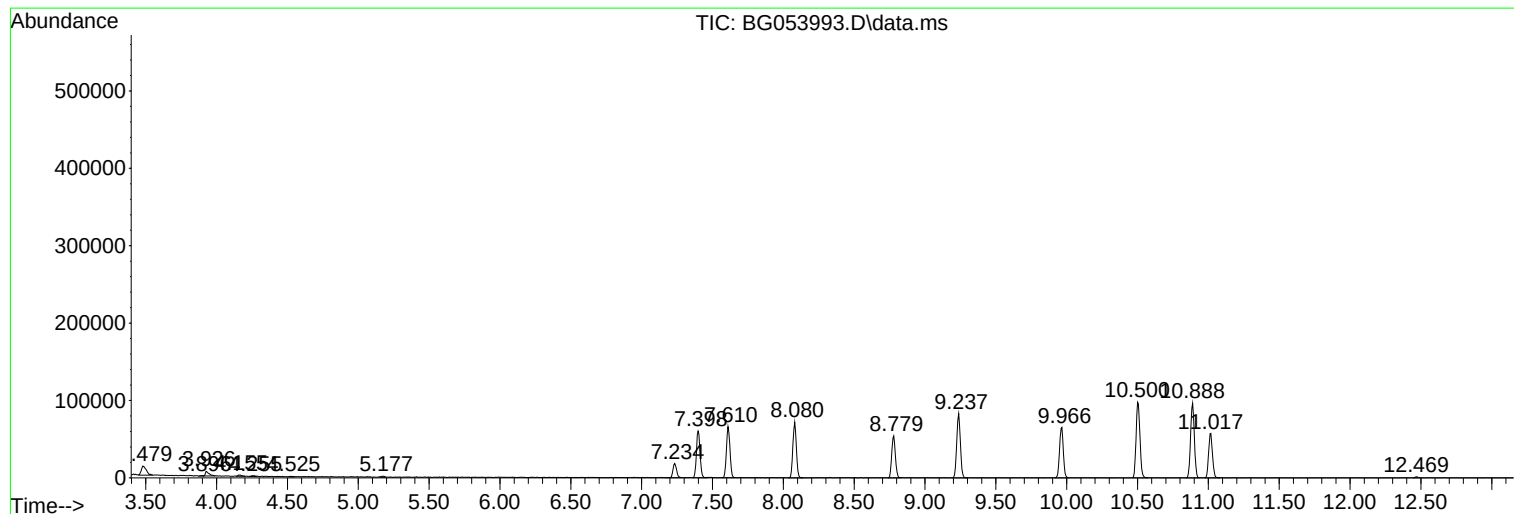

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053993.D
Acq On : 22 Jun 2022 1:12
Operator : CG/JU
Sample : N3355-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EY0D3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053993.D
Acq On : 22 Jun 2022 1:12
Operator : CG/JU
Sample : N3355-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EY0D3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc