

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053996.D
 Acq On : 22 Jun 2022 3:08
 Operator : CG/JU
 Sample : N3400-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.506	15	20	24	rVV	4320	6425	0.75%	0.086%
2	3.917	85	90	102	rBV	25103	45303	5.27%	0.606%
3	4.158	127	131	136	rVB4	1704	2588	0.30%	0.035%
4	4.258	145	148	153	rVB4	1481	2206	0.26%	0.030%
5	4.481	182	186	188	rVB3	1709	1529	0.18%	0.020%
6	7.237	648	655	661	rVV	17502	31887	3.71%	0.427%
7	7.396	675	682	690	rBV	58265	102956	11.98%	1.378%
8	7.460	690	693	699	rVV2	2007	3965	0.46%	0.053%
9	7.613	712	719	727	rBV2	62019	111958	13.03%	1.499%
10	8.077	792	798	807	rBV	75875	131316	15.29%	1.758%
11	8.776	910	917	926	rBB	56864	98027	11.41%	1.312%
12	9.235	988	995	1004	rBB	77822	144640	16.84%	1.936%
13	9.681	1066	1071	1074	rBB2	1402	2298	0.27%	0.031%
14	9.963	1113	1119	1126	rBV	61286	114702	13.35%	1.535%
15	10.504	1204	1211	1223	rBB	103835	187139	21.78%	2.505%
16	10.886	1269	1276	1284	rBB	102082	189668	22.08%	2.539%
17	11.015	1291	1298	1314	rBB	85569	160590	18.69%	2.149%
18	12.466	1541	1545	1550	rVB	1484	2153	0.25%	0.029%
19	13.530	1722	1726	1729	rBB2	1508	1689	0.20%	0.023%
20	14.099	1817	1823	1833	rBB	231910	349228	40.65%	4.674%
21	14.393	1866	1873	1881	rBV	236330	392059	45.64%	5.248%
22	14.699	1919	1925	1933	rBB	184855	300758	35.01%	4.026%
23	14.887	1952	1957	1969	rBB	12783	24079	2.80%	0.322%
24	15.692	2087	2094	2104	rBB	354616	554734	64.57%	7.425%
25	15.797	2107	2112	2121	rBV	87671	140430	16.35%	1.880%
26	15.927	2130	2134	2140	rBB2	3450	4807	0.56%	0.064%
27	16.467	2224	2226	2230	rBB2	869	1158	0.13%	0.015%
28	17.090	2324	2332	2336	rBB2	9089	11930	1.39%	0.160%
29	17.443	2384	2392	2399	rBV	270511	426938	49.70%	5.715%
30	17.543	2402	2409	2418	rVV	408344	643072	74.86%	8.607%
31	18.107	2502	2505	2508	rBV2	2171	2669	0.31%	0.036%
32	18.336	2540	2544	2554	rBV3	20747	32981	3.84%	0.441%
33	18.406	2554	2556	2559	rVB3	1426	1401	0.16%	0.019%
34	18.829	2622	2628	2631	rVB3	1212	1684	0.20%	0.023%
35	18.970	2648	2652	2654	rBV2	1467	1409	0.16%	0.019%
36	19.129	2674	2679	2681	rVB3	1038	1219	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053996.D
 Acq On : 22 Jun 2022 3:08
 Operator : CG/JU
 Sample : N3400-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	19.188	2688	2689	2693	rVB2	1413	1154	0.13%	0.015%
38	19.393	2719	2724	2728	rBV4	6277	9782	1.14%	0.131%
39	19.464	2731	2736	2741	rVV	5593	8581	1.00%	0.115%
40	19.605	2754	2760	2767	rBV2	9314	15861	1.85%	0.212%
41	19.740	2780	2783	2784	rBV2	1299	1141	0.13%	0.015%
42	19.828	2791	2798	2808	rBV	589884	854599	99.48%	11.439%
43	20.022	2826	2831	2832	rBV3	1356	1705	0.20%	0.023%
44	20.322	2878	2882	2886	rBV2	3848	6515	0.76%	0.087%
45	20.357	2886	2888	2892	rVV4	2599	3125	0.36%	0.042%
46	20.410	2896	2897	2900	rVV2	1409	1120	0.13%	0.015%
47	20.657	2936	2939	2941	rBV3	1379	1428	0.17%	0.019%
48	20.686	2942	2944	2946	rVV3	1512	1412	0.16%	0.019%
49	20.733	2949	2952	2955	rVB3	1331	2100	0.24%	0.028%
50	20.833	2967	2969	2970	rBV2	2136	1594	0.19%	0.021%
51	20.856	2970	2973	2976	rVB3	2238	2732	0.32%	0.037%
52	20.974	2990	2993	2998	rBV5	2588	3093	0.36%	0.041%
53	21.162	3023	3025	3027	rVV2	2158	1465	0.17%	0.020%
54	21.185	3027	3029	3032	rVV5	1710	1212	0.14%	0.016%
55	21.356	3052	3058	3067	rBV	91972	140284	16.33%	1.878%
56	21.720	3113	3120	3128	rBV	313451	526464	61.28%	7.047%
57	21.873	3145	3146	3148	rVB2	2653	1564	0.18%	0.021%
58	21.920	3148	3154	3160	rBV8	6773	14734	1.72%	0.197%
59	22.402	3235	3236	3240	rVB3	1949	1244	0.14%	0.017%
60	22.543	3253	3260	3266	rBV10	8425	21591	2.51%	0.289%
61	23.242	3374	3379	3387	rVB5	9460	17114	1.99%	0.229%
62	23.336	3393	3395	3396	rBV2	1744	1559	0.18%	0.021%
63	23.430	3408	3411	3412	rBV3	2627	2525	0.29%	0.034%
64	23.765	3466	3468	3470	rBV3	1339	1446	0.17%	0.019%
65	24.064	3512	3519	3524	rBV3	14243	33638	3.92%	0.450%
66	24.105	3524	3526	3527	rBV	2631	1867	0.22%	0.025%
67	24.264	3550	3553	3554	rBV3	1617	1456	0.17%	0.019%
68	24.323	3562	3563	3567	rBV3	1516	1683	0.20%	0.023%
69	24.758	3625	3637	3652	rVB	307616	859074	100.00%	11.499%
70	24.981	3664	3675	3691	rVB2	177628	554781	64.58%	7.426%
71	25.139	3700	3702	3704	rVB3	1617	1203	0.14%	0.016%
72	25.457	3754	3756	3758	rVB3	1867	1772	0.21%	0.024%
73	25.615	3781	3783	3784	rBV2	1488	1224	0.14%	0.016%
74	25.927	3835	3836	3842	rBV4	1359	2449	0.29%	0.033%
75	26.185	3871	3880	3889	rBV5	16978	49824	5.80%	0.667%
76	26.262	3891	3893	3895	rBV2	1818	2031	0.24%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG053996.D
 Acq On : 22 Jun 2022 3:08
 Operator : CG/JU
 Sample : N3400-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

77	26.303	3897	3900	3904	rVB6	3216	5647	0.66%	0.076%
78	26.473	3927	3929	3931	rBV3	1908	1197	0.14%	0.016%
79	26.691	3964	3966	3969	rVB4	1806	1503	0.17%	0.020%
80	26.779	3979	3981	3984	rBV3	1337	1727	0.20%	0.023%
81	26.902	4001	4002	4006	rBV3	1348	2025	0.24%	0.027%
82	27.137	4040	4042	4043	rBV	1427	1420	0.17%	0.019%
83	27.572	4109	4116	4129	rVB7	9222	28434	3.31%	0.381%
84	28.929	4345	4347	4349	rVB2	2006	1422	0.17%	0.019%
85	29.082	4372	4373	4376	rBV3	2450	2512	0.29%	0.034%
86	29.176	4387	4389	4391	rBV3	1613	1578	0.18%	0.021%
87	29.235	4391	4399	4400	rBV8	6852	13861	1.61%	0.186%
88	29.382	4422	4424	4425	rBV2	1372	1149	0.13%	0.015%
89	29.446	4433	4435	4437	rBV3	1322	1097	0.13%	0.015%
90	29.552	4452	4453	4455	rBV2	1664	1327	0.15%	0.018%
91	30.451	4604	4606	4608	rBV2	2162	1280	0.15%	0.017%
92	30.598	4629	4631	4633	rBV3	1390	1349	0.16%	0.018%
93	31.162	4725	4727	4729	rBV3	1254	1336	0.16%	0.018%
94	31.526	4787	4789	4790	rVB2	2028	1190	0.14%	0.016%
95	31.550	4790	4793	4794	rBV3	1442	1550	0.18%	0.021%
96	31.879	4846	4849	4852	rVB3	1818	2321	0.27%	0.031%
97	32.090	4883	4885	4886	rBV	2088	1455	0.17%	0.019%
98	32.261	4912	4914	4915	rVB2	2496	1282	0.15%	0.017%
99	32.390	4934	4936	4939	rVB4	1427	1190	0.14%	0.016%
100	32.613	4971	4974	4977	rBV4	2192	3491	0.41%	0.047%




Sum of corrected areas: 7471084

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053996.D
Acq On : 22 Jun 2022 3:08
Operator : CG/JU
Sample : N3400-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

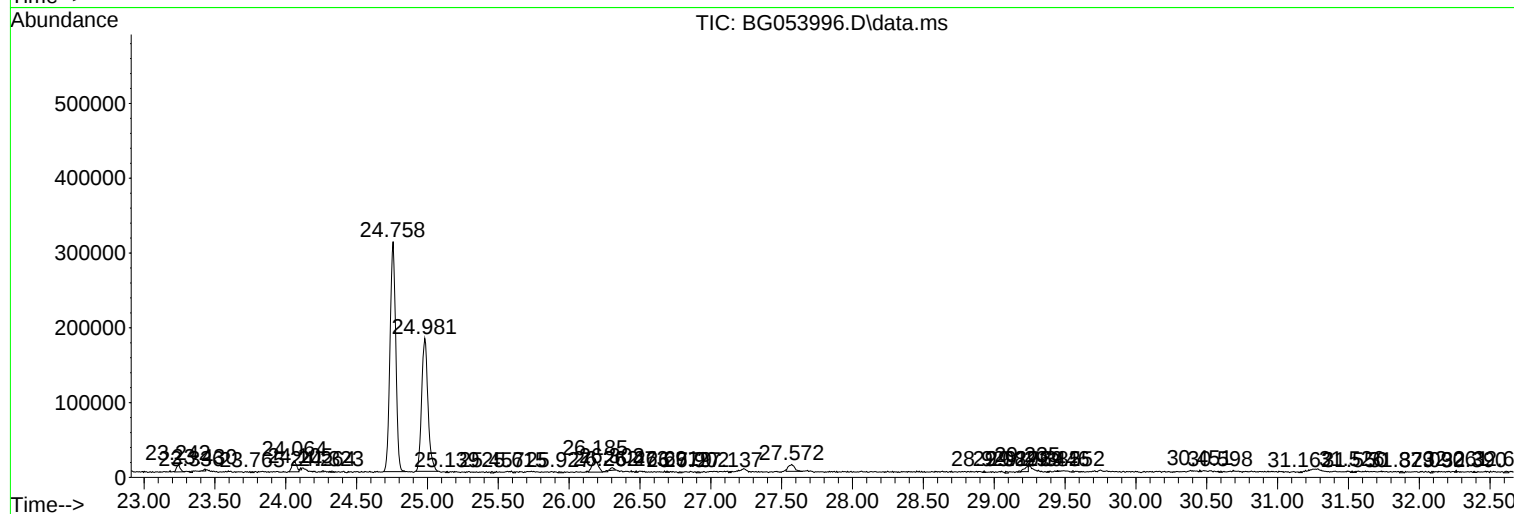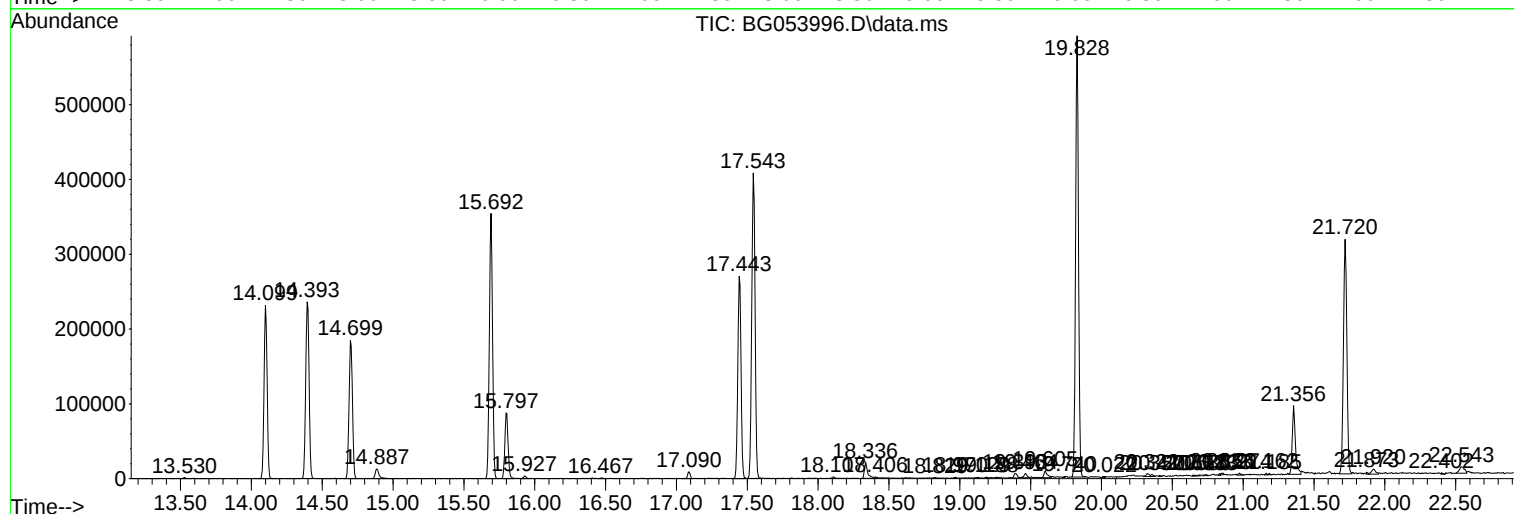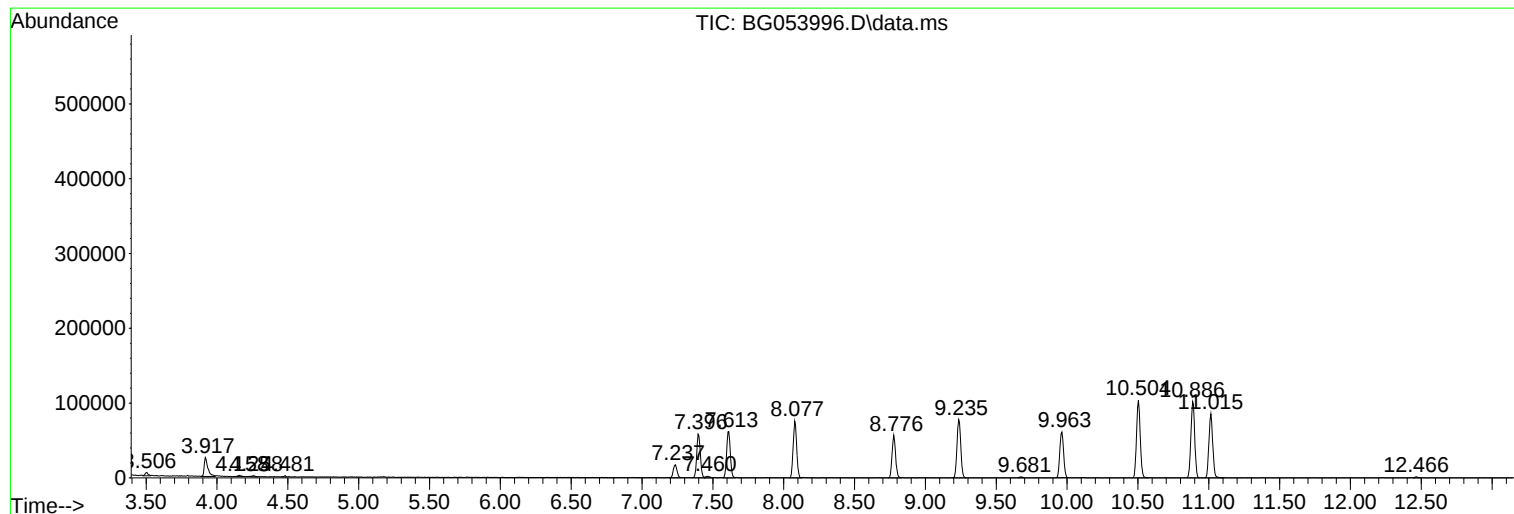

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053996.D
Acq On : 22 Jun 2022 3:08
Operator : CG/JU
Sample : N3400-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.356	5.33 ng/ul	140284	Chrysene-d12	21.720

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
2			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
3			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
4			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	94
5			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94

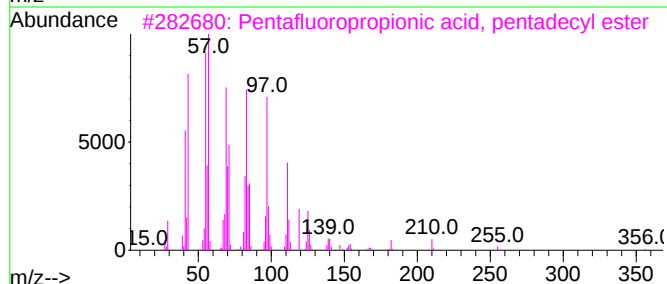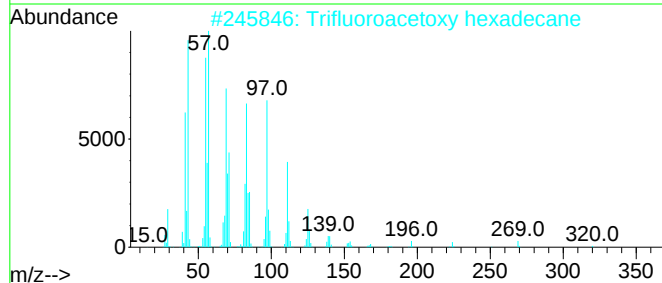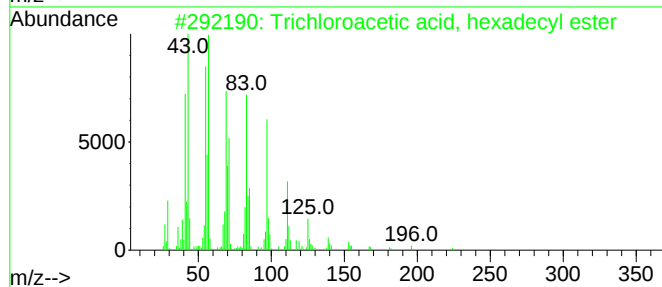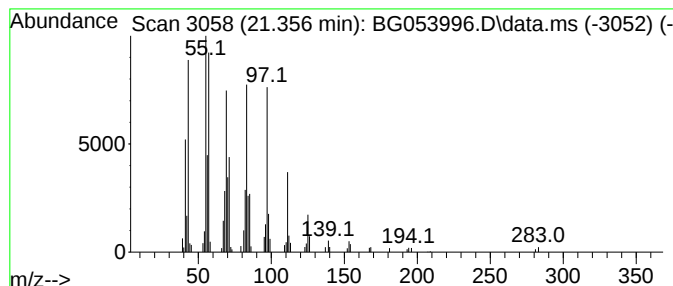

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG053996.D
Acq On : 22 Jun 2022 3:08
Operator : CG/JU
Sample : N3400-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.356	5.3	ng/ul	140284	5	21.720	526464	20.0