

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG054002.D
 Acq On : 22 Jun 2022 8:46
 Operator : CG/JU
 Sample : PB145728BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK728

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.499	16	19	27	rBV2	5163	7271	0.90%	0.106%
2	3.910	86	89	108	rBV	61520	114214	14.10%	1.671%
3	4.251	144	147	151	rBV4	1086	1454	0.18%	0.021%
4	7.230	648	654	665	rBV	76944	137674	17.00%	2.014%
5	7.395	676	682	692	rVB	56890	102202	12.62%	1.495%
6	7.606	712	718	728	rBV	75832	136182	16.81%	1.992%
7	8.076	791	798	807	rVB	65926	120881	14.92%	1.768%
8	8.775	911	917	925	rBV	97708	173143	21.38%	2.532%
9	9.234	988	995	1004	rBV	71522	135604	16.74%	1.983%
10	9.962	1112	1119	1128	rVB	61383	111073	13.71%	1.625%
11	10.503	1204	1211	1220	rBV	98387	179714	22.19%	2.629%
12	10.885	1269	1276	1285	rBB	92057	170453	21.05%	2.493%
13	11.014	1291	1298	1308	rBV	93011	174290	21.52%	2.549%
14	12.471	1541	1546	1550	rBB	1135	1649	0.20%	0.024%
15	14.104	1817	1824	1831	rBV	198798	308036	38.03%	4.506%
16	14.398	1867	1874	1882	rBV	214090	343496	42.41%	5.024%
17	14.704	1917	1926	1935	rBB	165016	267075	32.98%	3.906%
18	14.886	1951	1957	1968	rBV	75856	127285	15.72%	1.862%
19	15.691	2088	2094	2102	rVB	294577	474850	58.63%	6.945%
20	15.802	2107	2113	2125	rBV	75419	117710	14.53%	1.722%
21	15.932	2131	2135	2139	rVB3	2757	3932	0.49%	0.058%
22	16.478	2224	2228	2231	rBB	894	1081	0.13%	0.016%
23	17.230	2353	2356	2361	rBV	705	1146	0.14%	0.017%
24	17.448	2386	2393	2401	rBV	248301	382604	47.24%	5.596%
25	17.547	2402	2410	2423	rVV2	381163	597286	73.75%	8.736%
26	19.040	2662	2664	2667	rBV2	647	837	0.10%	0.012%
27	19.157	2680	2684	2687	rBV3	752	1024	0.13%	0.015%
28	19.392	2720	2724	2728	rVB3	5799	7926	0.98%	0.116%
29	19.463	2731	2736	2741	rBV	4290	6998	0.86%	0.102%
30	19.663	2767	2770	2773	rBV4	876	1084	0.13%	0.016%
31	19.827	2790	2798	2809	rBV	515033	784968	96.92%	11.481%
32	20.044	2833	2835	2838	rBV3	737	825	0.10%	0.012%
33	20.138	2849	2851	2854	rBV2	860	1257	0.16%	0.018%
34	20.215	2854	2864	2865	rBV3	3574	7599	0.94%	0.111%
35	20.321	2881	2882	2885	rVV3	1146	819	0.10%	0.012%
36	20.638	2934	2936	2940	rBV4	801	1341	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG054002.D
 Acq On : 22 Jun 2022 8:46
 Operator : CG/JU
 Sample : PB145728BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK728

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.726	2949	2951	2953	rBV2	1238	924	0.11%	0.014%
38	20.861	2972	2974	2975	rBV2	886	839	0.10%	0.012%
39	20.891	2977	2979	2983	rBV4	1025	1387	0.17%	0.020%
40	21.037	3001	3004	3006	rBV3	1078	998	0.12%	0.015%
41	21.120	3016	3018	3020	rBV2	1235	1233	0.15%	0.018%
42	21.372	3060	3061	3065	rVB4	1260	1196	0.15%	0.017%
43	21.719	3113	3120	3129	rBV2	281963	477017	58.90%	6.977%
44	22.207	3201	3203	3205	rBV2	1195	1222	0.15%	0.018%
45	22.365	3226	3230	3232	rBV3	1426	2246	0.28%	0.033%
46	22.424	3238	3240	3243	rBV2	1466	1815	0.22%	0.027%
47	22.600	3268	3270	3274	rVB5	1215	1228	0.15%	0.018%
48	22.712	3288	3289	3291	rBV2	1788	1354	0.17%	0.020%
49	22.847	3310	3312	3314	rBV2	1364	1342	0.17%	0.020%
50	22.882	3316	3318	3319	rVB2	1788	831	0.10%	0.012%
51	23.370	3399	3401	3403	rBV3	2165	1625	0.20%	0.024%
52	23.629	3443	3445	3447	rBV3	1248	1250	0.15%	0.018%
53	23.934	3495	3497	3498	rBV2	1548	1160	0.14%	0.017%
54	24.063	3516	3519	3525	rVB5	2392	4642	0.57%	0.068%
55	24.140	3530	3532	3534	rBV3	1576	1448	0.18%	0.021%
56	24.433	3579	3582	3583	rBV3	1747	1512	0.19%	0.022%
57	24.762	3626	3638	3651	rBV2	278939	809923	100.00%	11.846%
58	24.980	3663	3675	3690	rBV2	159465	484599	59.83%	7.088%
59	25.221	3714	3716	3718	rBV2	1613	1537	0.19%	0.022%
60	26.173	3875	3878	3879	rBV3	2666	3177	0.39%	0.046%
61	26.413	3917	3919	3923	rVB4	1323	959	0.12%	0.014%
62	26.507	3933	3935	3937	rBV3	1209	1086	0.13%	0.016%
63	26.543	3939	3941	3942	rBV2	1462	832	0.10%	0.012%
64	27.083	4032	4033	4036	rBV3	1737	1632	0.20%	0.024%
65	27.201	4051	4053	4055	rBV2	2027	1537	0.19%	0.022%
66	27.383	4082	4084	4086	rBV2	1150	1274	0.16%	0.019%
67	27.559	4112	4114	4115	rBV2	2482	1940	0.24%	0.028%
68	28.464	4266	4268	4270	rBV3	1564	1617	0.20%	0.024%
69	28.582	4286	4288	4289	rBV2	1340	1053	0.13%	0.015%
70	28.658	4299	4301	4302	rBV2	1100	939	0.12%	0.014%
71	28.752	4315	4317	4319	rBV2	1217	1391	0.17%	0.020%
72	29.228	4395	4398	4400	rBV3	1969	2794	0.34%	0.041%
73	29.939	4517	4519	4521	rBV2	1452	1156	0.14%	0.017%
74	30.021	4531	4533	4535	rBV3	1238	1377	0.17%	0.020%
75	30.820	4668	4669	4671	rBV2	1334	1150	0.14%	0.017%
76	30.879	4677	4679	4682	rBV3	1648	1273	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG054002.D
Acq On : 22 Jun 2022 8:46
Operator : CG/JU
Sample : PB145728BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK728

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Title : SVOA CALIBRATION

77	31.190	4730	4732	4733	rBV2	1440	1288	0.16%	0.019%
78	31.478	4779	4781	4783	rVB3	1526	998	0.12%	0.015%
79	31.625	4804	4806	4808	rBV3	1517	1167	0.14%	0.017%
80	31.931	4855	4858	4860	rBV4	1235	1909	0.24%	0.028%




Sum of corrected areas: 6836860

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG054002.D
Acq On : 22 Jun 2022 8:46
Operator : CG/JU
Sample : PB145728BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK728

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

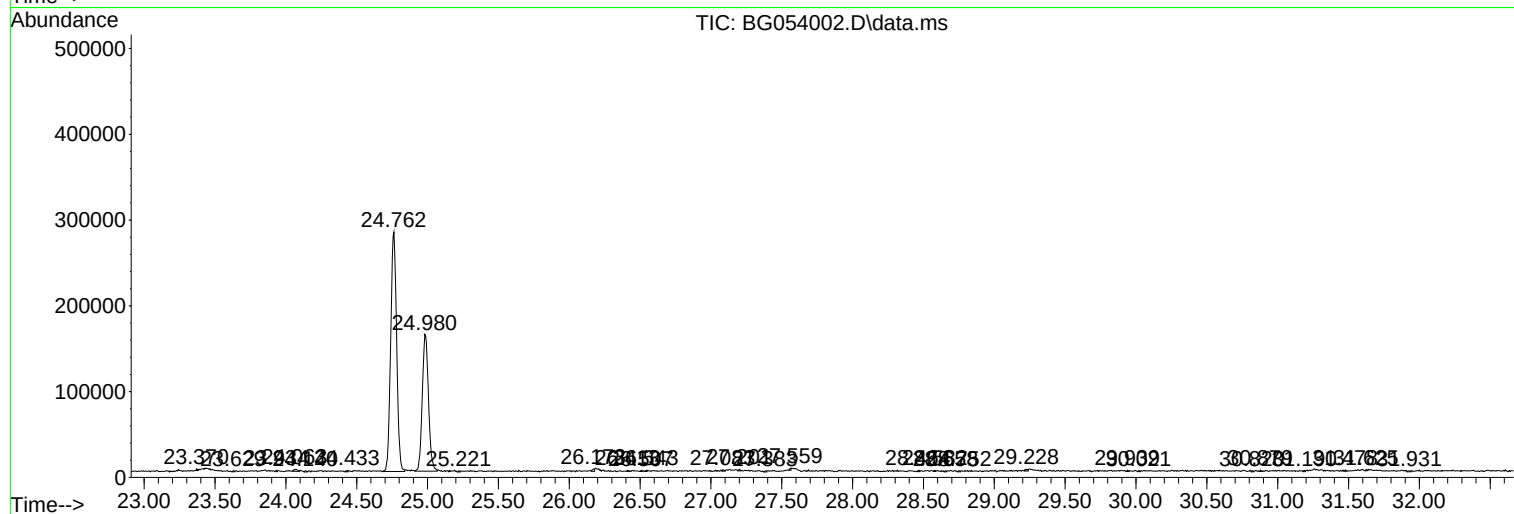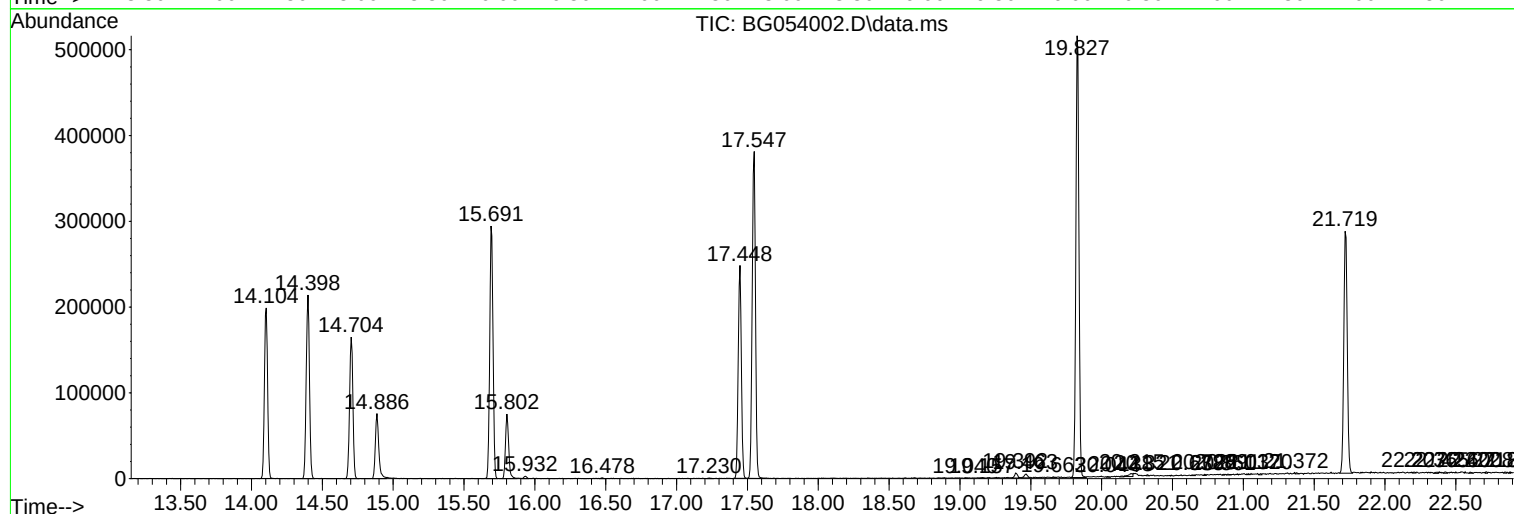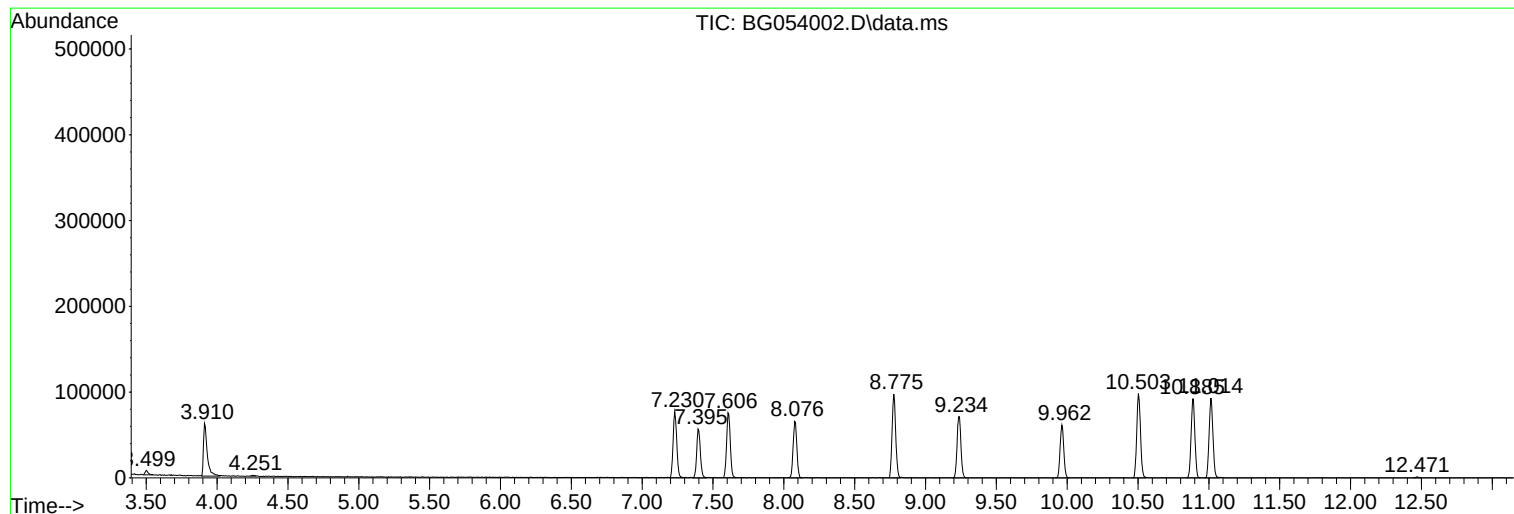

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG054002.D
Acq On : 22 Jun 2022 8:46
Operator : CG/JU
Sample : PB145728BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK728

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG054002.D
Acq On : 22 Jun 2022 8:46
Operator : CG/JU
Sample : PB145728BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK728

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------