

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG054011.D
 Acq On : 22 Jun 2022 14:52
 Operator : CG/JU
 Sample : N3319-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR-06-061022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

Signal : TIC: BG054011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	16	20	25	rBV3	3543	4984	0.46%	0.067%
2	3.916	87	90	108	rBV	36586	67514	6.20%	0.913%
3	4.163	127	132	136	rVB2	1880	3137	0.29%	0.042%
4	4.257	144	148	154	rVB2	2244	3277	0.30%	0.044%
5	4.533	192	195	198	rBV3	926	1296	0.12%	0.018%
6	5.174	300	304	309	rVB4	1151	1723	0.16%	0.023%
7	5.779	402	407	410	rBV3	768	1129	0.10%	0.015%
8	7.236	647	655	663	rBV2	14168	25650	2.36%	0.347%
9	7.400	676	683	691	rBV	71165	127192	11.69%	1.721%
10	7.612	714	719	725	rBV2	13587	23340	2.14%	0.316%
11	8.082	789	799	806	rBV	69369	123099	11.31%	1.665%
12	8.135	806	808	813	rVB2	1002	1360	0.12%	0.018%
13	8.781	912	918	928	rVB2	19437	34514	3.17%	0.467%
14	9.234	988	995	1008	rBB	94009	178459	16.40%	2.414%
15	9.968	1114	1120	1126	rBB2	9313	16467	1.51%	0.223%
16	10.503	1206	1211	1220	rBB	17396	30689	2.82%	0.415%
17	10.885	1268	1276	1286	rBB	95493	181180	16.65%	2.451%
18	11.014	1291	1298	1306	rBV	116629	224332	20.61%	3.035%
19	12.465	1541	1545	1547	rBV	1360	1882	0.17%	0.025%
20	14.098	1816	1823	1830	rBV	261252	406562	37.36%	5.500%
21	14.398	1866	1874	1882	rBV	275909	455794	41.88%	6.166%
22	14.704	1919	1926	1933	rBB	171746	281365	25.85%	3.806%
23	14.898	1954	1959	1968	rBV2	6030	13087	1.20%	0.177%
24	15.432	2045	2050	2055	rBV	2323	2870	0.26%	0.039%
25	15.691	2087	2094	2105	rVB	411222	652813	59.98%	8.831%
26	15.802	2108	2113	2118	rBV2	6688	10431	0.96%	0.141%
27	15.932	2129	2135	2139	rBB2	3715	5326	0.49%	0.072%
28	16.472	2224	2227	2230	rBB2	1403	1671	0.15%	0.023%
29	17.442	2386	2392	2403	rVB	246265	395061	36.30%	5.345%
30	17.541	2403	2409	2420	rVV2	527001	839647	77.15%	11.359%
31	17.718	2436	2439	2444	rVB2	1626	2348	0.22%	0.032%
32	18.405	2552	2556	2559	rVB2	1038	1222	0.11%	0.017%
33	19.398	2719	2725	2728	rBV4	6819	10327	0.95%	0.140%
34	19.463	2730	2736	2741	rVV	6119	9182	0.84%	0.124%
35	19.827	2791	2798	2805	rBV	692928	1055119	96.95%	14.274%
36	20.185	2857	2859	2860	rVV2	1676	1241	0.11%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
 Data File : BG054011.D
 Acq On : 22 Jun 2022 14:52
 Operator : CG/JU
 Sample : N3319-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR-06-061022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Title : SVOA CALIBRATION

37	20.215	2860	2864	2868	rVV4	1751	3427	0.31%	0.046%
38	20.244	2868	2869	2874	rVB2	1376	1641	0.15%	0.022%
39	20.738	2951	2953	2956	rVB3	1263	1125	0.10%	0.015%
40	20.802	2961	2964	2966	rBV3	1068	1495	0.14%	0.020%
41	20.838	2968	2970	2972	rBV2	1089	1177	0.11%	0.016%
42	21.278	3043	3045	3046	rBV2	1628	1459	0.13%	0.020%
43	21.355	3054	3058	3062	rBV3	10413	16209	1.49%	0.219%
44	21.601	3098	3100	3103	rVB4	1432	1139	0.10%	0.015%
45	21.719	3112	3120	3130	rBV2	287305	490358	45.06%	6.634%
46	21.854	3141	3143	3145	rBV2	1565	1190	0.11%	0.016%
47	21.919	3152	3154	3158	rBV3	2000	2068	0.19%	0.028%
48	22.530	3255	3258	3265	rVB8	3283	6047	0.56%	0.082%
49	22.694	3284	3286	3290	rVB3	2155	1971	0.18%	0.027%
50	22.724	3290	3291	3294	rBV3	1619	1990	0.18%	0.027%
51	23.241	3376	3379	3383	rBV4	3105	4898	0.45%	0.066%
52	23.294	3386	3388	3390	rBV2	1342	1262	0.12%	0.017%
53	23.423	3408	3410	3411	rBV2	2667	1890	0.17%	0.026%
54	24.052	3514	3517	3525	rVB5	5734	11498	1.06%	0.156%
55	24.757	3626	3637	3649	rBV2	380561	1088340	100.00%	14.723%
56	24.980	3664	3675	3690	rVB2	170223	498532	45.81%	6.744%
57	25.209	3712	3714	3717	rBV3	1394	1225	0.11%	0.017%
58	25.279	3724	3726	3729	rBV4	1773	1682	0.15%	0.023%
59	25.421	3748	3750	3751	rBV2	1977	1814	0.17%	0.025%
60	26.178	3874	3879	3887	rVB7	7099	21144	1.94%	0.286%
61	27.171	4046	4048	4049	rBV2	1723	1126	0.10%	0.015%
62	27.565	4110	4115	4122	rVB8	5087	13332	1.22%	0.180%
63	28.540	4279	4281	4283	rBV3	1759	1784	0.16%	0.024%
64	29.187	4389	4391	4392	rBV2	2688	1630	0.15%	0.022%
65	29.234	4393	4399	4400	rVV5	3587	6092	0.56%	0.082%
66	30.033	4533	4535	4537	rBV3	1335	1265	0.12%	0.017%
67	30.620	4633	4635	4638	rBV3	1702	2499	0.23%	0.034%
68	31.231	4737	4739	4740	rBV2	1679	1266	0.12%	0.017%
69	31.813	4835	4838	4840	rBV4	2012	2704	0.25%	0.037%
70	32.072	4881	4882	4885	rVB3	2226	1332	0.12%	0.018%




Sum of corrected areas: 7391901

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG054011.D
Acq On : 22 Jun 2022 14:52
Operator : CG/JU
Sample : N3319-01
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-06-061022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

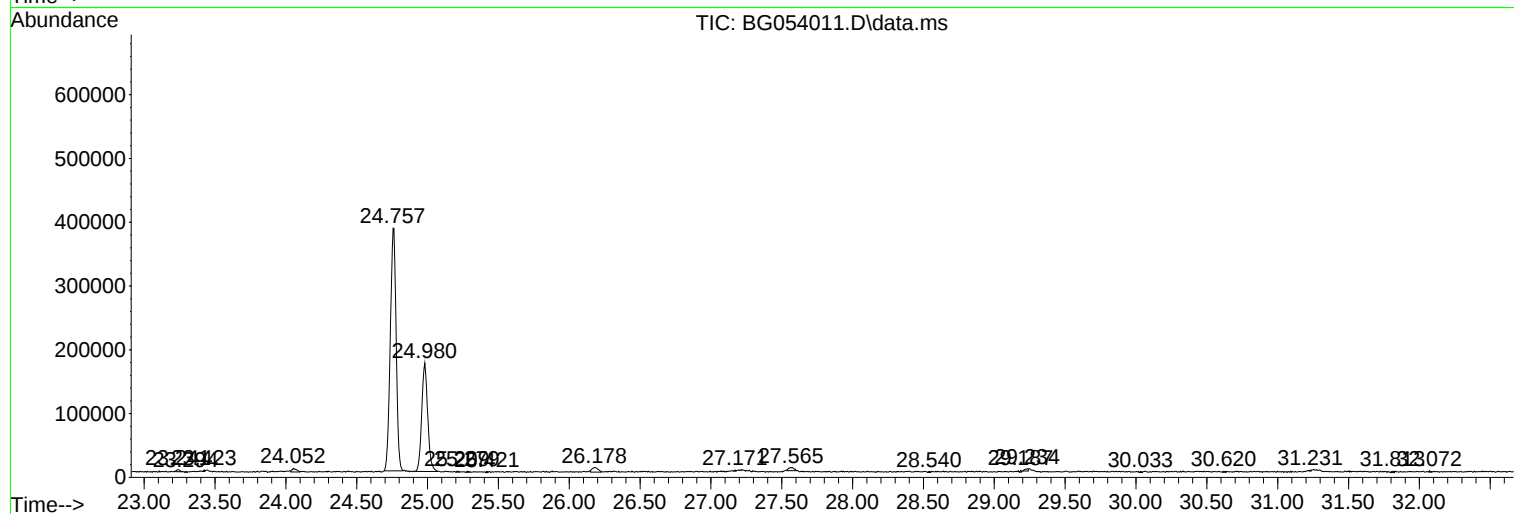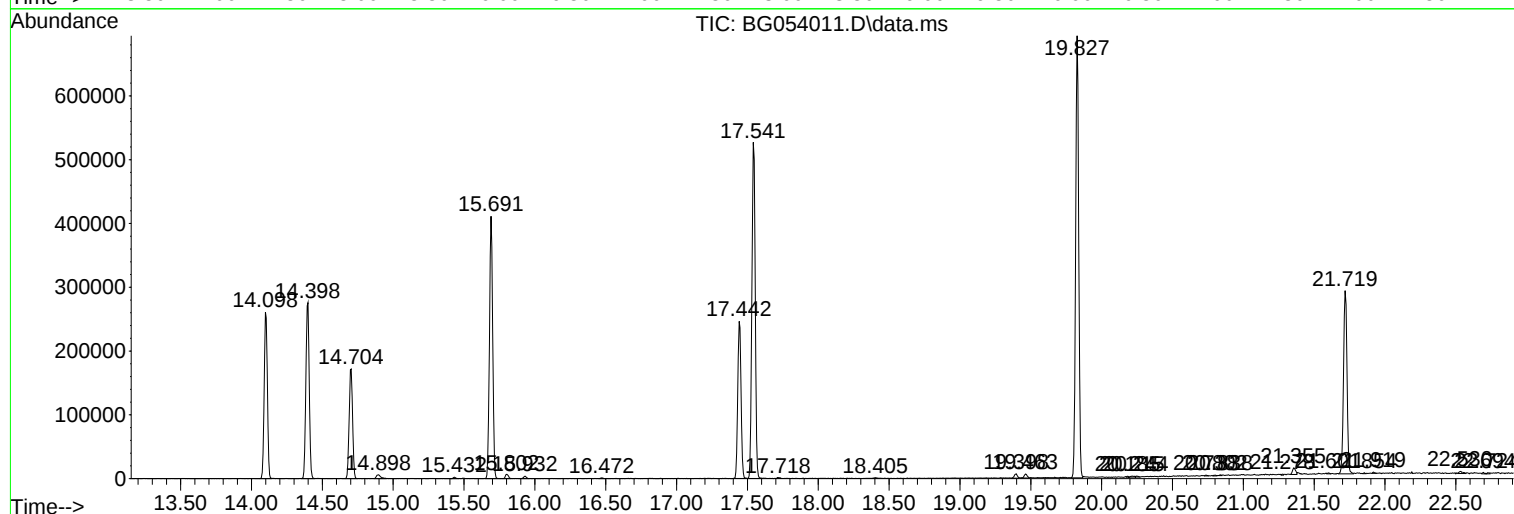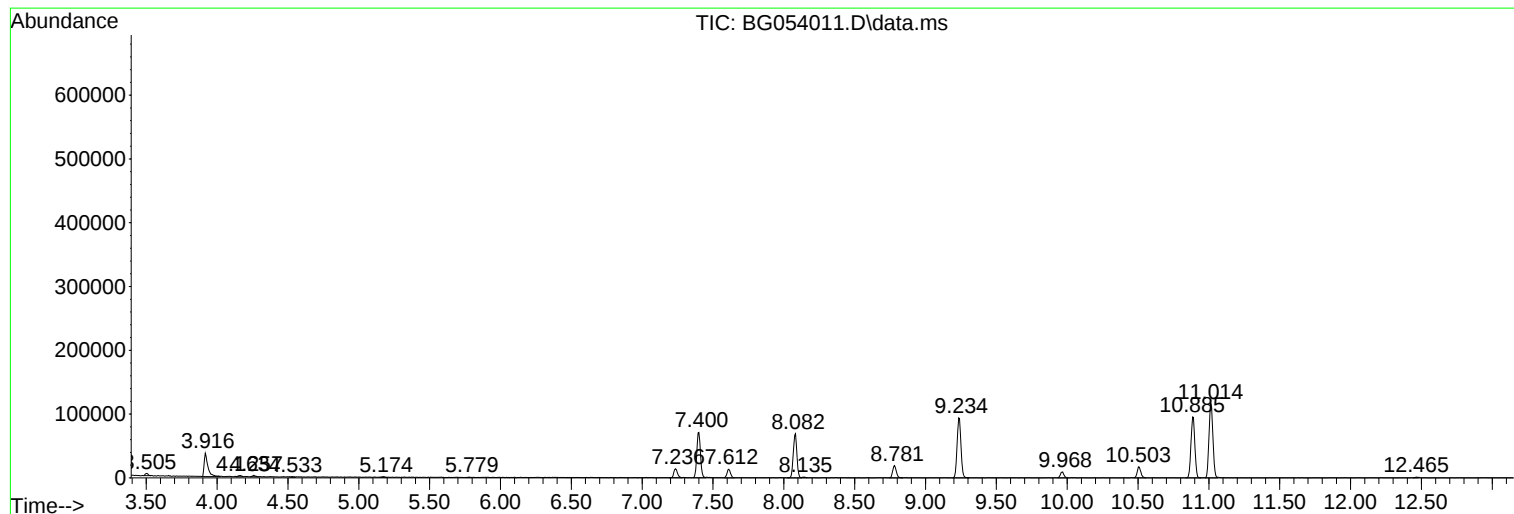

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG054011.D
Acq On : 22 Jun 2022 14:52
Operator : CG/JU
Sample : N3319-01
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-06-061022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062122\
Data File : BG054011.D
Acq On : 22 Jun 2022 14:52
Operator : CG/JU
Sample : N3319-01
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR-06-061022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------