
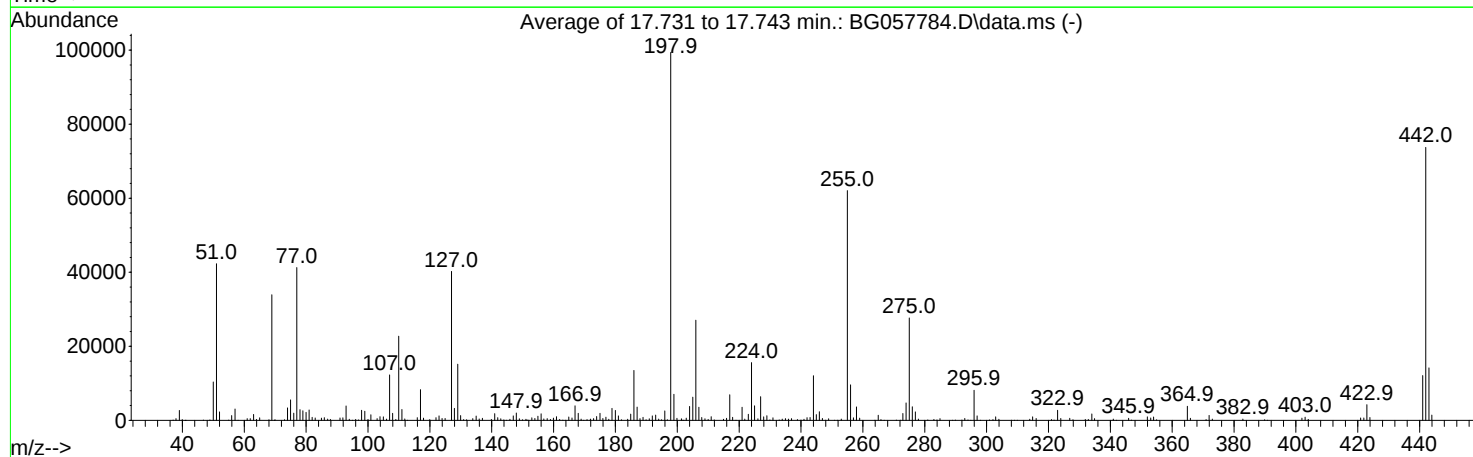


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062123\
Data File : BG057784.D
Acq On : 21 Jun 2023 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 20 03:40:38 2023

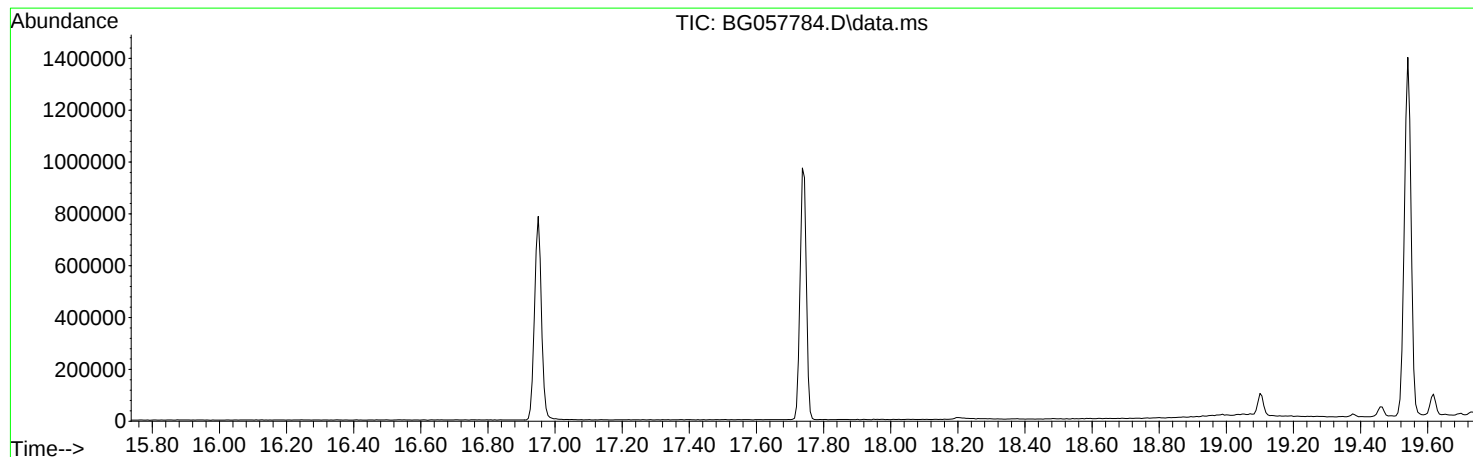




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	42312	PASS
68	69	0.00	2	0.5	176	PASS
69	198	0.00	100	34.1	33915	PASS
70	69	0.00	2	0.5	165	PASS
127	198	10	80	40.5	40232	PASS
197	198	0.00	2	0.2	185	PASS
198	198	100	100	100.0	99357	PASS
199	198	5	9	7.1	7027	PASS
275	198	10	60	27.8	27659	PASS
365	198	1	100	3.8	3790	PASS
441	198	0.01	100	12.2	12091	PASS
442	442	50	100	100.0	73736	PASS
443	442	15	24	19.2	14178	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062123\
Data File : BG057784.D
Acq On : 21 Jun 2023 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 22 06:21:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

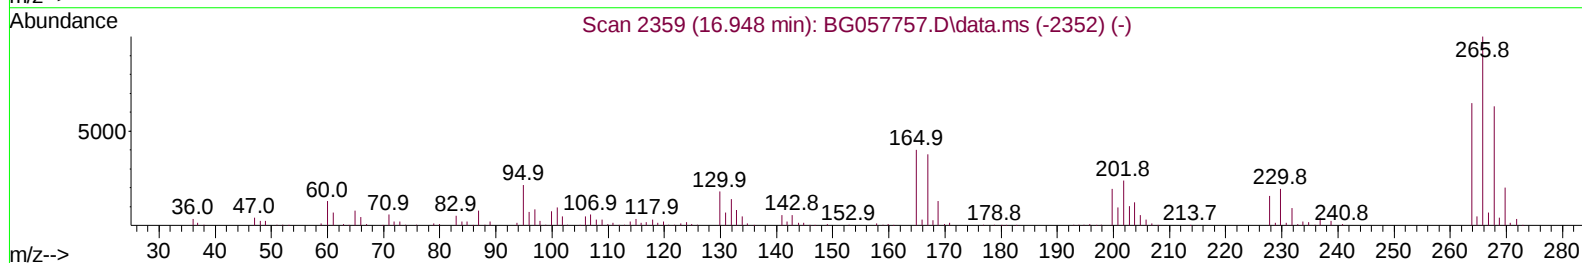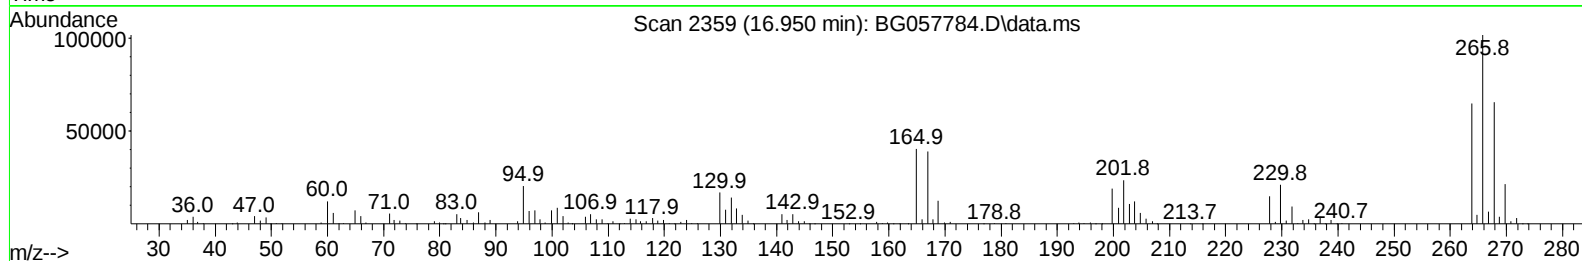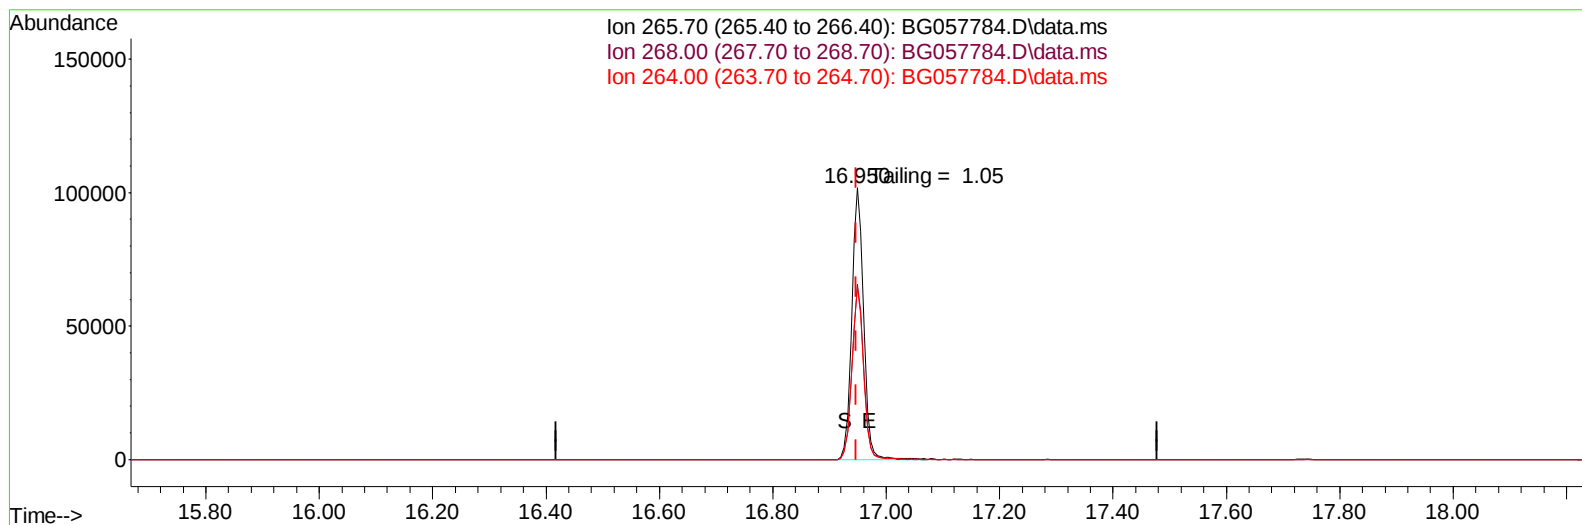

TIC: BG057784.D\data.ms

(70) Pentachlorophenol (C)

16.950min (+ 0.002) 30186.05 ng




response 146349

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.55
264.00	64.70	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062123\
Data File : BG057784.D
Acq On : 21 Jun 2023 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 22 06:21:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

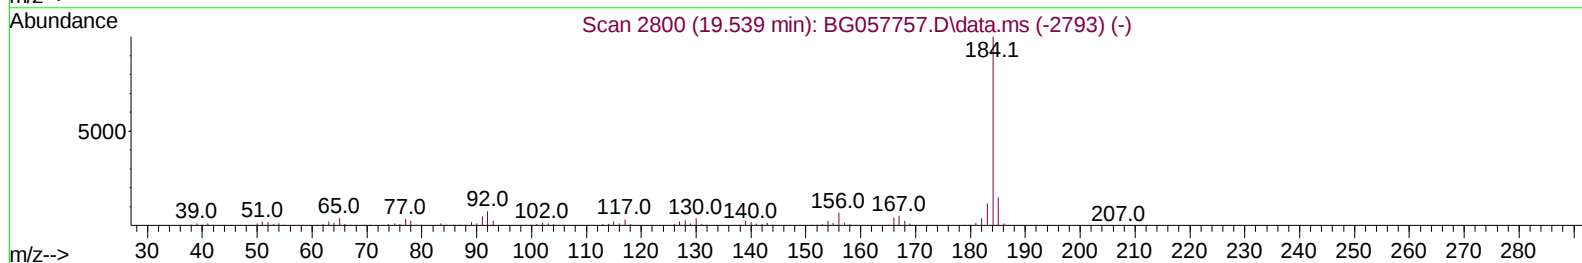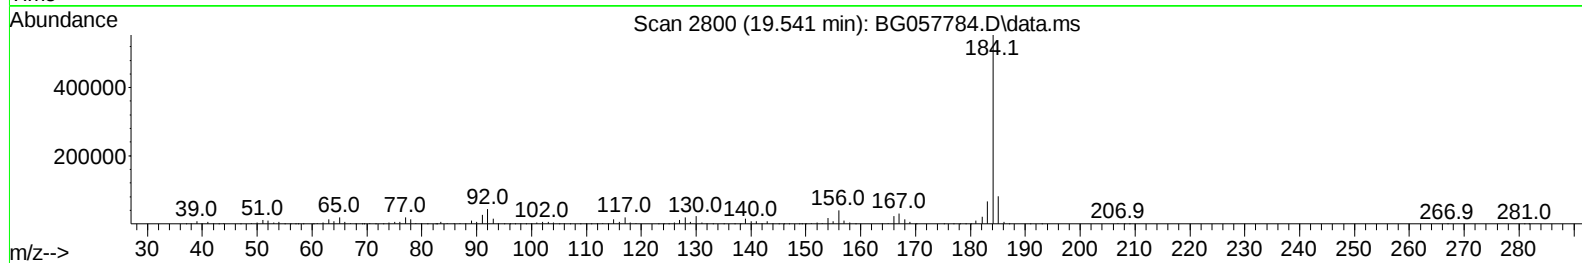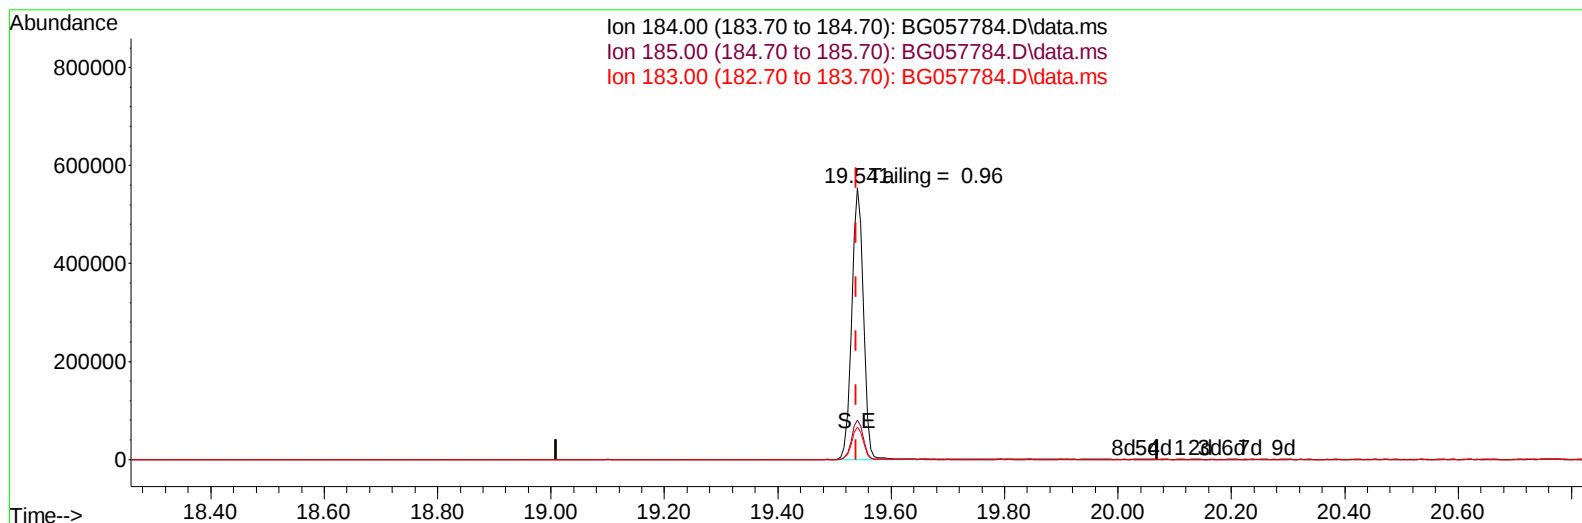

TIC: BG057784.D\data.ms

(77) Benzidine

19.541min (+ 0.002) 638317.93 ng m

response 793031

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.51
183.00	11.70	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2023	BNA_G	<u>BG057784.D</u>
Compound Name	Response	Retention Time
DDT	344103	20.769
DDD	4783	20.381
DDE	0	19.823
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4783	348886	1.37

Instrument :
BNA_G
ClientSampleId :
DFTPP