

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062218\
 Data File : BG035350.D
 Acq On : 23 Jun 2018 1:50
 Operator : JU/SJ
 Sample : PB110484BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB110484BL

Quant Time: Jun 23 02:33:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	45193	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	153549	20.00	ng	-0.02
38) Acenaphthene-d10	14.67	164	104197	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	297414	20.00	ng	-0.02
75) Chrysene-d12	21.68	240	363084	20.00	ng	-0.04
86) Perylene-d12	24.90	264	339018	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	324035	121.00	ng	-0.01
7) Phenol-d6	7.21	99	461493	116.76	ng	-0.01
23) Nitrobenzene-d5	9.22	82	290042	89.79	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	197163	147.81	ng	-0.02
44) 2-Fluorobiphenyl	13.30	172	677276	84.50	ng	-0.03
78) Terphenyl-d14	20.02	244	1349721	77.87	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.22	70	38657	11.512	ng	# 66
50) 2,6-Dinitrotoluene	14.67	165	15269	9.211	ng	# 22
56) 2,4-Dinitrotoluene	14.67	165	15269	6.934	ng	# 19
66) 4-Bromophenyl-phenylether	16.16	248	15601	4.356	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062218\
Data File : BG035350.D
Acq On : 23 Jun 2018 1:50
Operator : JU/SJ
Sample : PB110484BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB110484BL

Quant Time: Jun 23 02:33:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

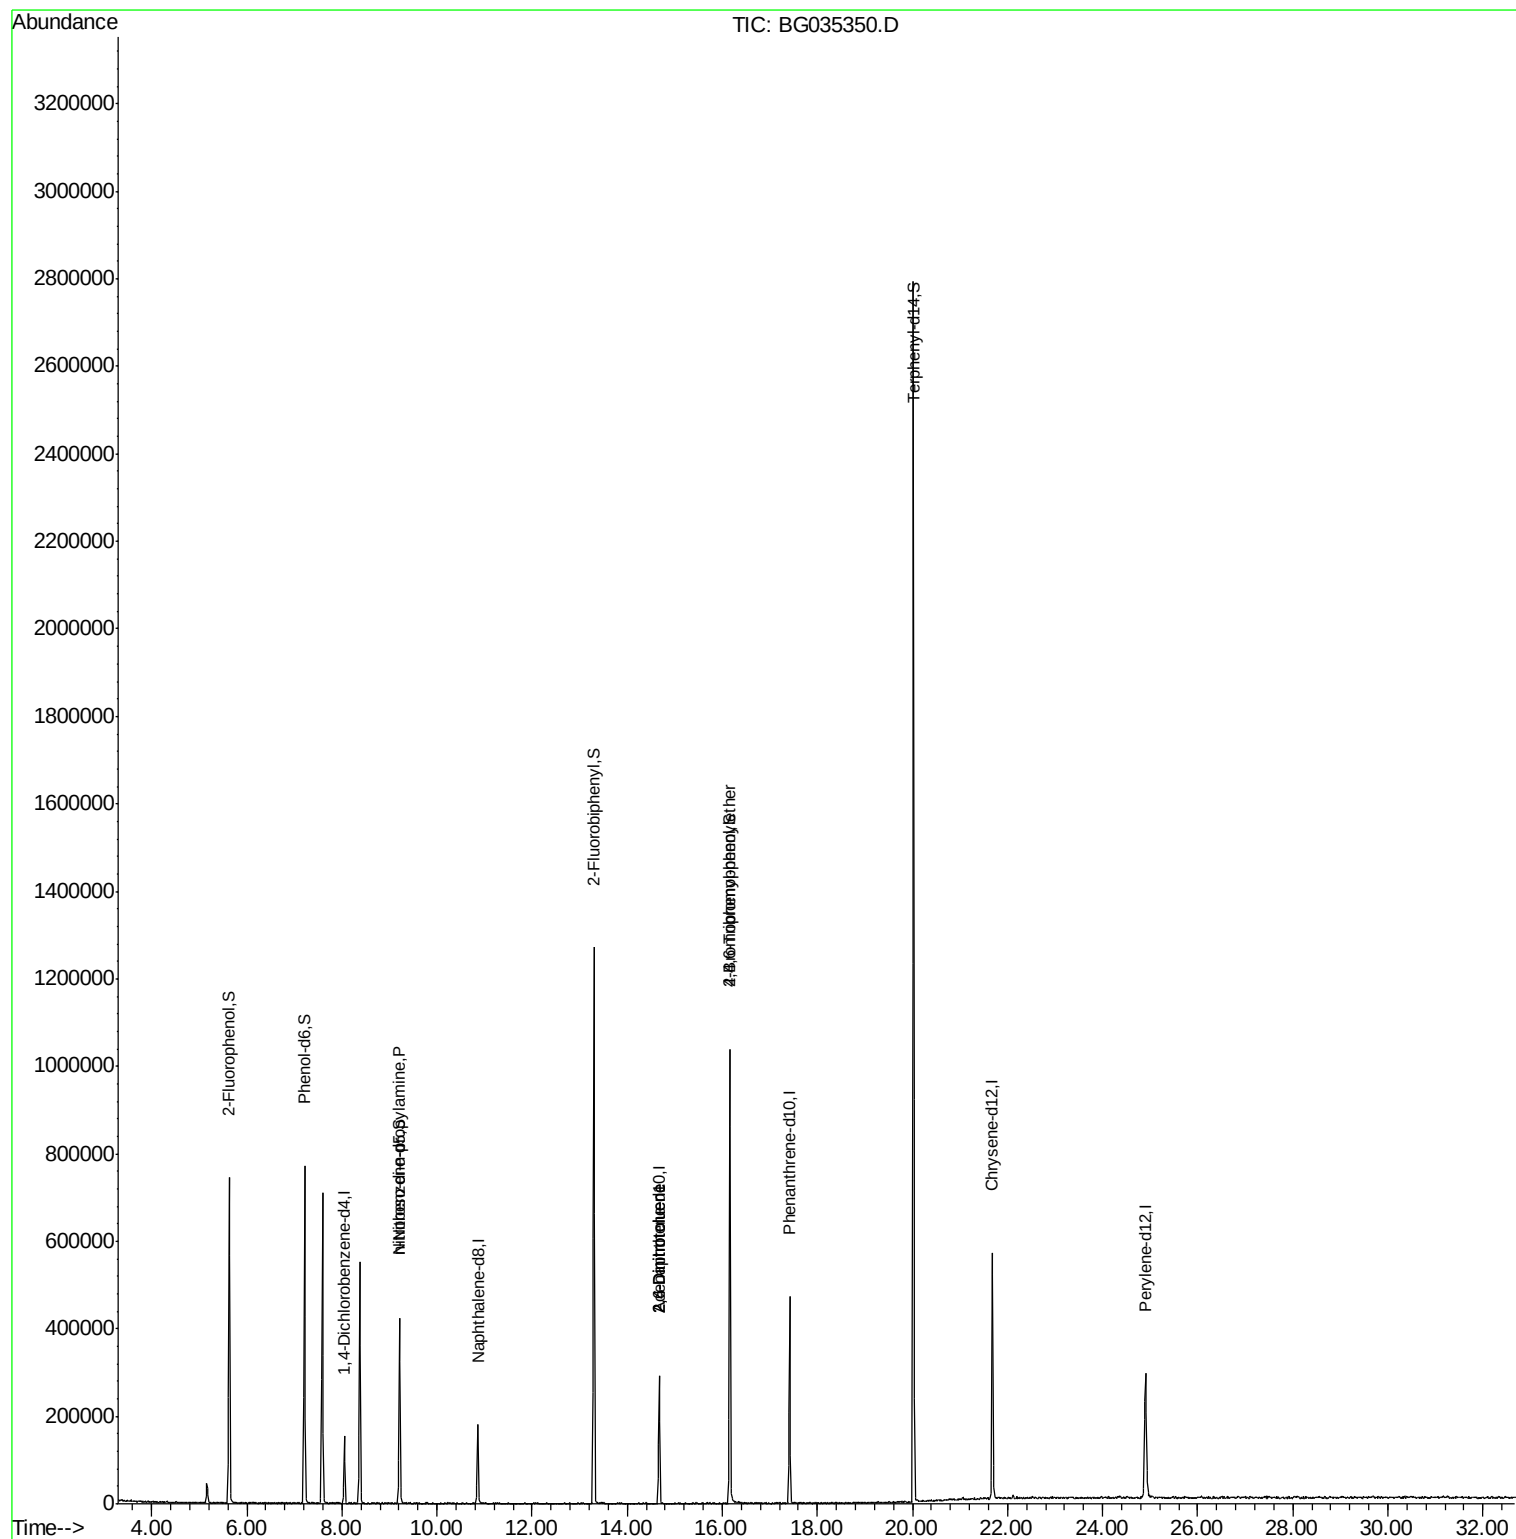




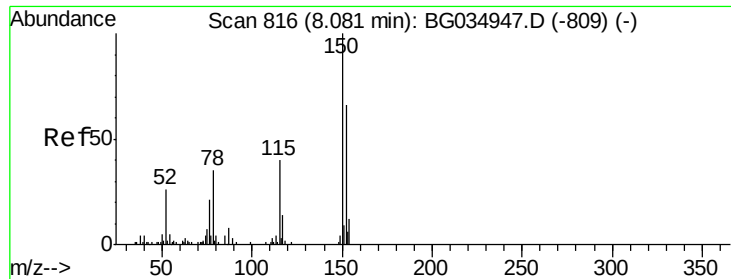


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 811
Delta R.T. -0.02 min
Lab File: BG035350.D
Acq: 23 Jun 2018 1:50

Instrument :
BNA_G
ClientSampleId :
PB110484BL




Tgt Ion:152 Resp: 45193
Ion Ratio Lower Upper
152 100
150 140.7 126.6 189.8
115 55.6 53.0 79.4

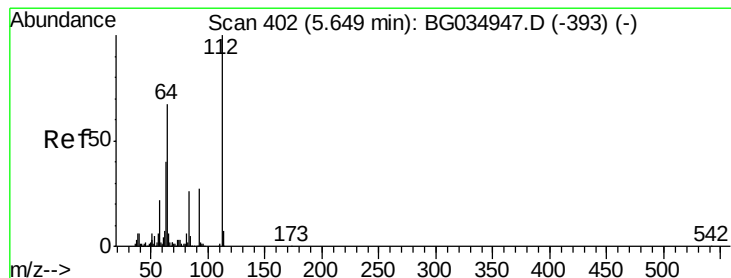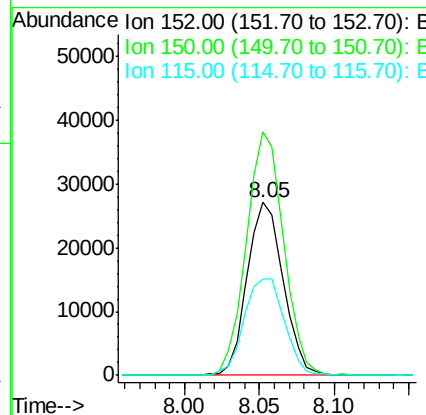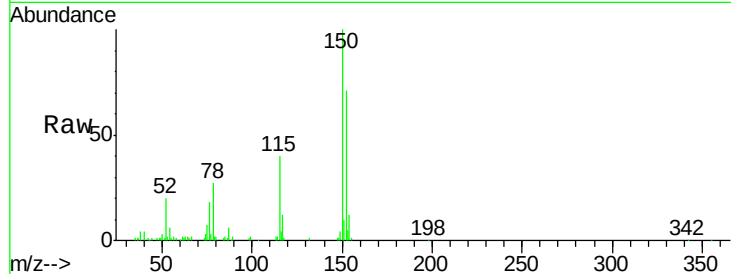


#5

2-Fluorophenol
Concen: 121.002 ng
RT: 5.63 min Scan# 399
Delta R.T. -0.01 min
Lab File: BG035350.D
Acq: 23 Jun 2018 1:50

Tgt Ion:112 Resp: 324035
Ion Ratio Lower Upper
112 100
64 62.1 56.3 84.5
63 36.3 30.1 45.1

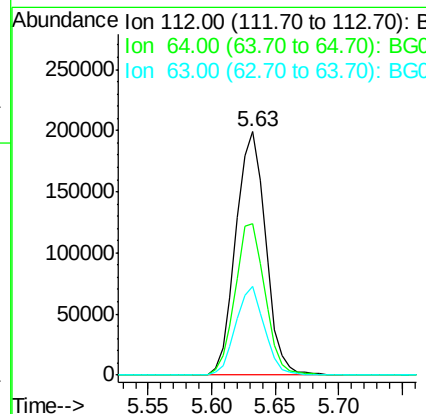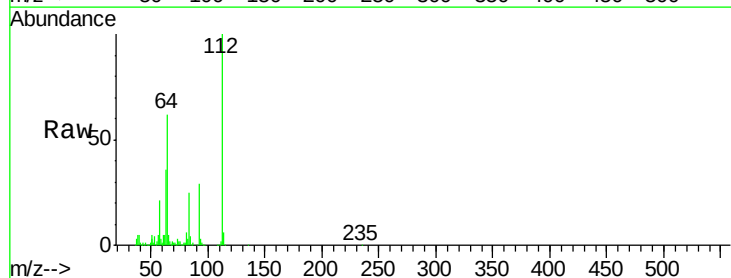

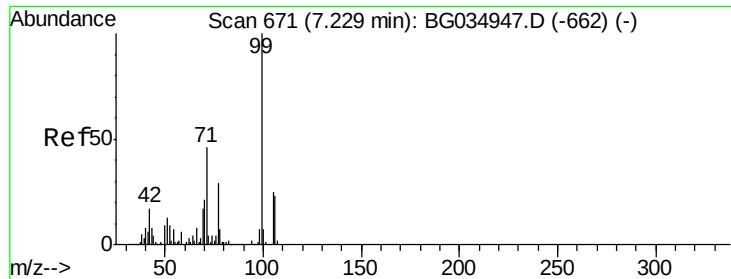

#7

Phenol-d6

Concen: 116.761 ng

RT: 7.21 min Scan# 668

Delta R.T. -0.01 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50

Instrument :

BNA_G

ClientSampleId :

PB110484BL


Tgt Ion: 99 Resp: 461493

Ion Ratio Lower Upper




99 100

42 14.7 14.1 21.1

71 42.5 26.1 39.1#

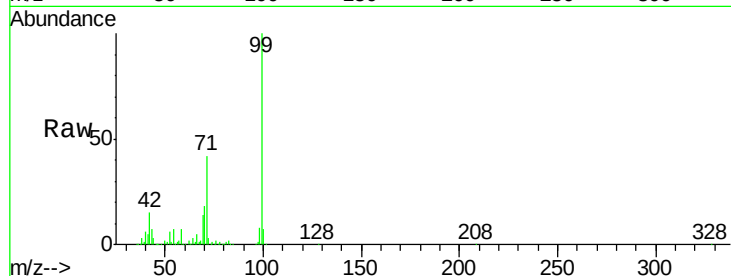

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

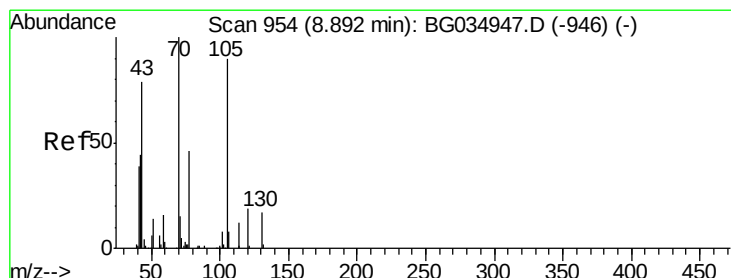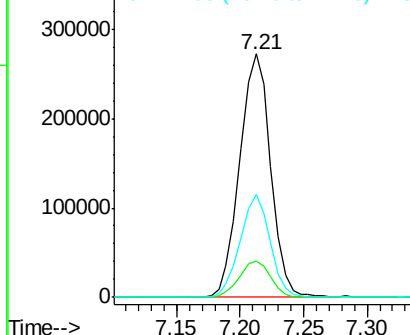

#19

n-Nitroso-di-n-propylamine

Concen: 11.512 ng

RT: 9.22 min Scan# 1009

Delta R.T. 0.33 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50

Tgt Ion: 70 Resp: 38657


Ion Ratio Lower Upper

70 100



42 35.0 49.1 73.7#


101 0.0 8.5 12.7#

130 1.9 13.4 20.0#

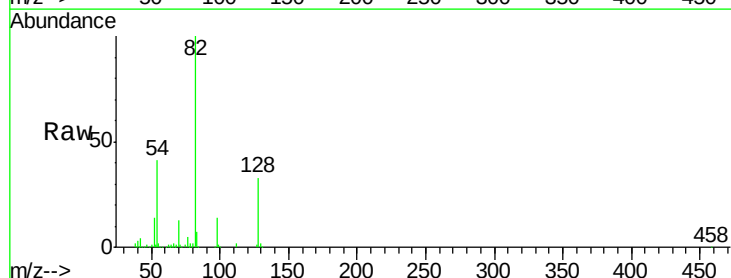

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

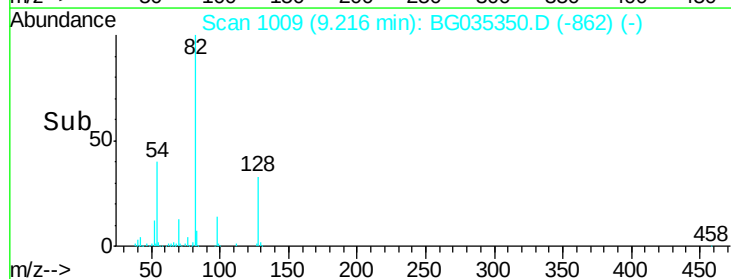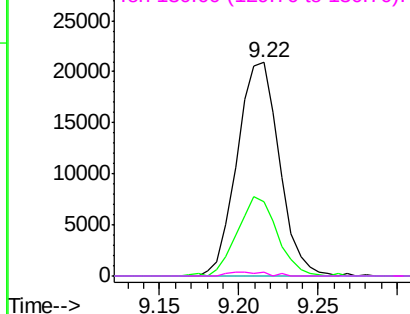



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1289

Delta R.T. -0.02 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50

Instrument :

BNA_G

ClientSampleId :

PB110484BL

Tgt Ion: 136 Resp: 153549


Ion Ratio Lower Upper

136 100

137 10.9 9.2 13.8

54 6.2 10.3 15.5#

68 4.1 4.5 6.7#



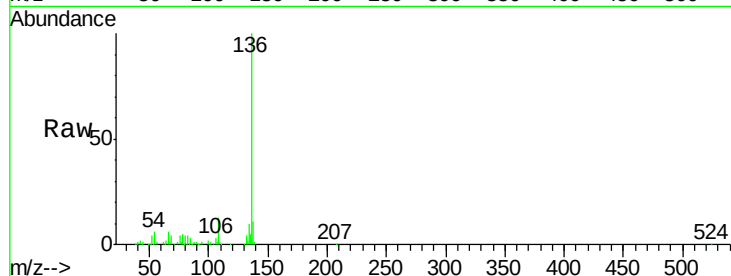


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

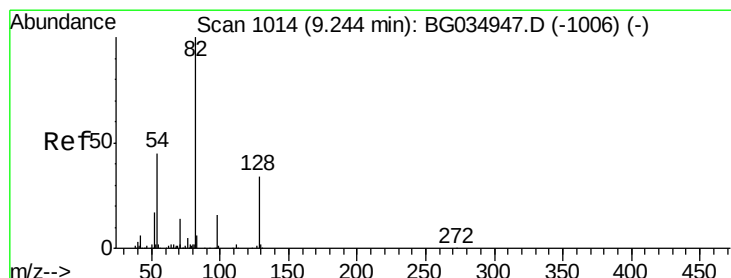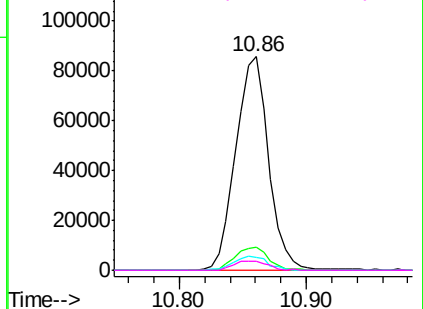

#23

Nitrobenzene-d5

Concen: 89.789 ng

RT: 9.22 min Scan# 1009

Delta R.T. -0.02 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50


Tgt Ion: 82 Resp: 290042

Ion Ratio Lower Upper

82 100

128 32.5 29.7 44.5



54 40.7 43.1 64.7#

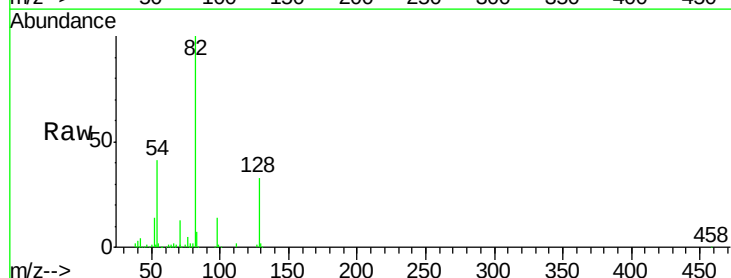


Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BGC

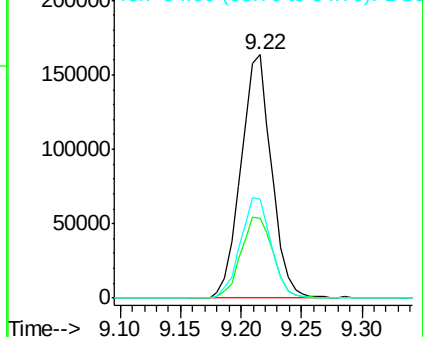

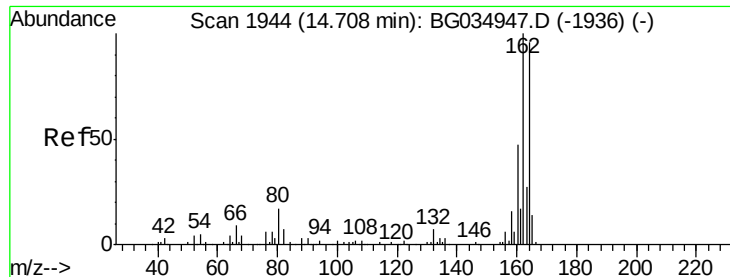

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1938

Delta R.T. -0.02 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50

Instrument :

BNA_G

ClientSampleId :

PB110484BL


Tgt Ion:164 Resp: 104197

Ion Ratio Lower Upper

164 100

162 100.9 78.8 118.2




160 45.6 35.4 53.0

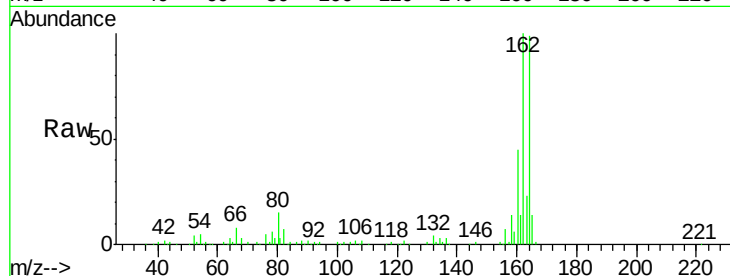

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

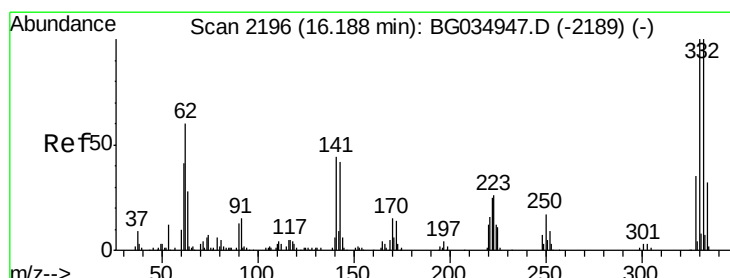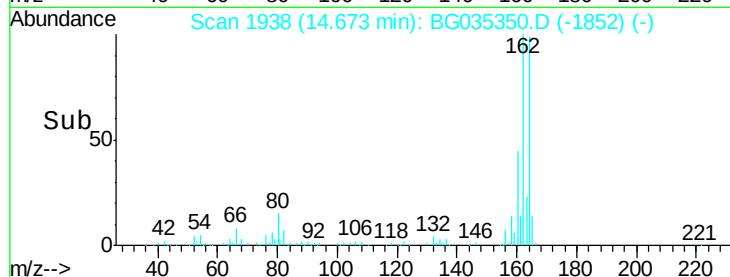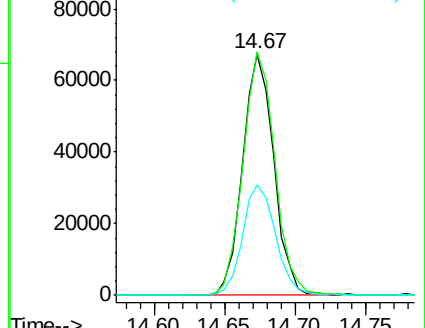

#41

2,4,6-Tribromophenol

Concen: 147.815 ng

RT: 16.16 min Scan# 2191

Delta R.T. -0.02 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50


Tgt Ion:330 Resp: 197163

Ion Ratio Lower Upper

330 100

332 95.2 77.0 115.6



141 36.7 25.2 37.8

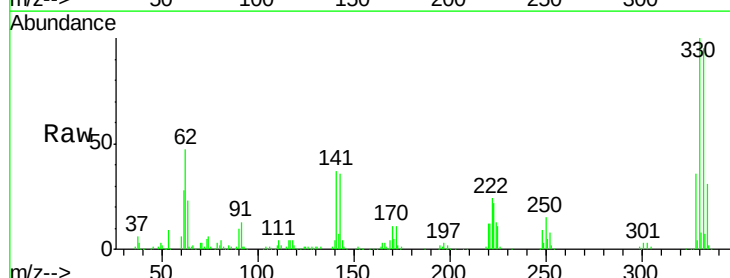


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



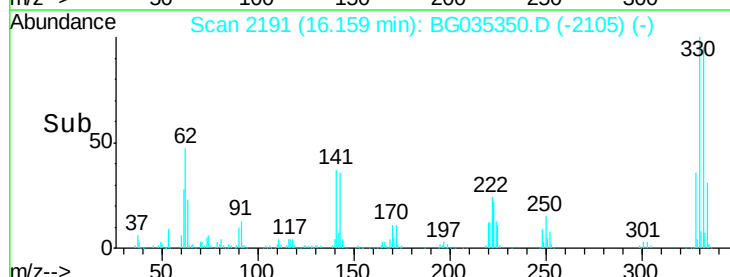
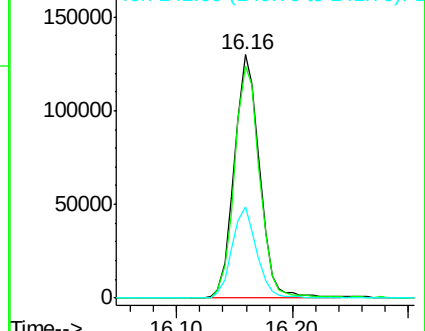


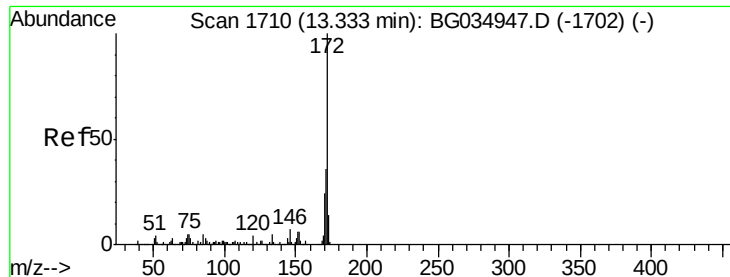

#44
2-Fluorobiphenyl
Concen: 84.499 ng
RT: 13.30 min Scan# 1704
Delta R.T. -0.03 min
Lab File: BG035350.D
Acq: 23 Jun 2018 1:50




Instrument :
BNA_G
ClientSampleId :
PB110484BL


Tgt Ion:172 Resp: 677276
Ion Ratio Lower Upper
172 100
171 34.1 30.0 45.0
170 23.8 19.5 29.3

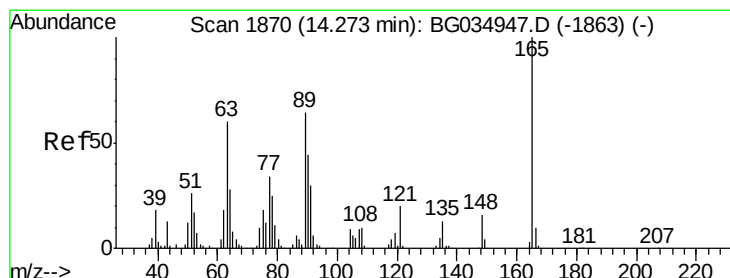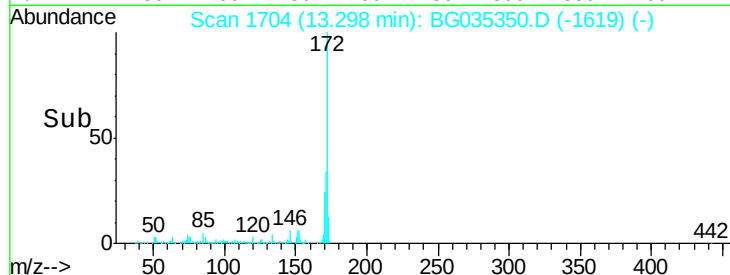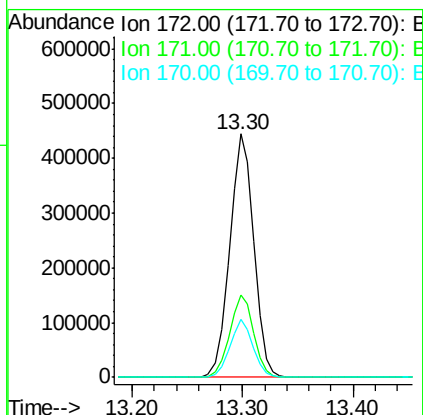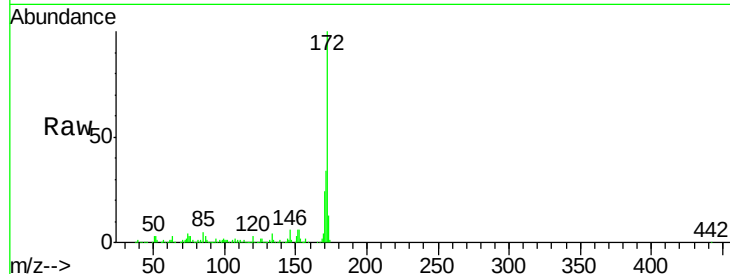

#50
2,6-Dinitrotoluene
Concen: 9.211 ng
RT: 14.67 min Scan# 1938
Delta R.T. 0.41 min
Lab File: BG035350.D
Acq: 23 Jun 2018 1:50

Tgt Ion:165 Resp: 15269
Ion Ratio Lower Upper
165 100
63 2.7 52.7 79.1#
89 2.4 49.2 73.8#

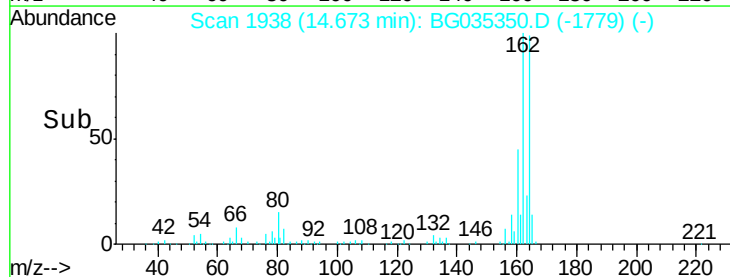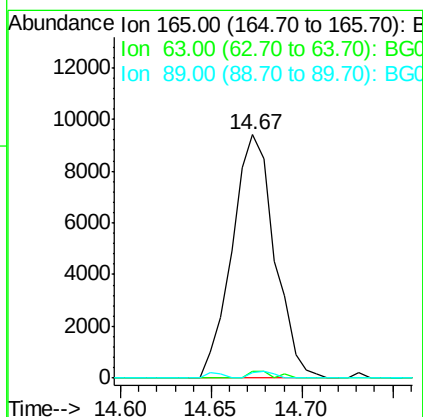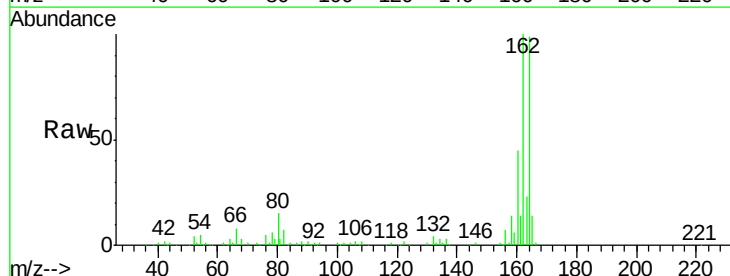







#56
 2,4-Dinitrotoluene
 Concen: 6.934 ng
 RT: 14.67 min Scan# 1938
 Delta R.T. -0.38 min
 Lab File: BG035350.D
 Acq: 23 Jun 2018 1:50

Instrument :
 BNA_G
 ClientSampleId :
 PB110484BL

Tgt Ion:165 Resp: 15269
 Ion Ratio Lower Upper
 165 100
 63 2.7 42.0 63.0#
 89 2.4 66.9 100.3#
 182 0.0 2.6 3.8#

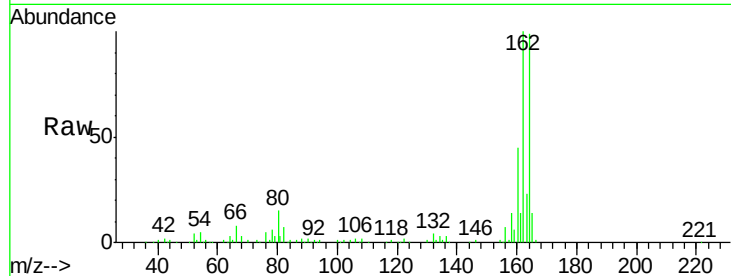


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

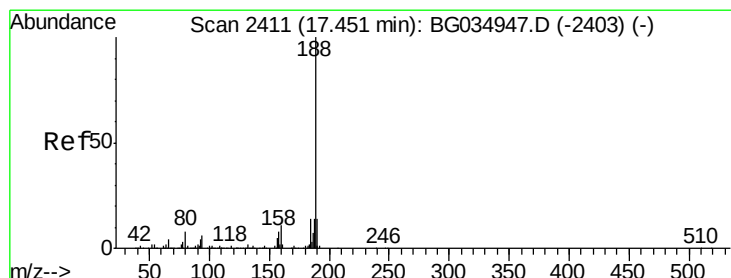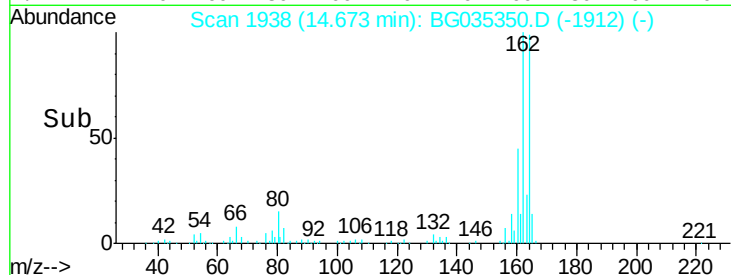
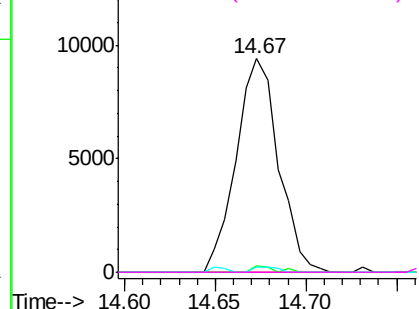



#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.42 min Scan# 2405
 Delta R.T. -0.02 min
 Lab File: BG035350.D
 Acq: 23 Jun 2018 1:50

Tgt Ion:188 Resp: 297414
 Ion Ratio Lower Upper
 188 100
 94 5.2 6.9 10.3#
 80 7.4 7.7 11.5#

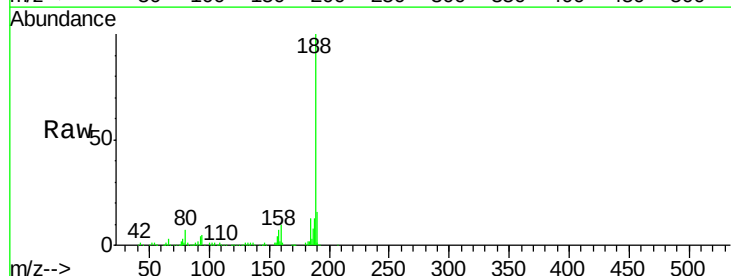

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC




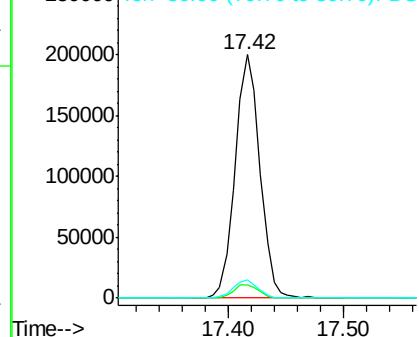




#66
 4-Bromophenyl-phenylether
 Concen: 4.356 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.48 min
 Lab File: BG035350.D
 Acq: 23 Jun 2018 1:50




Instrument :
 BNA_G
 ClientSampleId :
 PB110484BL


Tgt Ion:248 Resp: 15601
 Ion Ratio Lower Upper
 248 100
 250 179.1 77.1 115.7#
 141 434.4 50.8 76.2#

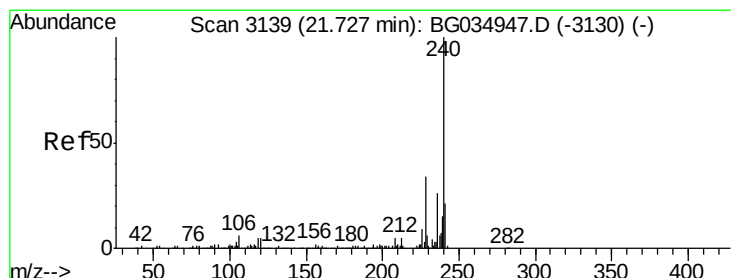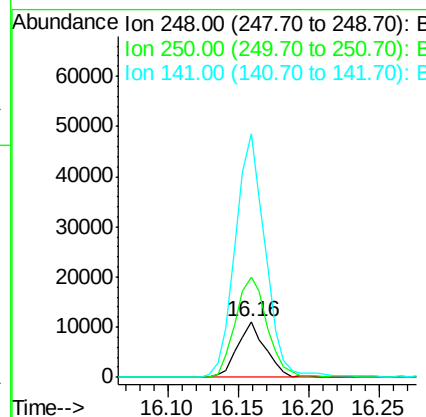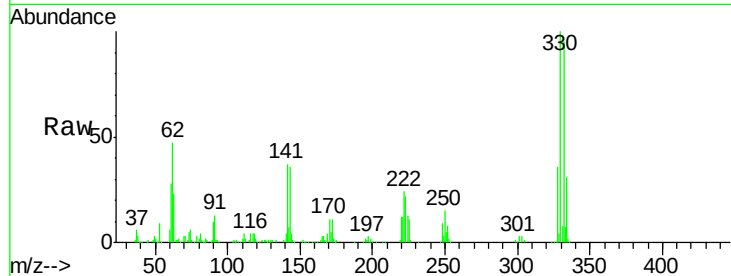

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.68 min Scan# 3131
 Delta R.T. -0.04 min
 Lab File: BG035350.D
 Acq: 23 Jun 2018 1:50

Tgt Ion:240 Resp: 363084
 Ion Ratio Lower Upper
 240 100
 120 4.7 6.8 10.2#
 236 26.5 20.9 31.3

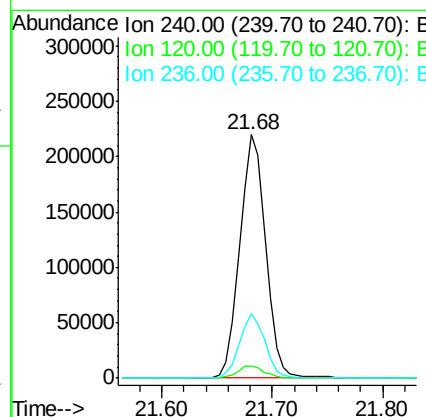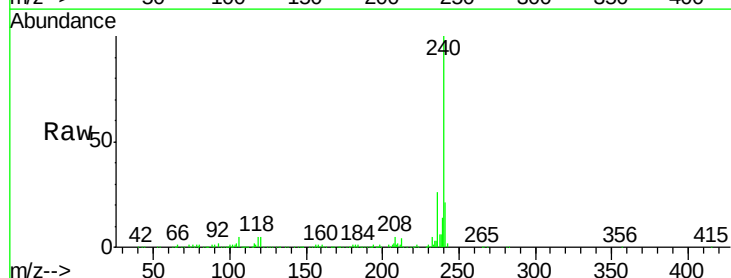

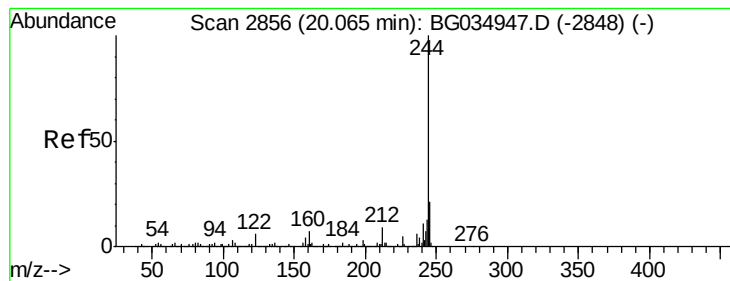

#78

Terphenyl-d14

Concen: 77.867 ng

RT: 20.02 min Scan# 2849

Delta R.T. -0.02 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50

Instrument :

BNA_G

ClientSampleId :

PB110484BL


Tgt Ion:244 Resp: 1349721

Ion Ratio Lower Upper

244 100

212 8.9 5.8 8.8#




122 6.6 7.0 10.4#

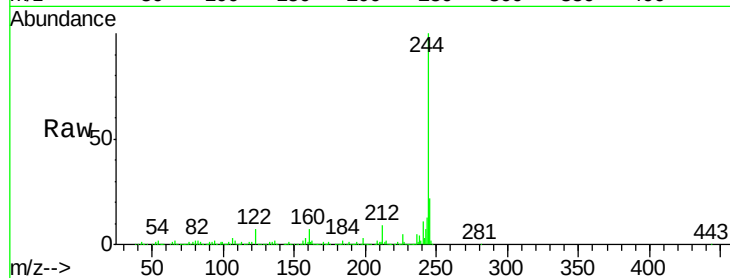

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

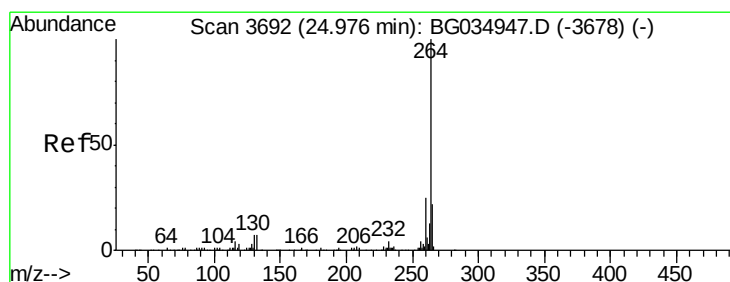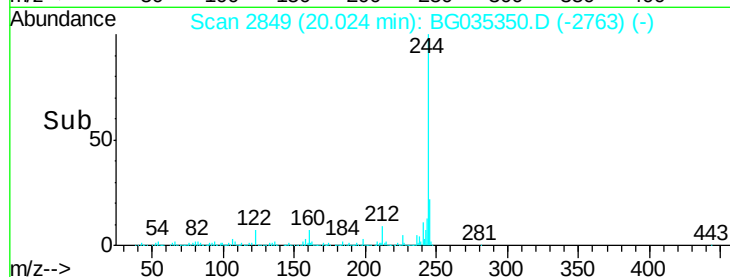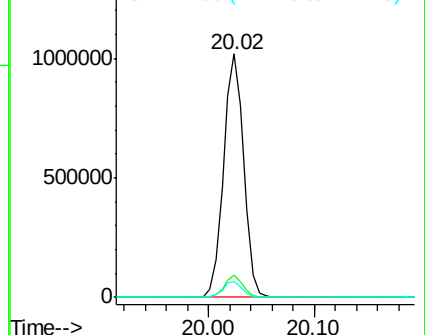

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.90 min Scan# 3679

Delta R.T. -0.05 min

Lab File: BG035350.D

Acq: 23 Jun 2018 1:50


Tgt Ion:264 Resp: 339018

Ion Ratio Lower Upper

264 100

260 24.4 17.4 26.0

265 21.6 17.7 26.5

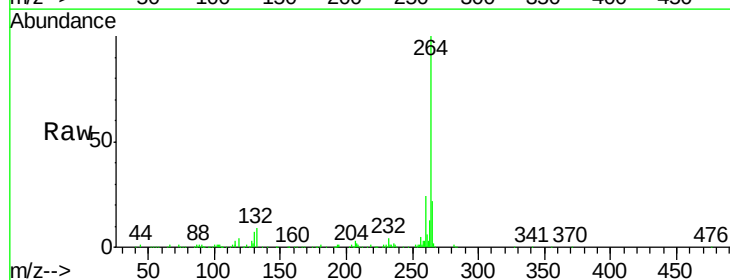

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

