
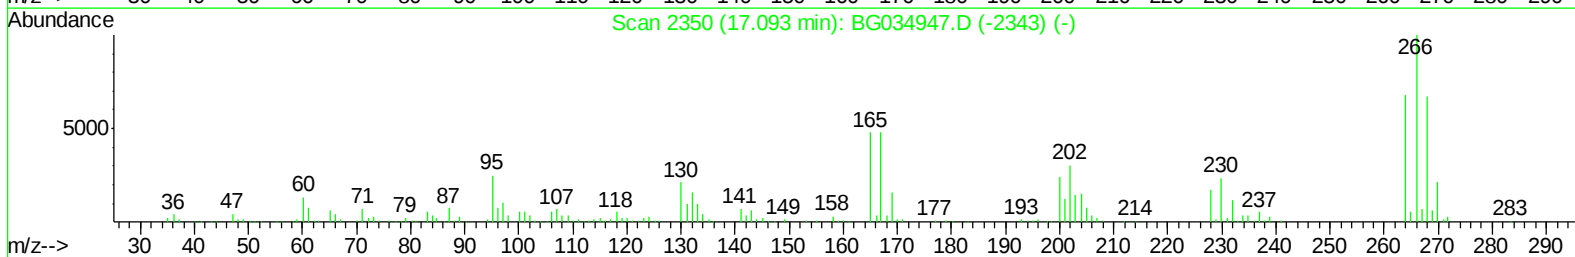
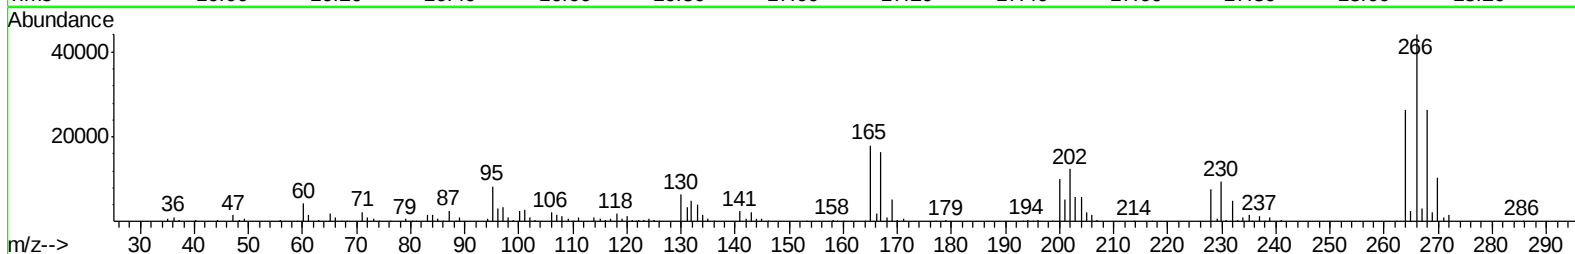


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062218\
Data File : BG035332.D
Acq On : 22 Jun 2018 14:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:55:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

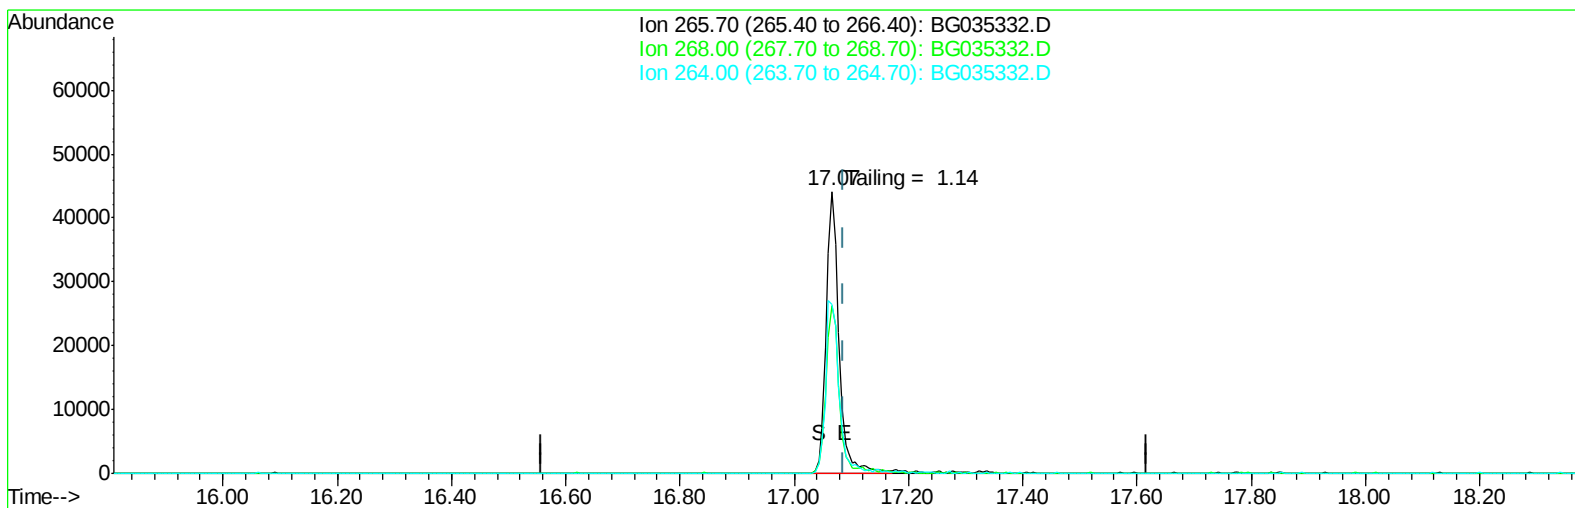

TIC: BG035332.D

(69) Pentachlorophenol (C)




17.066min (-0.021) 156486.30ng

response 68358

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.72
264.00	62.00	59.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062218\
 Data File : BG035332.D
 Acq On : 22 Jun 2018 14:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:55:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration

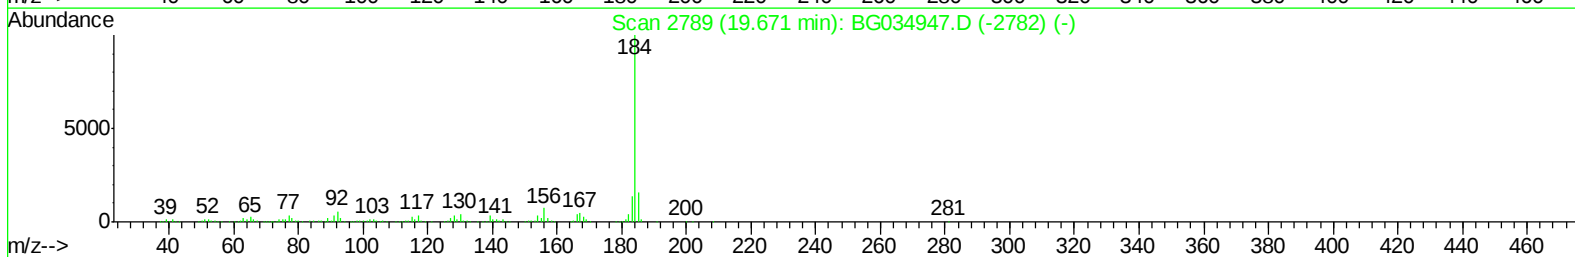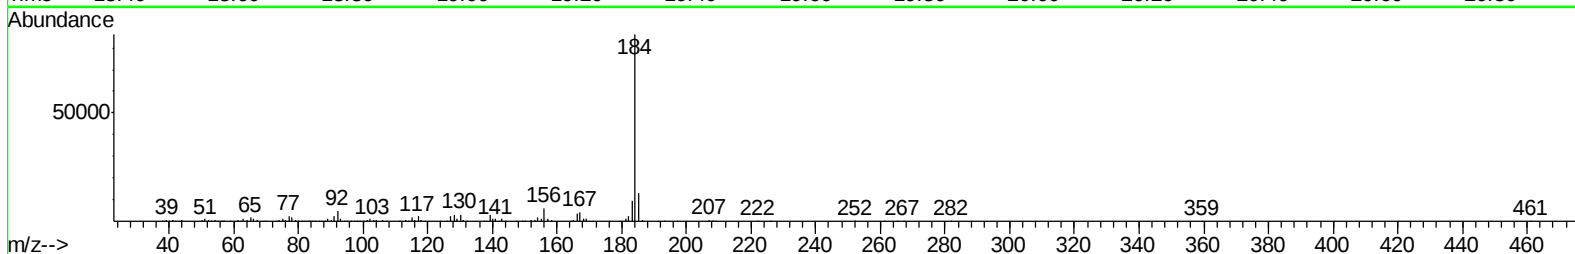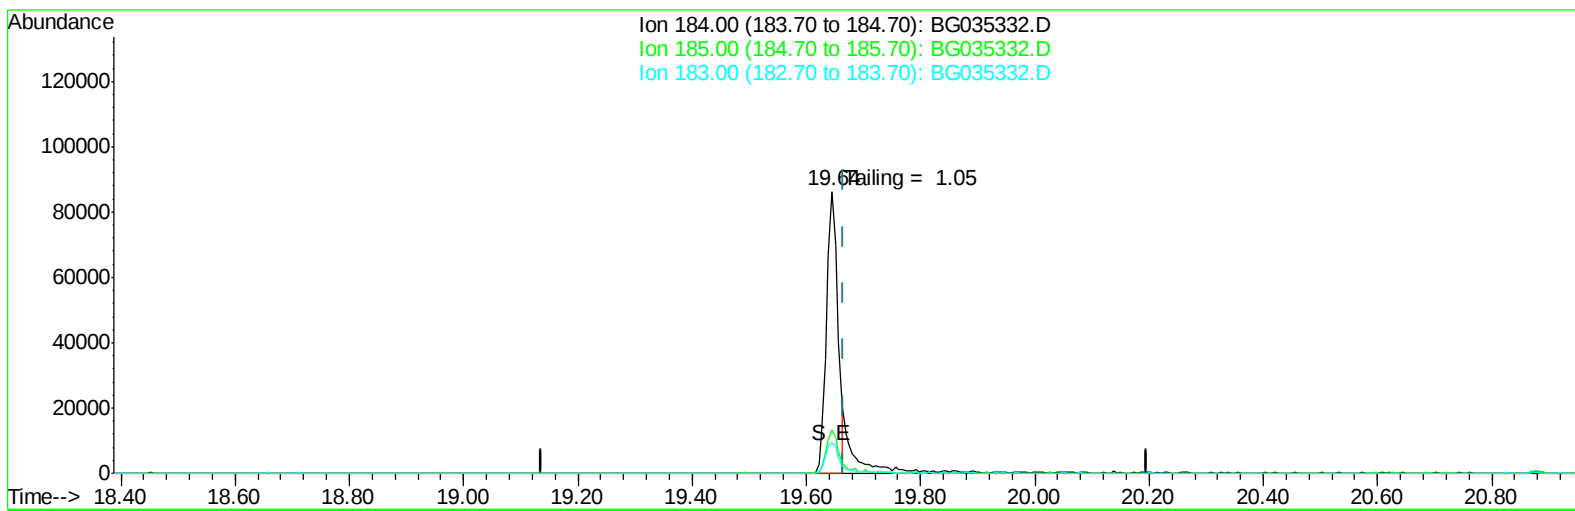

TIC: BG035332.D

(76) Benzidine

19.645min (-0.021) 45567.14ng

response 96630

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.52
183.00	13.30	10.81
0.00	0.00	0.00