


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062218\
Data File : BG035332.D
Acq On : 22 Jun 2018 14:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 08 17:16:28 2018

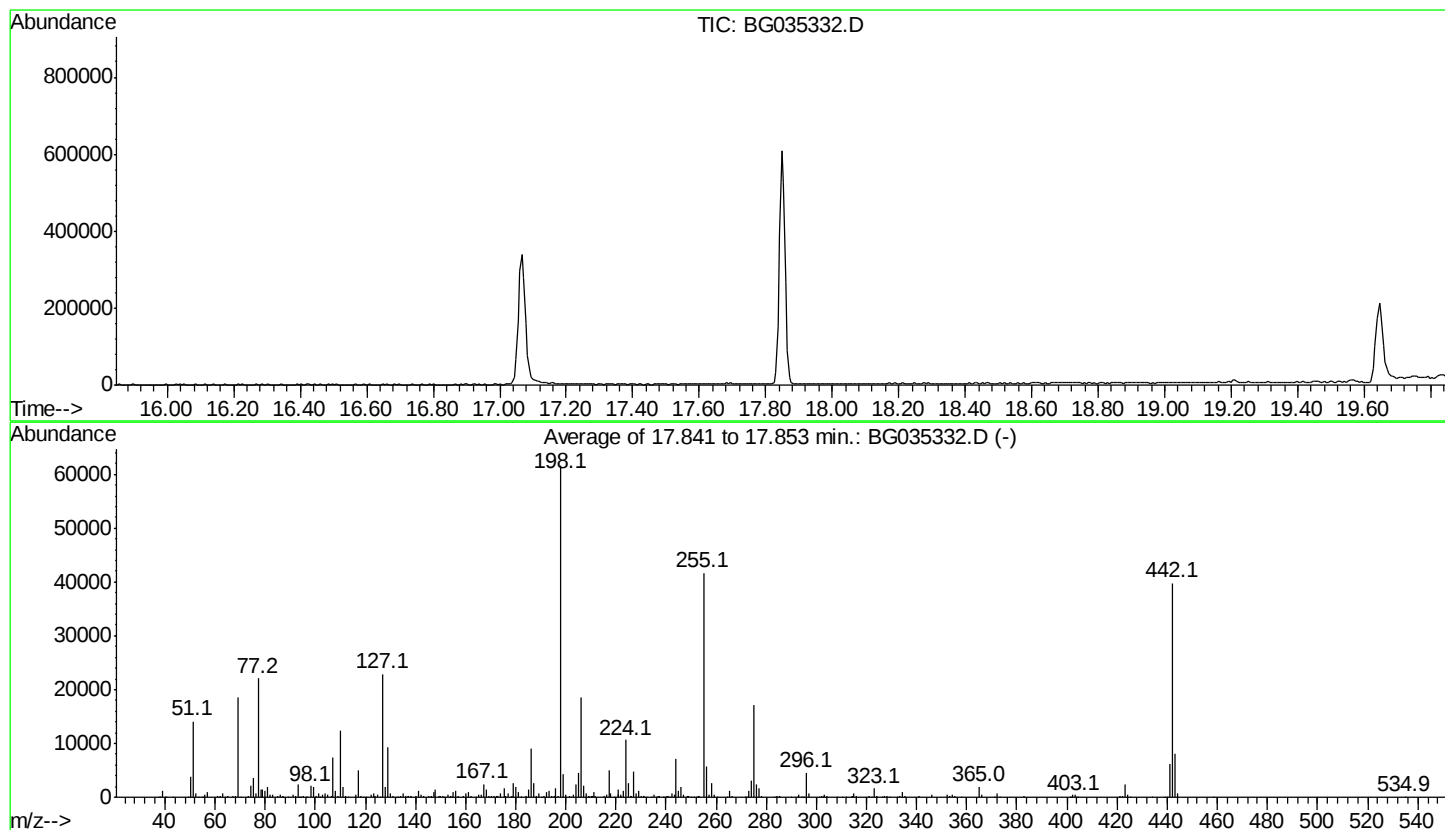

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	14121	PASS
68	69	0.00	2	1.2	227	PASS
69	198	0.00	100	30.2	18602	PASS
70	69	0.00	2	0.5	94	PASS
127	198	10	80	37.2	22930	PASS
197	198	0.00	2	0.5	304	PASS
198	198	100	100	100.0	61602	PASS
199	198	5	9	7.0	4322	PASS
275	198	10	60	28.0	17242	PASS
365	198	1	100	3.3	2018	PASS
441	443	0.01	100	75.7	6138	PASS
442	198	50	100	64.6	39824	PASS
443	442	15	24	20.3	8104	PASS