


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062218\
 Data File : BG035351.D
 Acq On : 23 Jun 2018 3:48
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

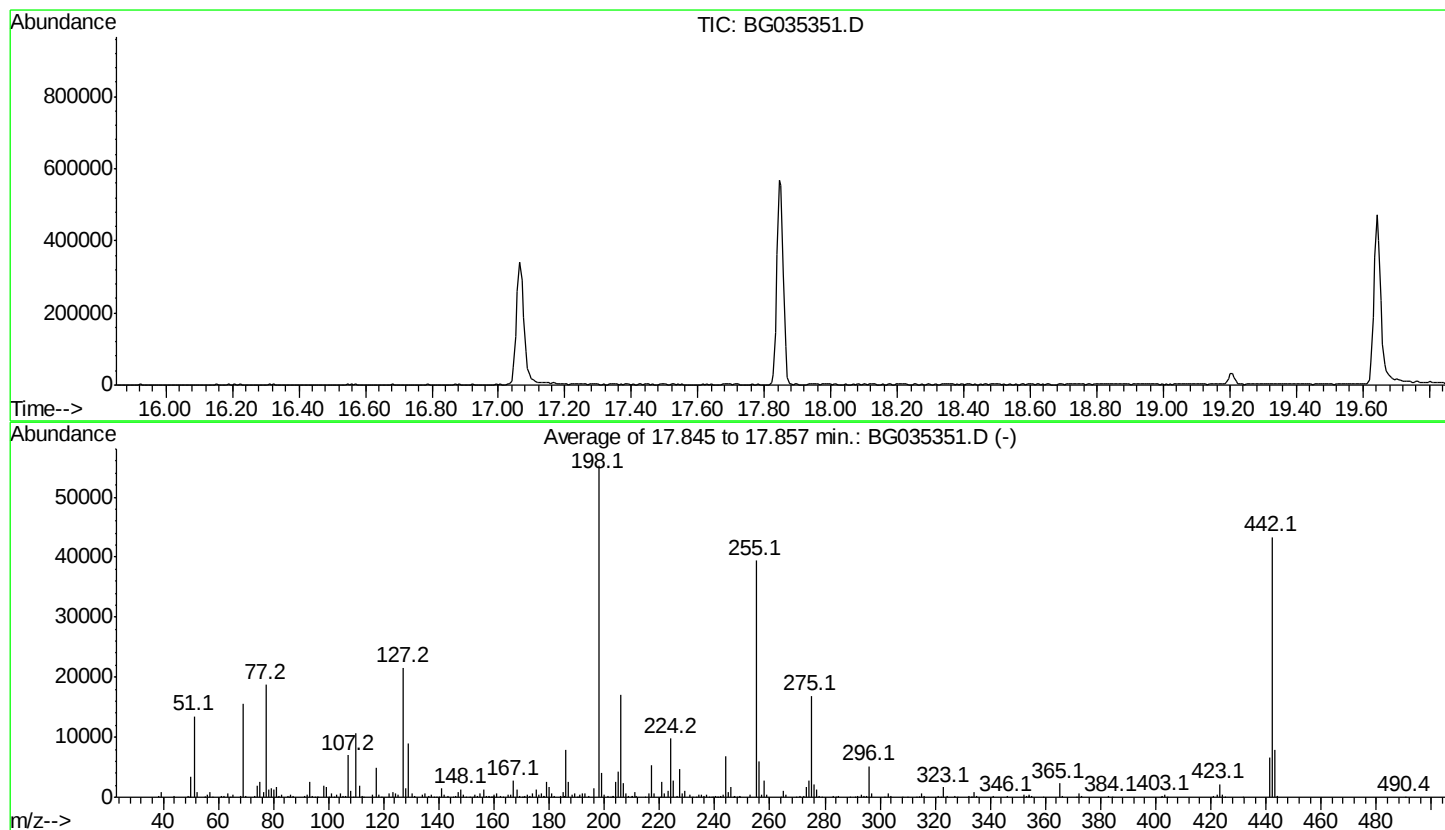

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.5	13523	PASS
68	69	0.00	2	1.4	220	PASS
69	198	0.00	100	28.3	15647	PASS
70	69	0.00	2	1.1	172	PASS
127	198	10	80	39.0	21562	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55248	PASS
199	198	5	9	7.2	3957	PASS
275	198	10	60	30.6	16904	PASS
365	198	1	100	4.1	2289	PASS
441	443	0.01	100	84.0	6570	PASS
442	198	50	100	78.4	43320	PASS
443	442	15	24	18.1	7823	PASS