
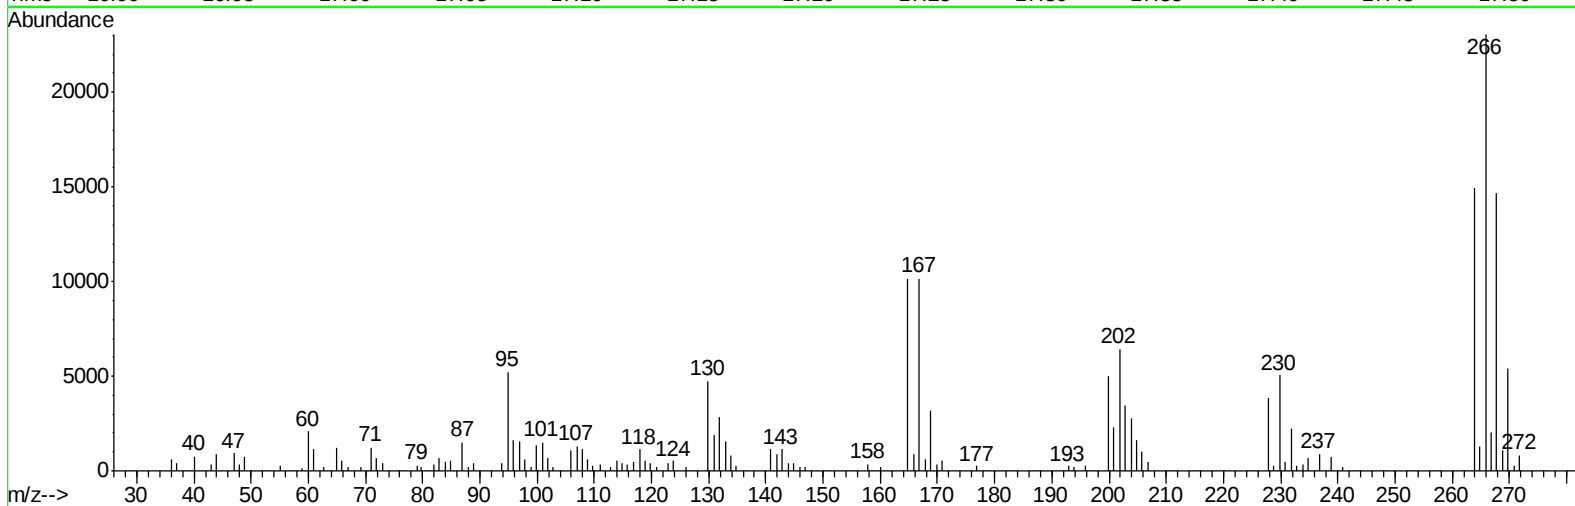


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062219\
Data File : BG041399.D
Acq On : 22 Jun 2019 12:20
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:07:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

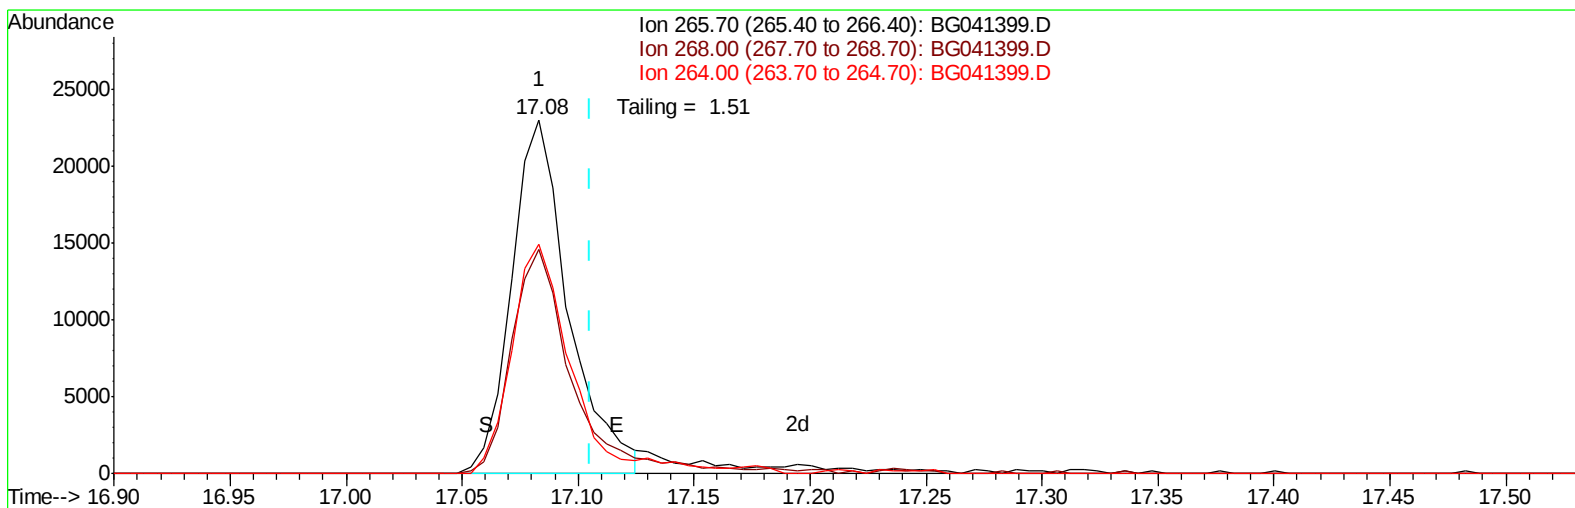

TIC: BG041399.D

(70) Pentachlorophenol (C)



17.083min (-0.023) 0.00ng

response 40388

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.51
264.00	64.00	70.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062219\
Data File : BG041399.D
Acq On : 22 Jun 2019 12:20
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:07:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 14:58:02 2019
Response via : Initial Calibration

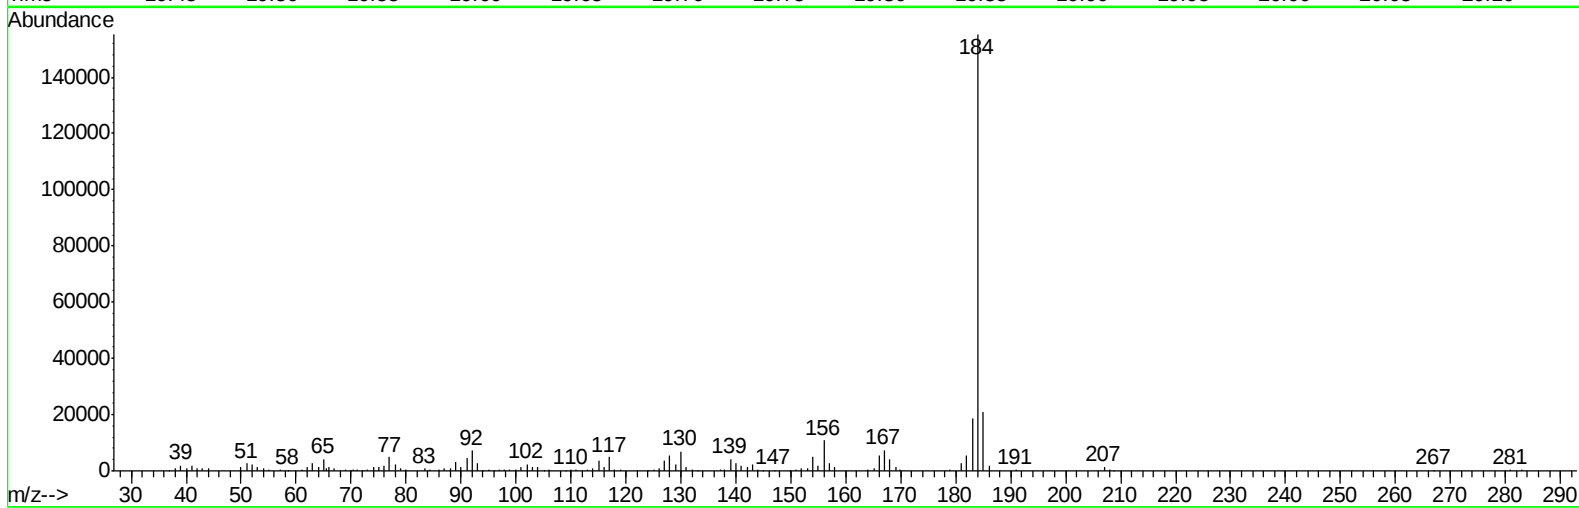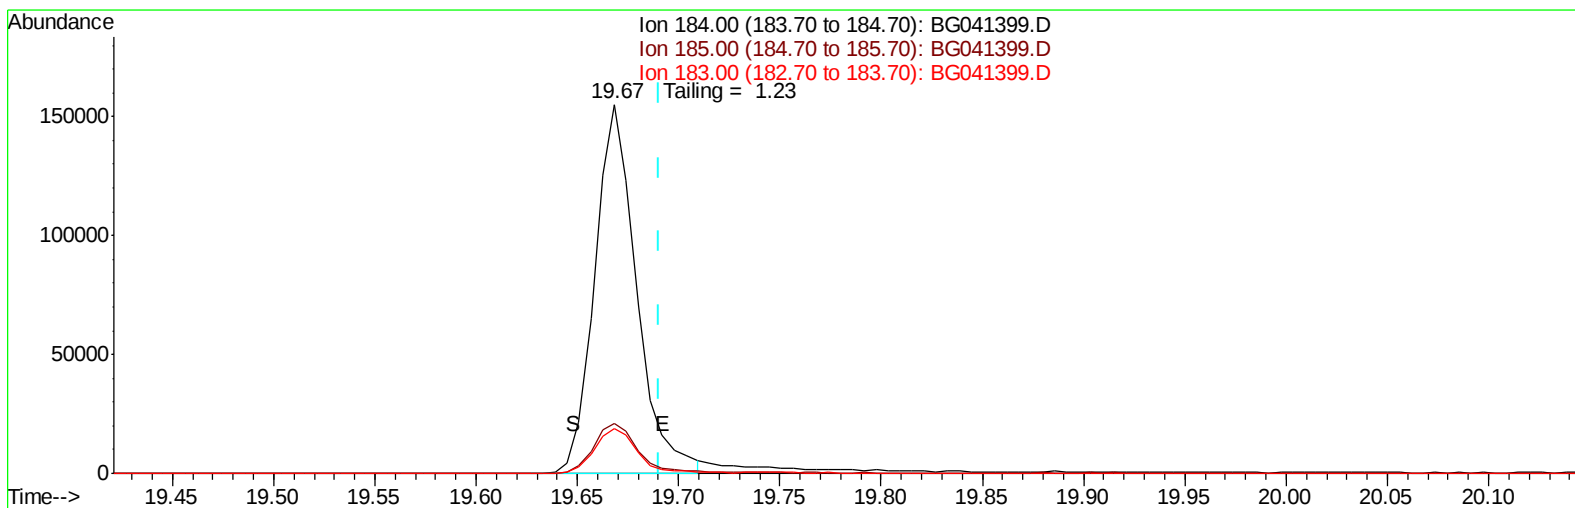

TIC: BG041399.D

(77) Benzidine

19.668min (-0.023) 183004.93ng

response 239029

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.60
183.00	12.00	12.13
0.00	0.00	0.00