


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG062219\
 Data File : BG041399.D
 Acq On : 22 Jun 2019 12:20
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 14:58:02 2019

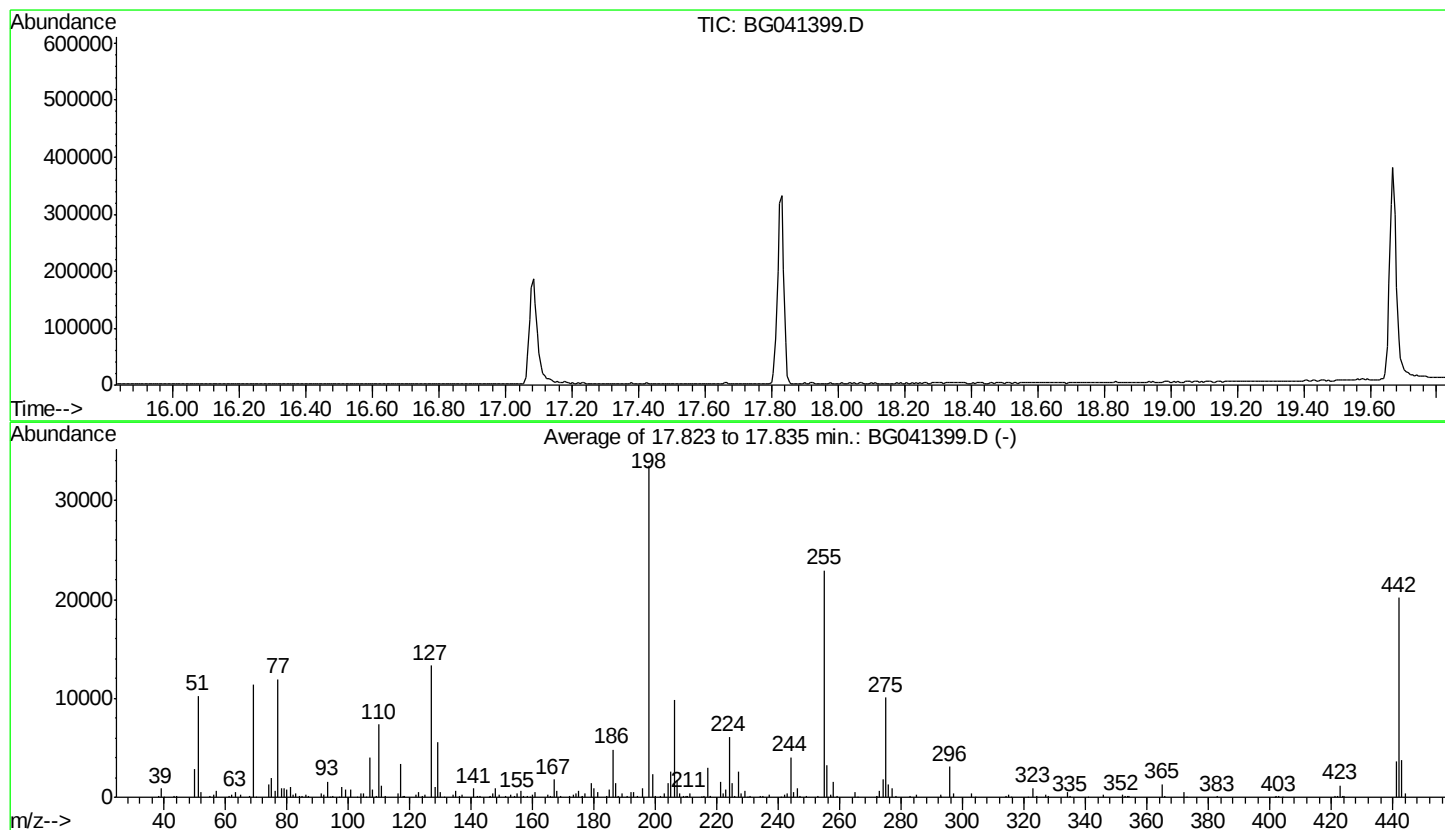

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	10251	PASS
68	69	0.00	2	0.8	93	PASS
69	198	0.00	100	34.1	11443	PASS
70	69	0.00	2	0.5	59	PASS
127	198	10	80	39.6	13291	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33541	PASS
199	198	5	9	7.0	2353	PASS
275	198	10	60	30.1	10089	PASS
365	198	1	100	3.9	1316	PASS
441	198	0.01	100	10.9	3644	PASS
442	198	50	100	60.2	20178	PASS
443	442	15	24	18.5	3740	PASS