
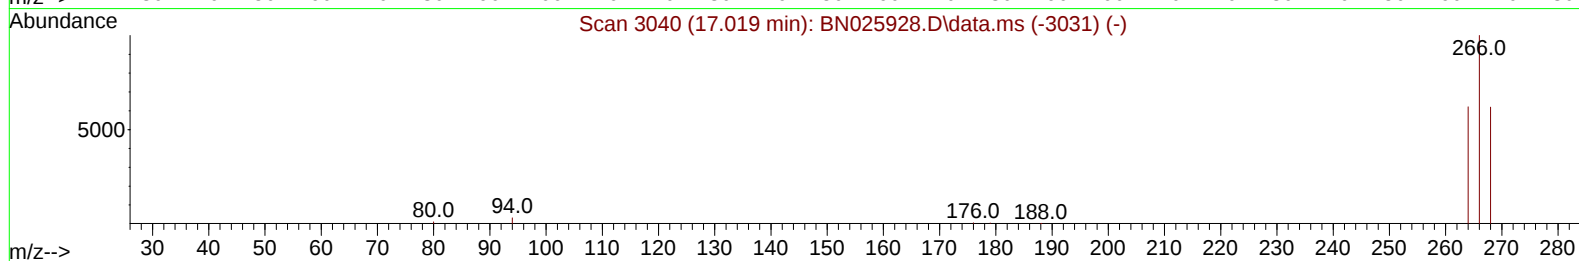
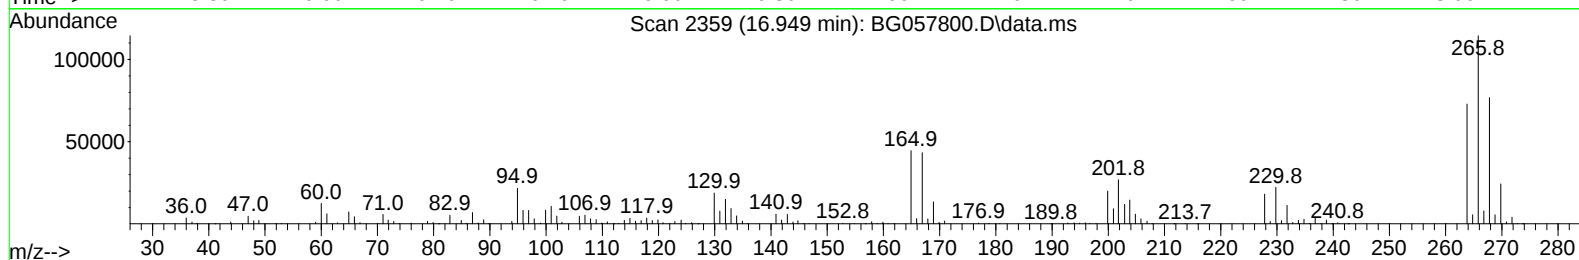


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
Data File : BG057800.D
Acq On : 22 Jun 2023 7:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 13:34:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

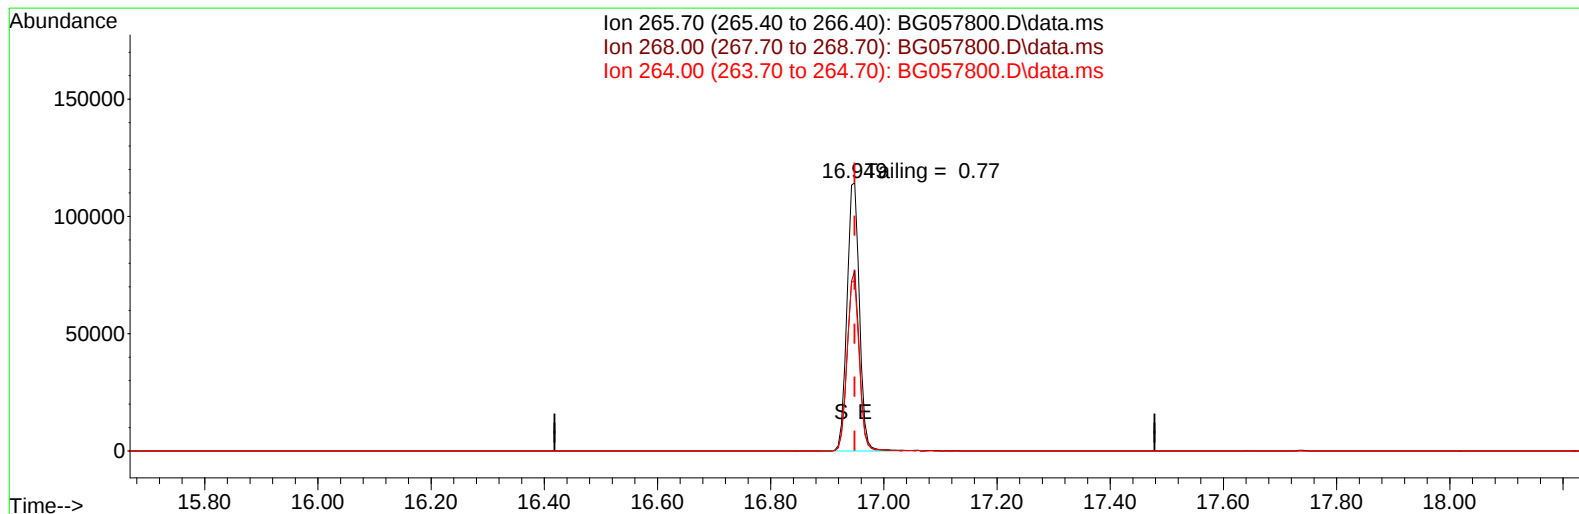

TIC: BG057800.D\data.ms

(70) Pentachlorophenol (C)




16.949min (+ 0.001) 28680.55 ng

response 174557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	67.12
264.00	64.70	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
Data File : BG057800.D
Acq On : 22 Jun 2023 7:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 13:34:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

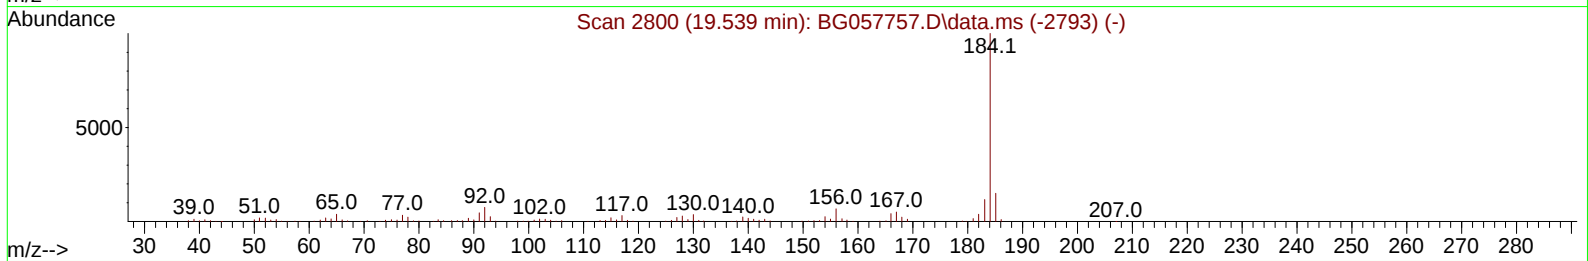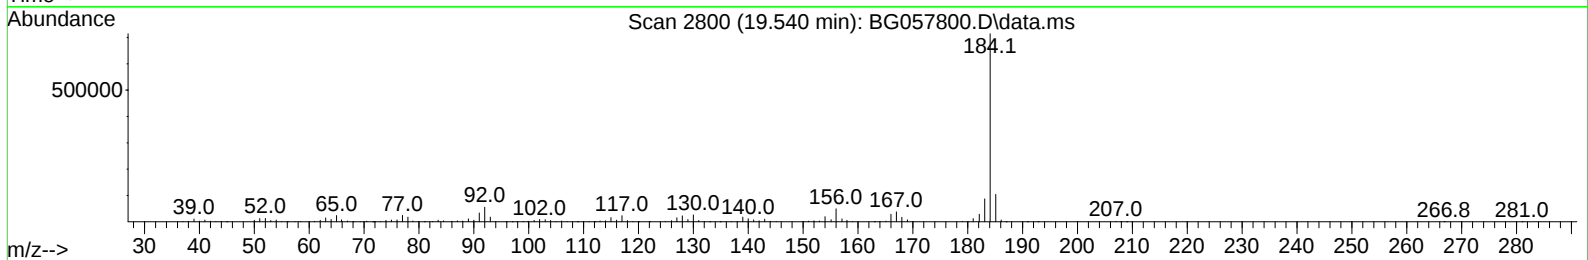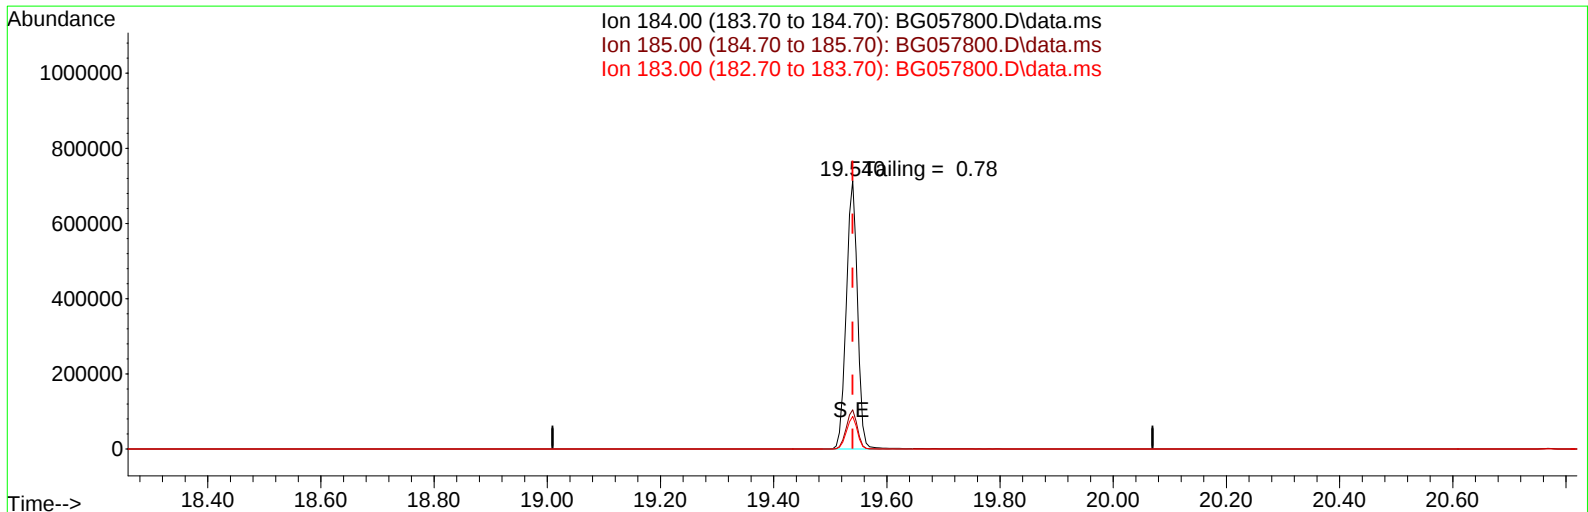

TIC: BG057800.D\data.ms

(77) Benzidine**19.540min (+ 0.001) 0.00 ng****response 985089**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.61
183.00	11.70	12.19
0.00	0.00	0.00