
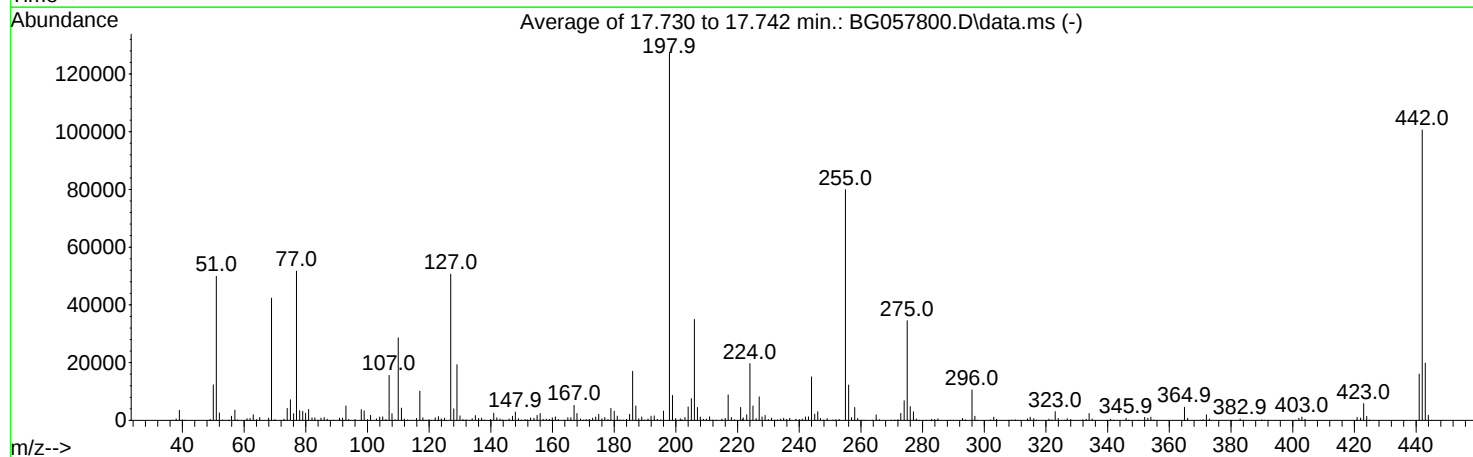


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
Data File : BG057800.D
Acq On : 22 Jun 2023 7:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 20 03:40:38 2023

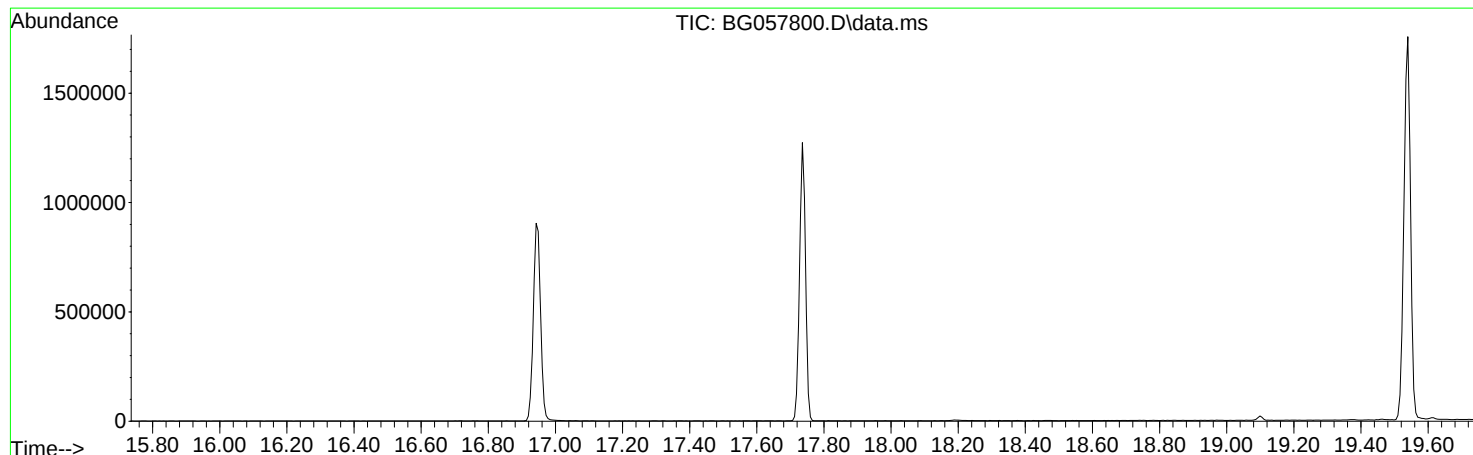

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	49912	PASS
68	69	0.00	2	1.9	784	PASS
69	198	0.00	100	33.2	42333	PASS
70	69	0.00	2	0.5	207	PASS
127	198	10	80	39.7	50640	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	127437	PASS
199	198	5	9	6.8	8662	PASS
275	198	10	60	27.1	34555	PASS
365	198	1	100	3.6	4542	PASS
441	198	0.01	100	12.6	16022	PASS
442	442	50	100	100.0	100611	PASS
443	442	15	24	19.7	19870	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/22/2023	BNA_G	<u>BG057800.D</u>
Compound Name	Response	Retention Time
DDT	447134	20.768
DDD	5801	20.38
DDE	0	19.823
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5801	452935	1.28

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
 Data File : BG057800.D
 Acq On : 22 Jun 2023 7:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 22 13:34:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 03:40:38 2023
 Response via : Initial Calibration

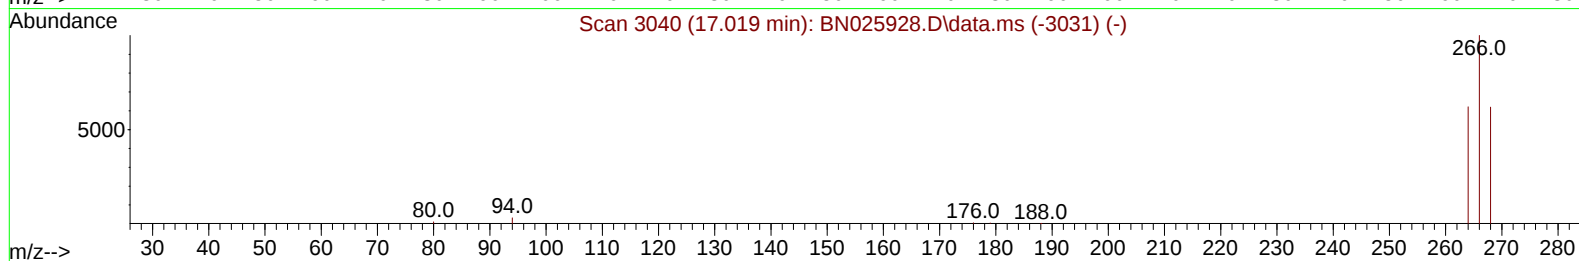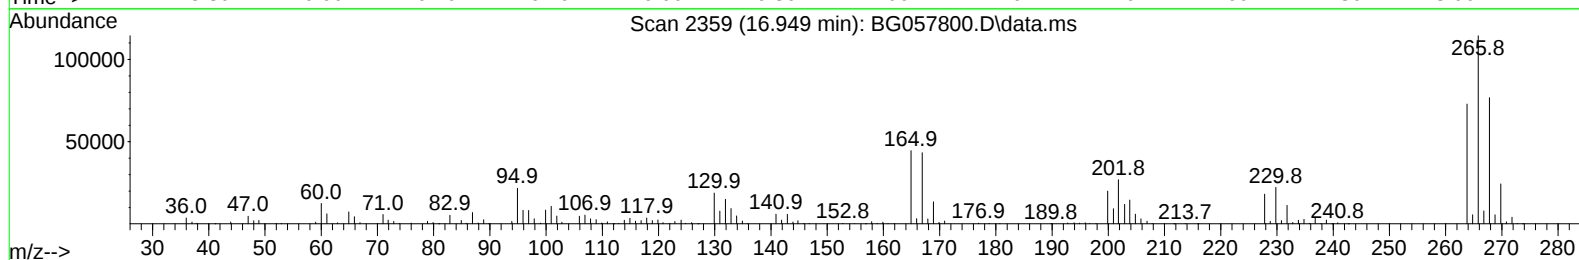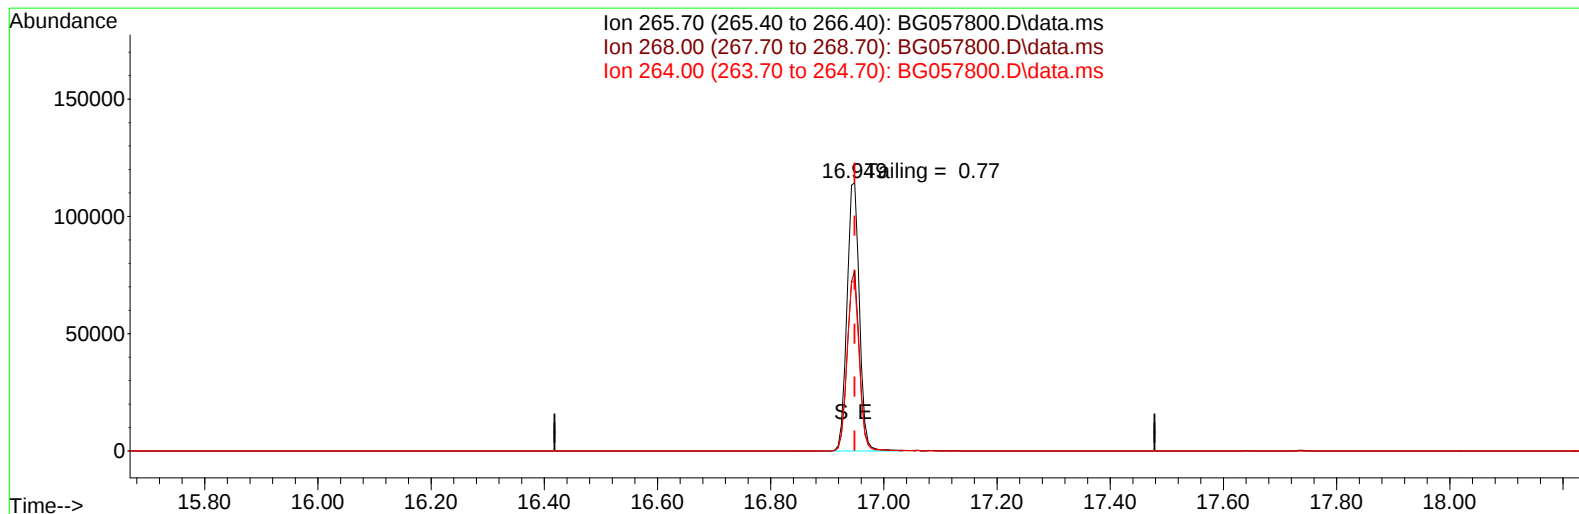

TIC: BG057800.D\data.ms

(70) Pentachlorophenol (C)

16.949min (+ 0.001) 28680.55 ng




response 174557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	67.12
264.00	64.70	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
Data File : BG057800.D
Acq On : 22 Jun 2023 7:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 22 13:34:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

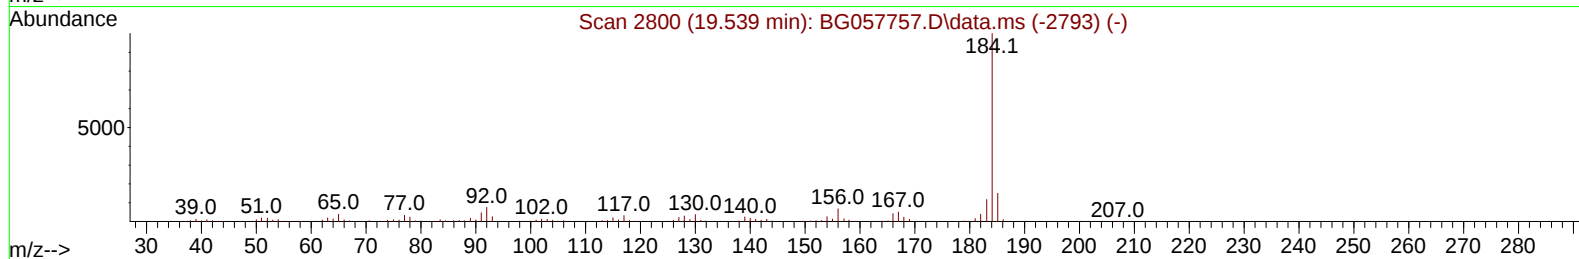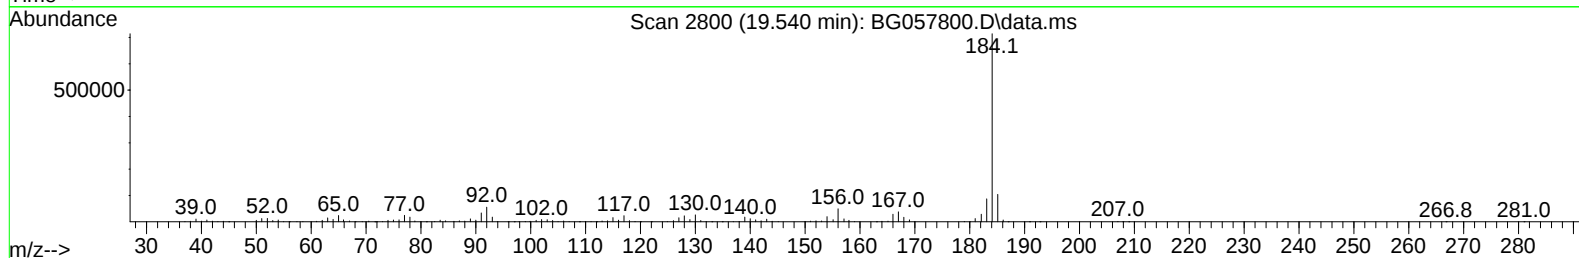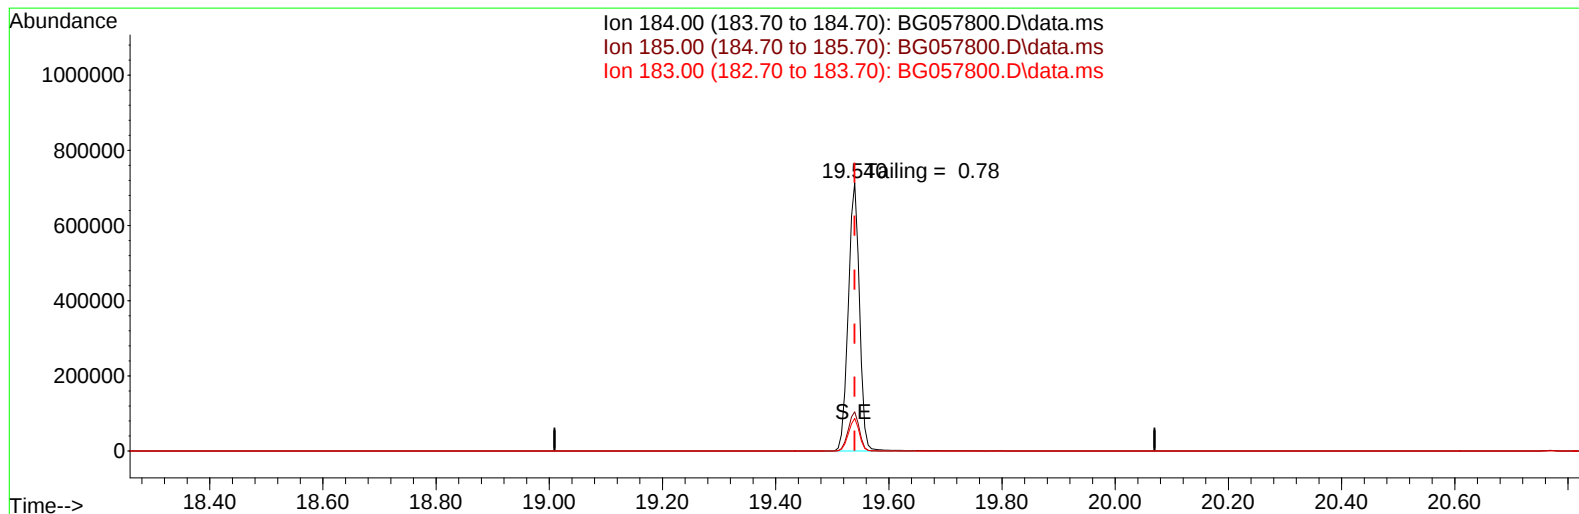

TIC: BG057800.D\data.ms

(77) Benzidine

19.540min (+ 0.001) 0.00 ng

response 985089

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.61
183.00	11.70	12.19
0.00	0.00	0.00