
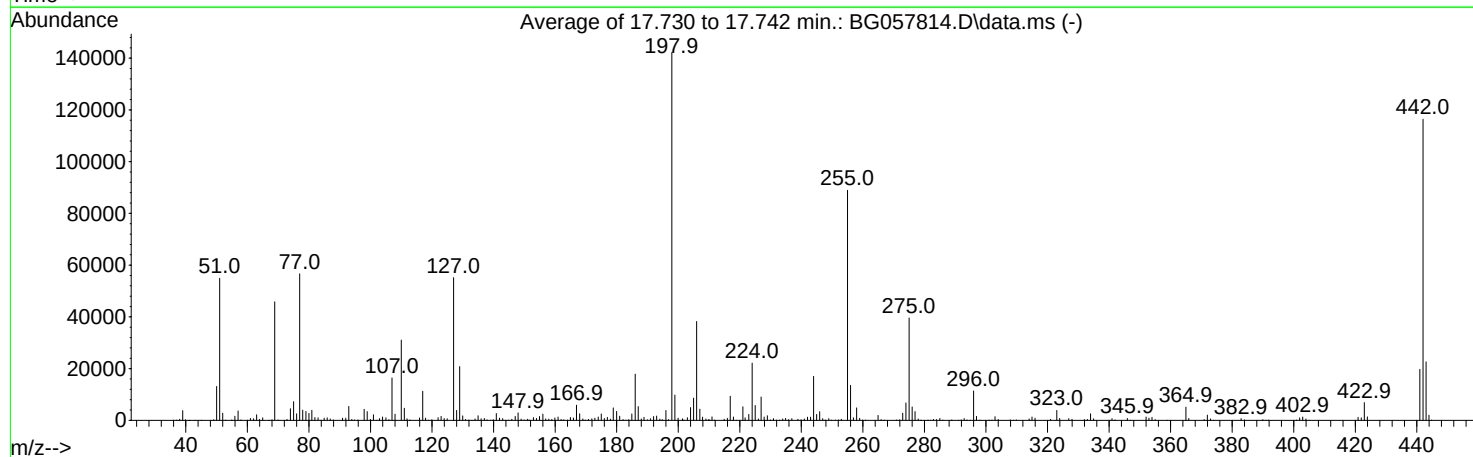


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
Data File : BG057814.D
Acq On : 22 Jun 2023 18:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 20 03:40:38 2023

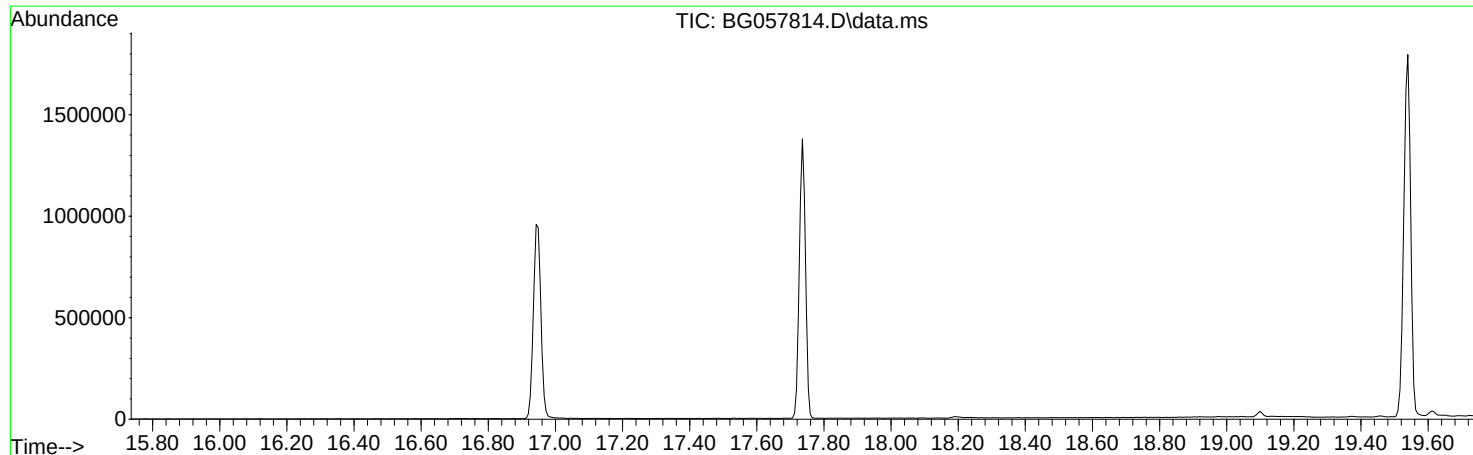

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	54907	PASS
68	69	0.00	2	0.6	284	PASS
69	198	0.00	100	32.2	45824	PASS
70	69	0.00	2	0.5	219	PASS
127	198	10	80	38.8	55152	PASS
197	198	0.00	2	0.2	339	PASS
198	198	100	100	100.0	142189	PASS
199	198	5	9	6.9	9795	PASS
275	198	10	60	27.8	39589	PASS
365	198	1	100	3.6	5135	PASS
441	198	0.01	100	13.9	19705	PASS
442	442	50	100	100.0	116389	PASS
443	442	15	24	19.5	22667	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/22/2023	BNA_G	<u>BG057814.D</u>
Compound Name	Response	Retention Time
DDT	472766	20.768
DDD	5466	20.38
DDE	0	19.823
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5466	478232	1.14

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
Data File : BG057814.D
Acq On : 22 Jun 2023 18:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 23 06:47:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

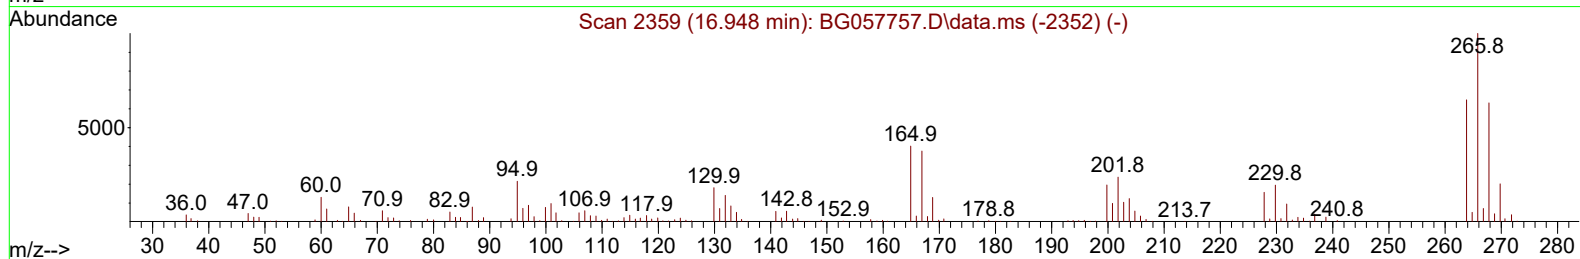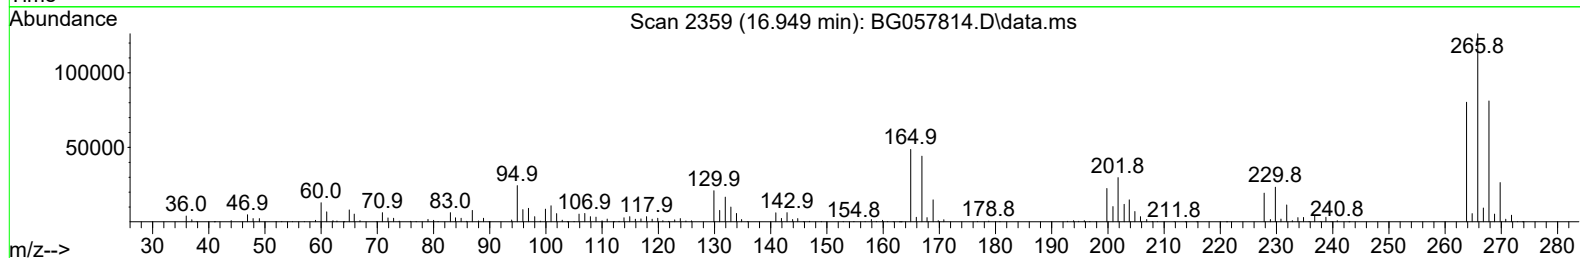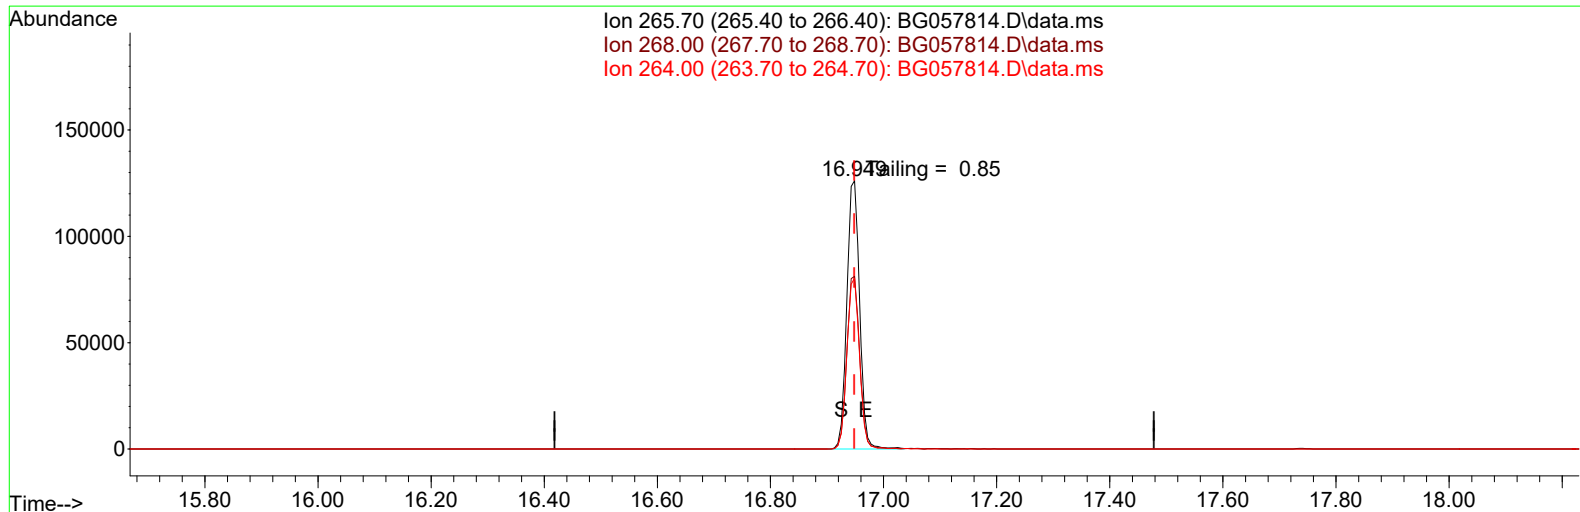

TIC: BG057814.D\data.ms

(70) Pentachlorophenol (C)

16.949min (+ 0.001) 30057.96 ng




response 197345

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.31
264.00	64.70	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062223\
Data File : BG057814.D
Acq On : 22 Jun 2023 18:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 23 06:47:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 03:40:38 2023
Response via : Initial Calibration

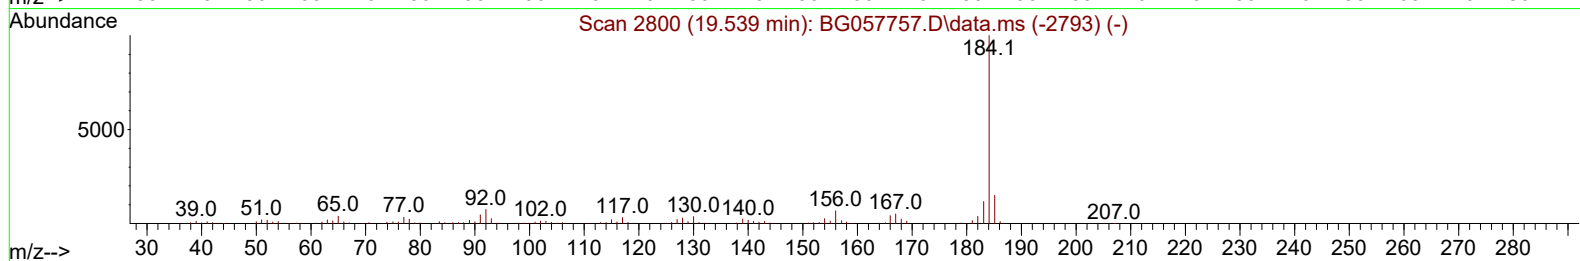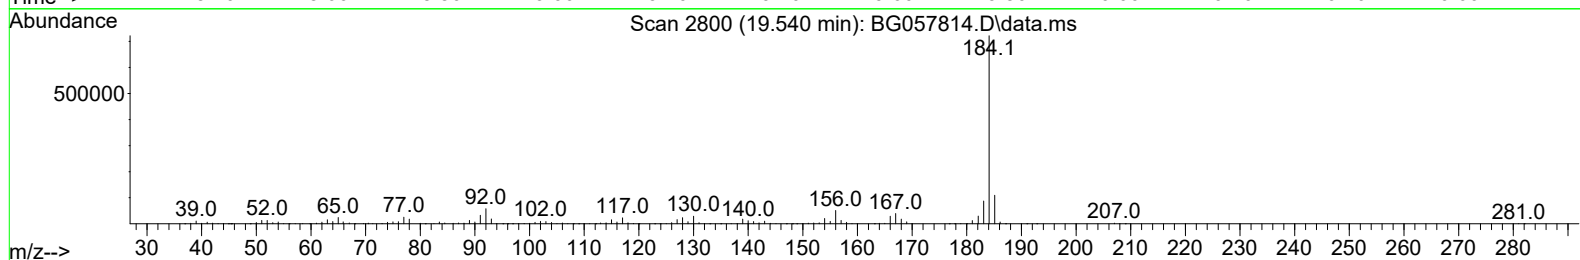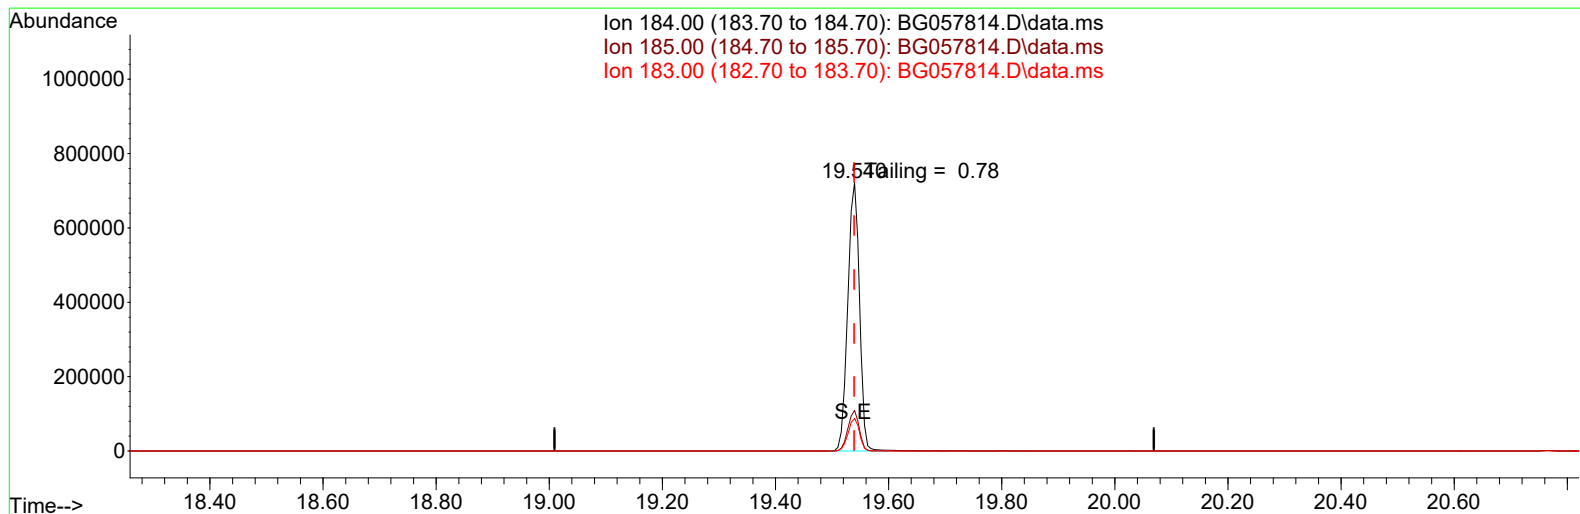

TIC: BG057814.D\data.ms

(77) Benzidine

19.540min (+ 0.001) 0.00 ng

response 1043927

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.16
183.00	11.70	12.09
0.00	0.00	0.00