

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054022.D
 Acq On : 23 Jun 2022 20:53
 Operator : CG/JU
 Sample : N3400-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AD6

Quant Time: Jun 23 23:05:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.072	152	19422	20.000	ng/ul	0.00
20) Naphthalene-d8	10.880	136	92155	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.699	164	74478	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.443	188	190695	20.000	ng/ul	0.00
79) Chrysene-d12	21.714	240	209998	20.000	ng/ul	0.00
88) Perylene-d12	24.969	264	204465	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.489	96	1895	4.642	ng/uL	-0.02
4) Pyridine-d5	3.912	84	12361	11.133	ng/ul	0.00
7) Phenol-d5	7.231	99	14956	10.749	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.390	67	32429	38.637	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.607	132	35978	32.425	ng/ul	0.00
15) 4-Methylphenol-d8	8.777	113	29226	24.635	ng/ul	0.00
21) Nitrobenzene-d5	9.235	128	23009	33.638	ng/ul	0.00
24) 2-Nitrophenol-d4	9.958	143	26367	36.279	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.498	165	54700	34.018	ng/ul	0.00
31) 4-Chloroaniline-d4	11.009	131	61847	30.445	ng/ul	0.00
46) Dimethylphthalate-d6	14.094	166	219928	37.536	ng/ul	0.00
49) Acenaphthylene-d8	14.394	160	230299	36.147	ng/ul	0.00
54) 4-Nitrophenol-d4	14.881	143	7724	9.628	ng/ul	0.00
60) Fluorene-d10	15.686	176	193683	36.802	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	38493	37.003	ng/ul	0.00
73) Anthracene-d10	17.537	188	347865	40.393	ng/ul	0.00
81) Pyrene-d10	19.822	212	451128	41.202	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.746	264	442842	42.907	ng/ul	-0.01
Target Compounds						
					Qvalue	
19) Hexachloroethane	9.176	117	484	1.008	ng/ul#	1
30) Naphthalene	10.933	128	11580	2.533	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054022.D
Acq On : 23 Jun 2022 20:53
Operator : CG/JU
Sample : N3400-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AD6

Quant Time: Jun 23 23:05:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration




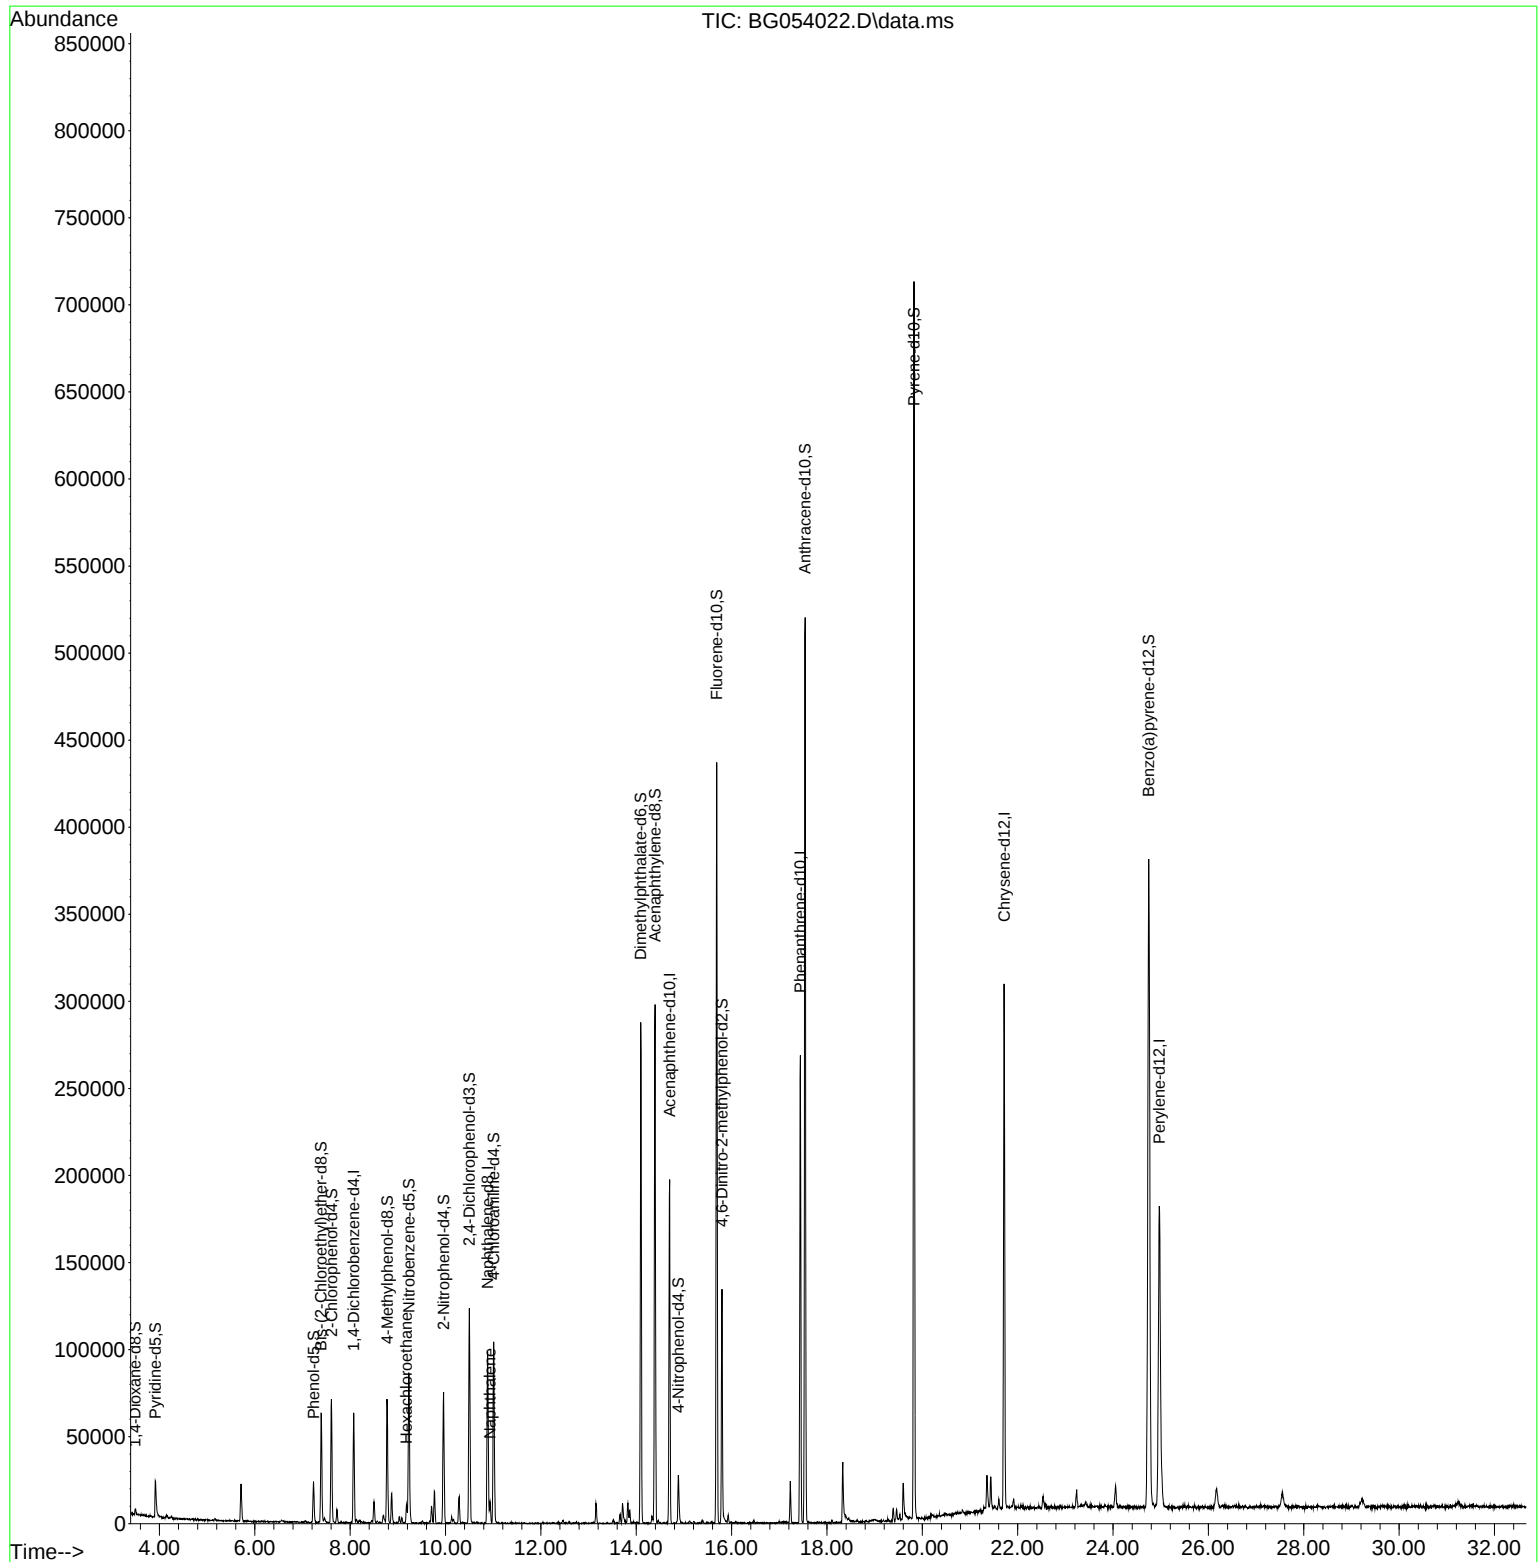


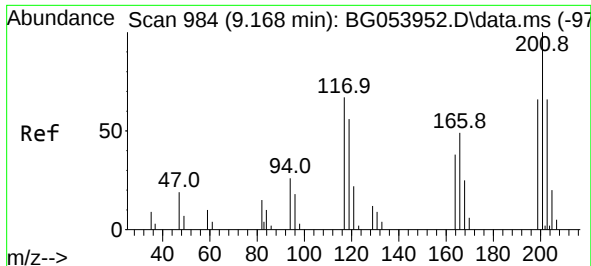

#19
Hexachloroethane
Concen: 1.008 ng/ul
RT: 9.176 min Scan# 91
Delta R.T. 0.006 min
Lab File: BG054022.D
Acq: 23 Jun 2022 20:53

Instrument :
BNA_G
ClientSampleId :
C0AD6

Tgt Ion:117 Resp: 484
Ion Ratio Lower Upper
117 100
201 0.0 117.4 176.0#
199 0.0 64.0 96.0#

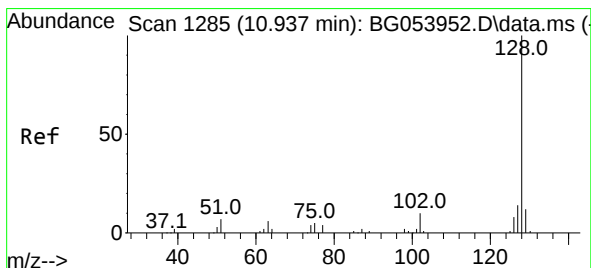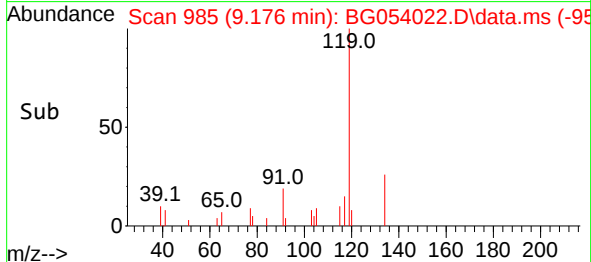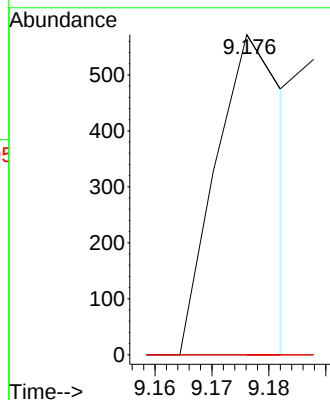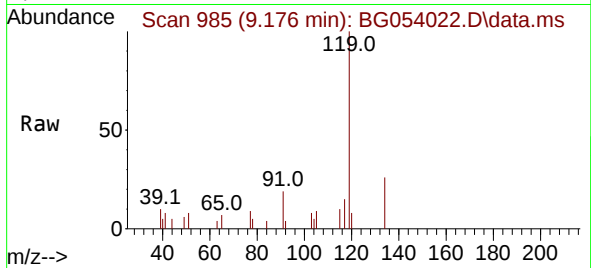

#30
Naphthalene
Concen: 2.533 ng/ul
RT: 10.933 min Scan# 1284
Delta R.T. -0.005 min
Lab File: BG054022.D
Acq: 23 Jun 2022 20:53

Tgt Ion:128 Resp: 11580
Ion Ratio Lower Upper
128 100
129 14.1 9.0 13.6#
127 17.0 11.1 16.7#

