

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054044.D
 Acq On : 24 Jun 2022 12:27
 Operator : CG/JU
 Sample : PB145683BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK683

Quant Time: Jun 24 23:53:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.073	152	23153	20.000	ng/u1	0.00
20) Naphthalene-d8	10.882	136	109643	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.695	164	91522	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.439	188	238443	20.000	ng/u1	0.00
79) Chrysene-d12	21.716	240	270390	20.000	ng/u1	0.00
88) Perylene-d12	24.971	264	261508	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.491	96	2800	5.754	ng/uL	-0.02
4) Pyridine-d5	3.908	84	40400	30.524	ng/u1	0.00
7) Phenol-d5	7.227	99	55040	33.182	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.392	67	33178	33.159	ng/u1	0.00
11) 2-Chlorophenol-d4	7.603	132	42768	32.333	ng/u1	0.00
15) 4-Methylphenol-d8	8.773	113	49735	35.166	ng/u1	0.00
21) Nitrobenzene-d5	9.231	128	23095	28.378	ng/u1	0.00
24) 2-Nitrophenol-d4	9.960	143	26863	31.066	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.500	165	55232	28.870	ng/u1	0.00
31) 4-Chloroaniline-d4	11.011	131	71264	29.486	ng/u1	0.00
46) Dimethylphthalate-d6	14.096	166	205870	28.593	ng/u1	0.00
49) Acenaphthylene-d8	14.390	160	223905	28.599	ng/u1	0.00
54) 4-Nitrophenol-d4	14.883	143	27397	27.790	ng/u1	0.00
60) Fluorene-d10	15.688	176	183418	28.361	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.800	200	32726	25.160	ng/u1	0.00
73) Anthracene-d10	17.539	188	311386	28.917	ng/u1	0.00
81) Pyrene-d10	19.824	212	420719	29.843	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.748	264	403322	30.554	ng/u1	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.779	70	1216	1.091 ng/u1#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054044.D
Acq On : 24 Jun 2022 12:27
Operator : CG/JU
Sample : PB145683BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK683


Quant Time: Jun 24 23:53:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

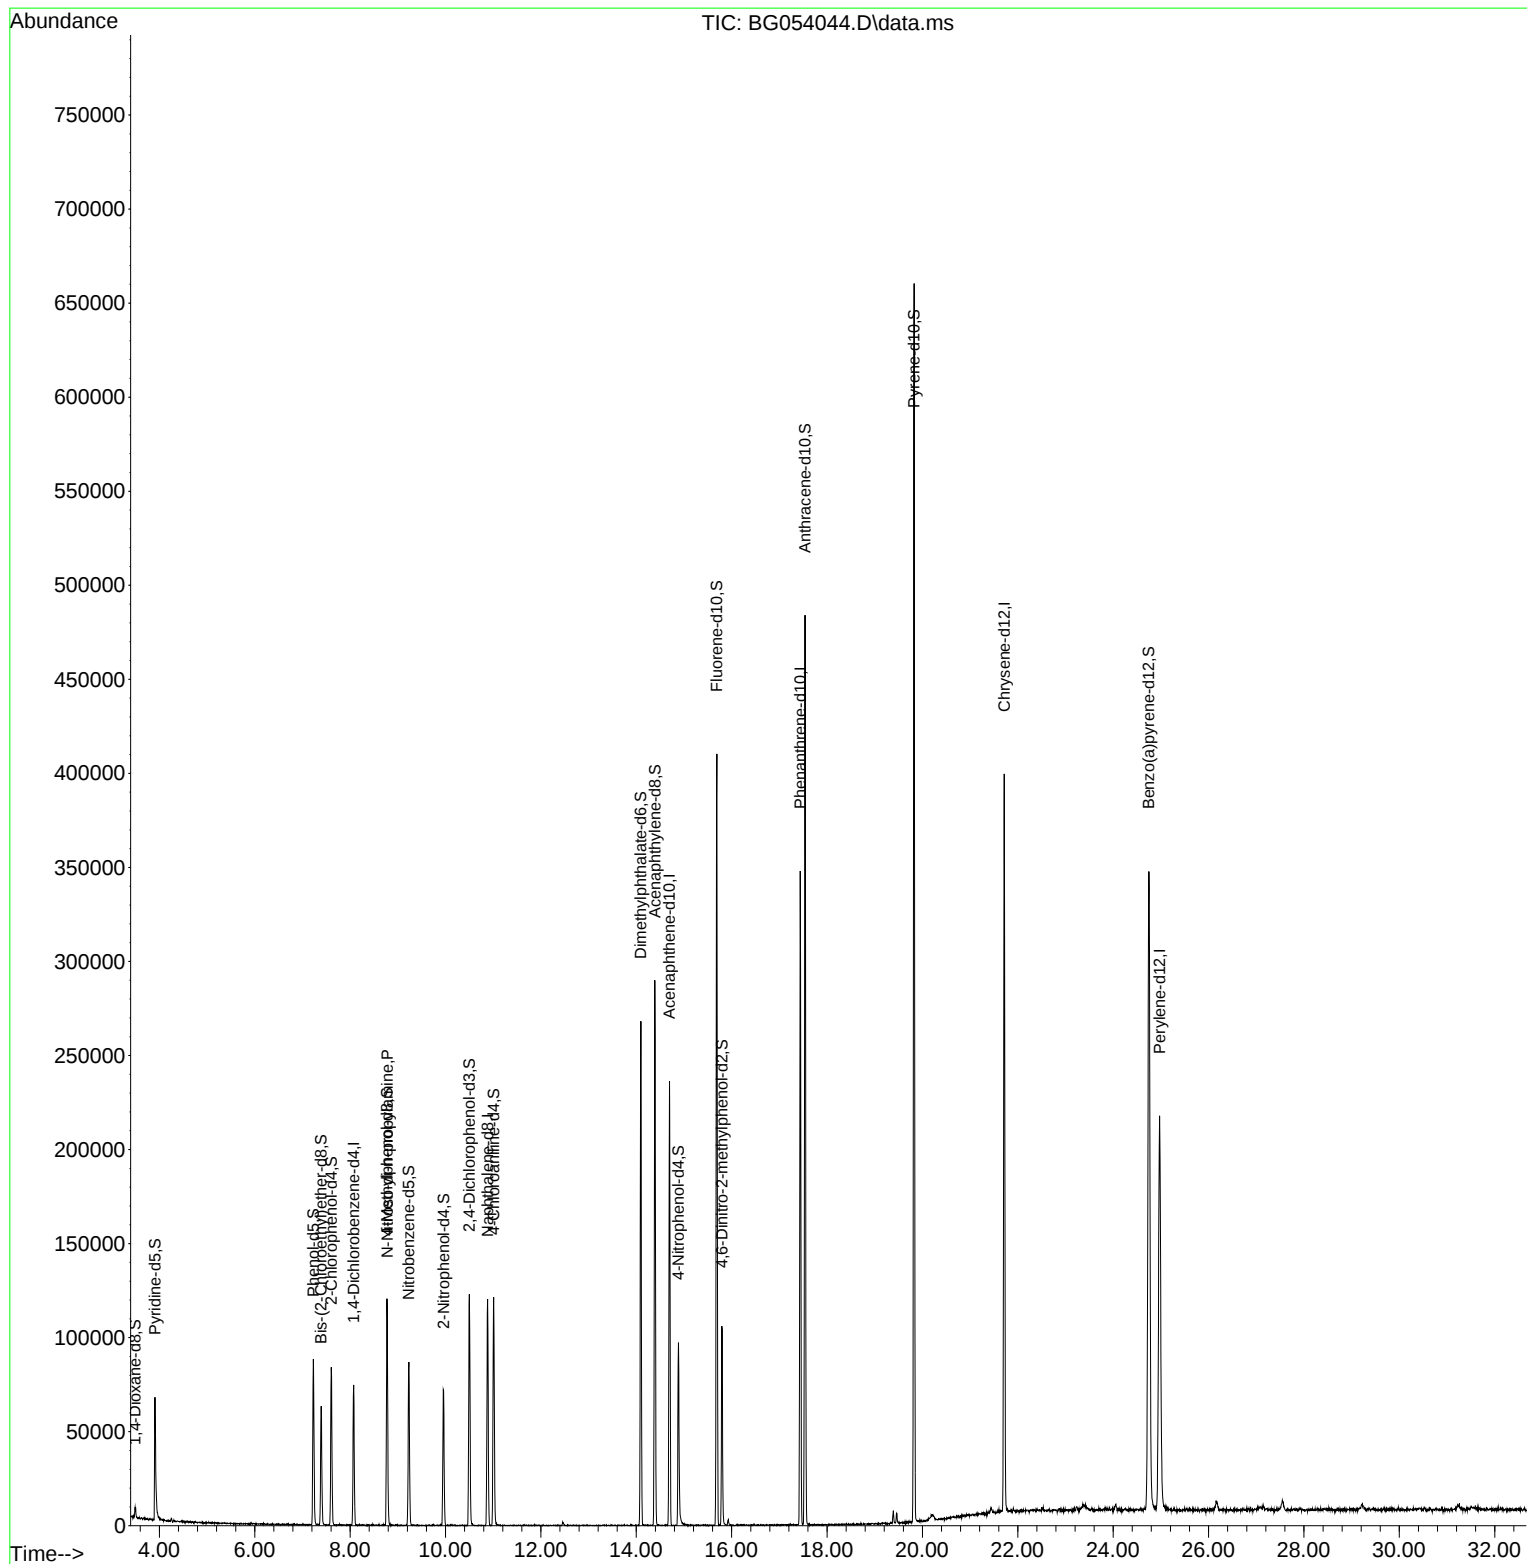

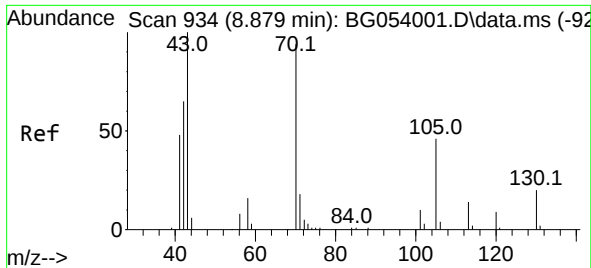

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.091 ng/ul
 RT: 8.779 min Scan# 917
 Delta R.T. -0.103 min
 Lab File: BG054044.D
 Acq: 24 Jun 2022 12:27

Instrument :
 BNA_G
 ClientSampleId :
 SBLK683

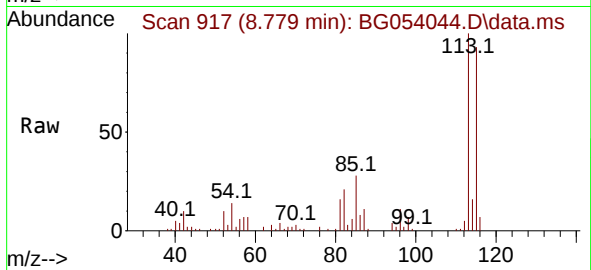

Tgt Ion:	70	Resp:	1216
Ion	Ratio	Lower	Upper
70	100		
42	344.4	50.2	75.4#
101	0.0	7.1	10.7#
130	0.0	15.5	23.3#

