




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054037.D
Acq On : 24 Jun 2022 7:16
Operator : CG/JU
Sample : N3395-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0163

Manual IntegrationsAPPROVED

Quant Time: Jun 24 07:54:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/24/2022
Supervised By :mohammad ahmed 06/29/2022

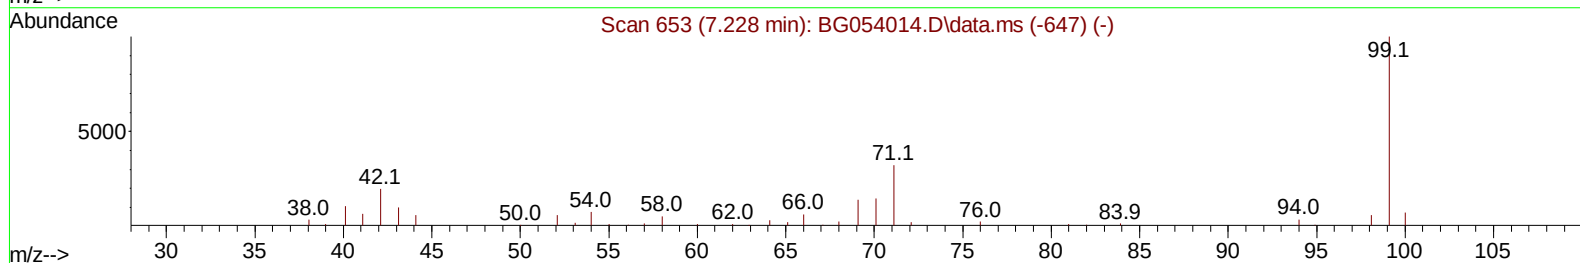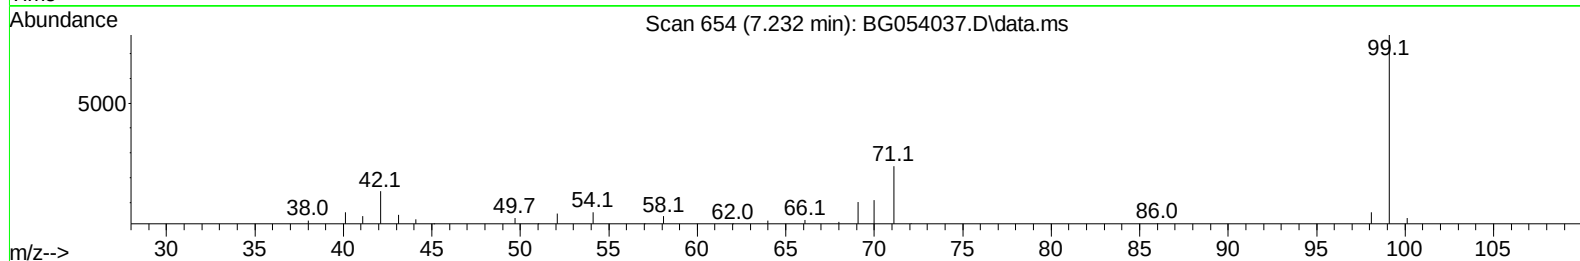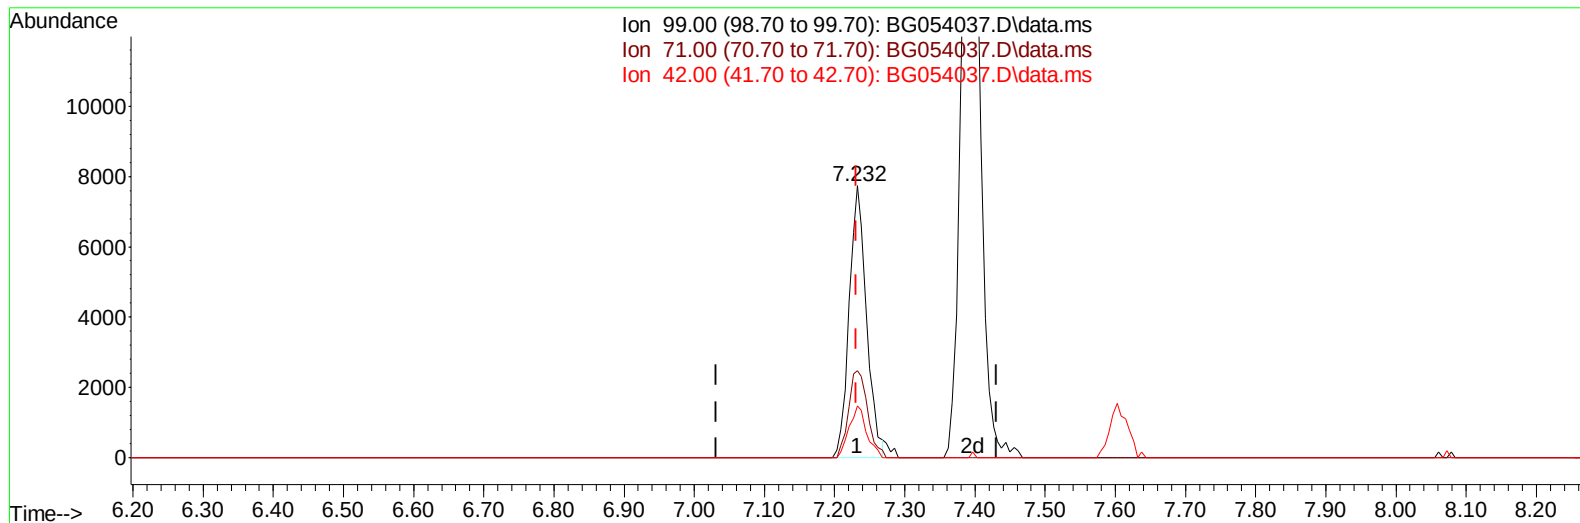

TIC: BG054037.D\data.ms

(7) Phenol-d5 (S)

7.232min (+ 0.001) 9.72 ng/u1

response 13276

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	39.00	32.06
42.00	22.60	18.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054037.D
Acq On : 24 Jun 2022 7:16
Operator : CG/JU
Sample : N3395-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0163

Manual IntegrationsAPPROVED

Quant Time: Jun 24 07:54:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/24/2022
Supervised By :mohammad ahmed 06/29/2022

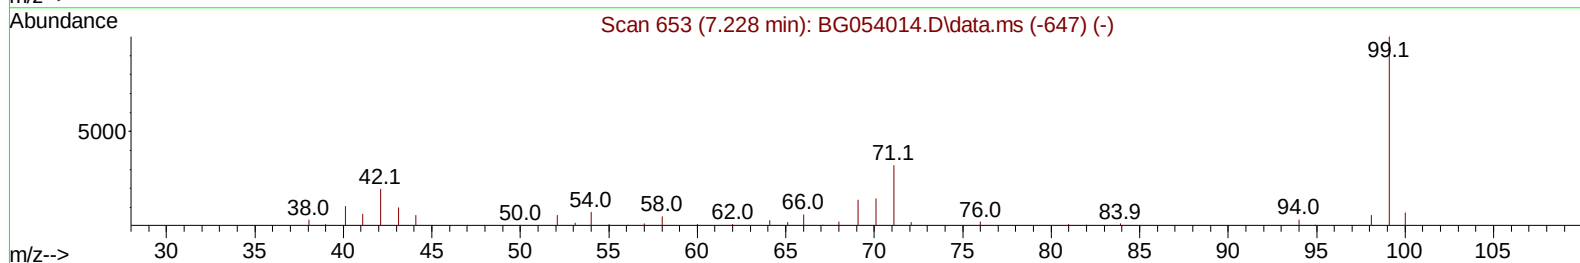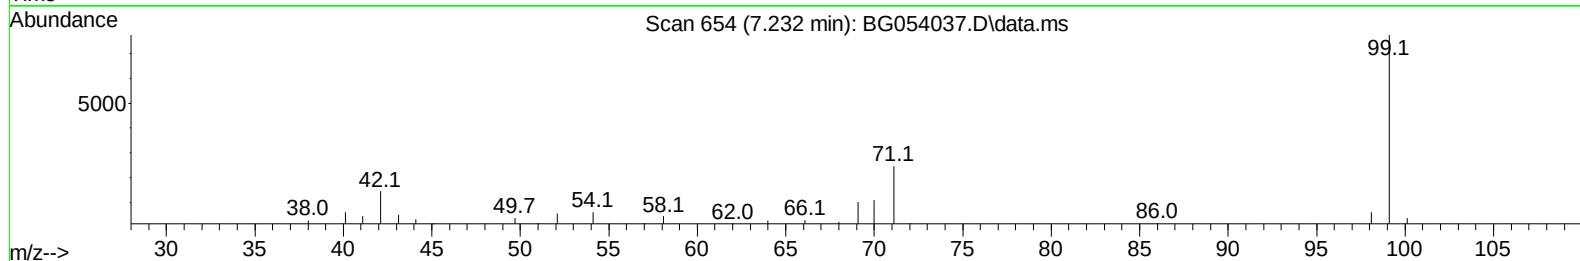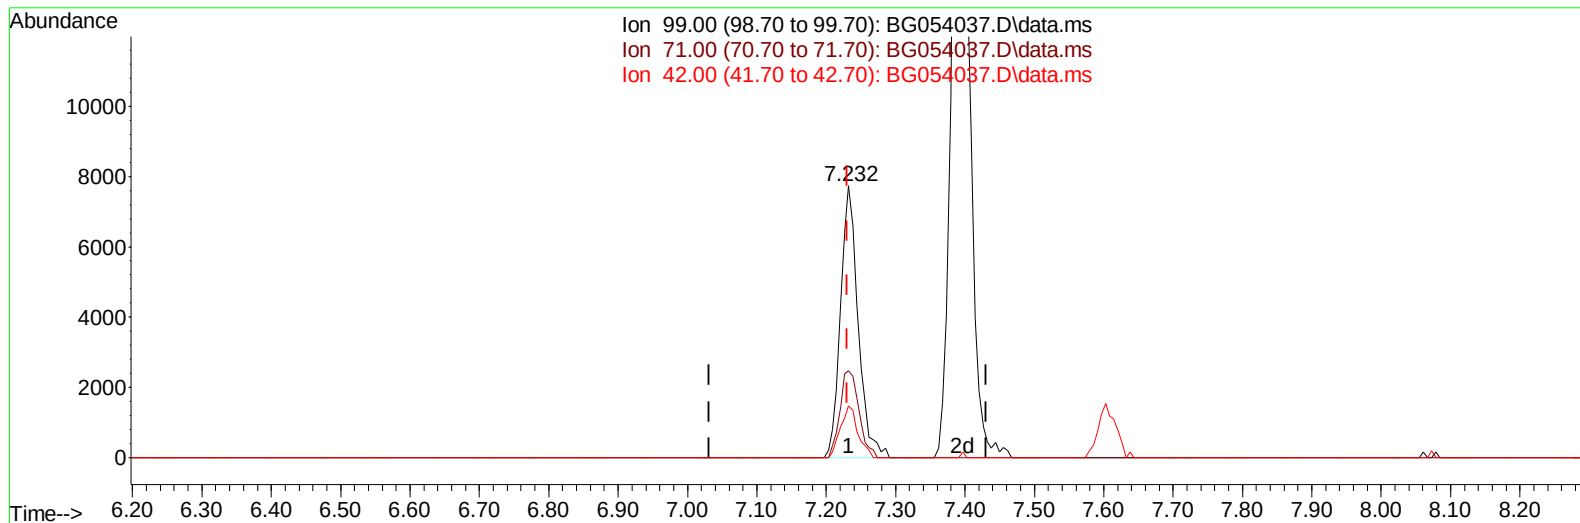

TIC: BG054037.D\data.ms

(7) Phenol-d5 (S)

7.232min (+ 0.001) 9.93 ng/ul m

response 13574

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	39.00	32.06
42.00	22.60	18.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054037.D
 Acq On : 24 Jun 2022 7:16
 Operator : CG/JU
 Sample : N3395-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0163

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022
 Supervised By :mohammad ahmed 06/29/2022

Quant Time: Jun 24 07:54:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.078	152	19072	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	90575	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.694	164	75377	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.438	188	190375	20.000	ng/ul	0.00
79) Chrysene-d12	21.715	240	210718	20.000	ng/ul	0.00
88) Perylene-d12	24.970	264	206848	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.496	96	2052	5.119	ng/uL	-0.01
4) Pyridine-d5	3.919	84	8433	7.735	ng/ul	0.00
7) Phenol-d5	7.232	99	13574m	9.935	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.391	67	32112	38.961	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.608	132	33924	31.135	ng/ul	0.00
15) 4-Methylphenol-d8	8.778	113	26870	23.064	ng/ul	0.00
21) Nitrobenzene-d5	9.230	128	22796	33.908	ng/ul	0.00
24) 2-Nitrophenol-d4	9.959	143	25140	35.194	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.499	165	50117	31.711	ng/ul	0.00
31) 4-Chloroaniline-d4	11.010	131	55899	27.997	ng/ul	0.00
46) Dimethylphthalate-d6	14.095	166	208688	35.193	ng/ul	0.00
49) Acenaphthylene-d8	14.389	160	223102	34.600	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.888	143	6343	7.812	ng/ul	0.00
60) Fluorene-d10	15.687	176	185651	34.855	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.799	200	36426	35.075	ng/ul	0.00
73) Anthracene-d10	17.538	188	350134	40.724	ng/ul	0.00
81) Pyrene-d10	19.824	212	450415	40.996	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.753	264	440291	42.169	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054037.D
Acq On : 24 Jun 2022 7:16
Operator : CG/JU
Sample : N3395-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0163

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/24/2022
Supervised By :mohammad ahmed 06/29/2022

Quant Time: Jun 24 07:54:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

