




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054052.D
Acq On : 24 Jun 2022 17:47
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Manual IntegrationsAPPROVED

Quant Time: Jun 24 23:53:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :mohammad ahmed 06/29/2022

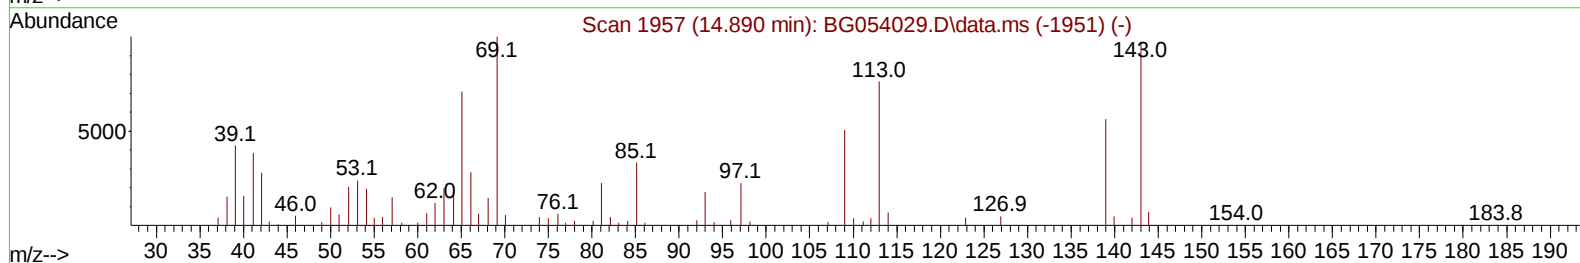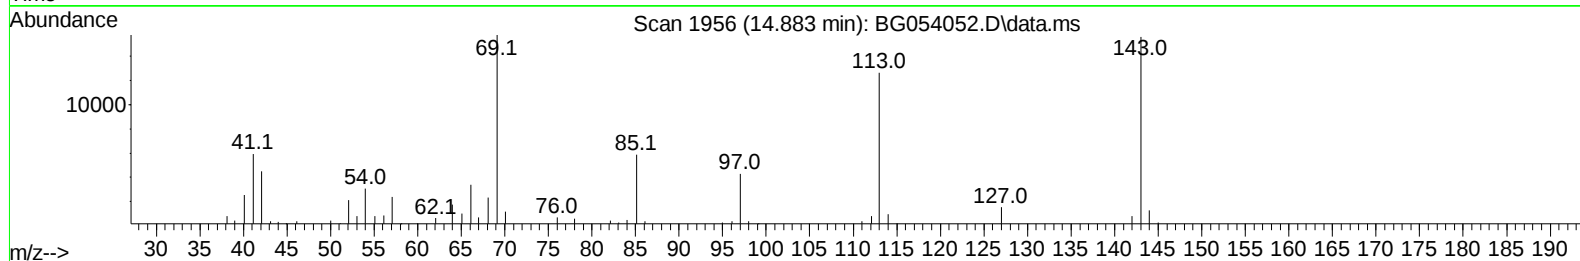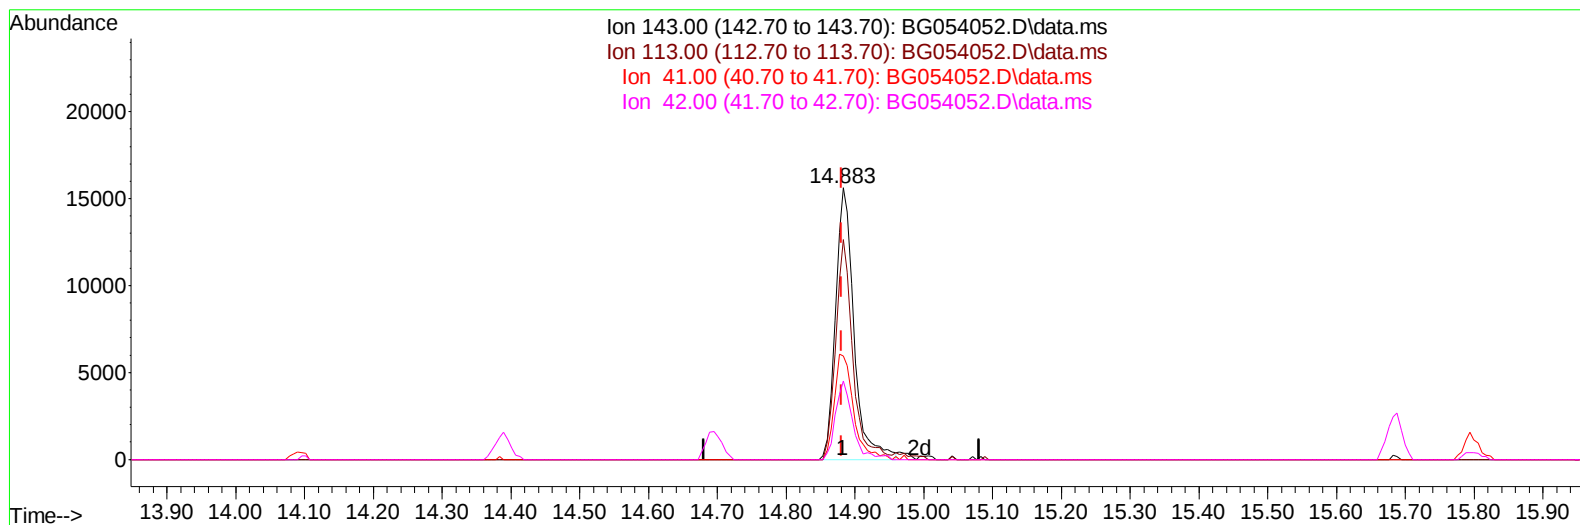

TIC: BG054052.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.883min (+ 0.002) 28.81 ng/u1

response 28942

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.90	81.04
41.00	51.40	38.04#
42.00	37.10	28.86#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054052.D
Acq On : 24 Jun 2022 17:47
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Manual IntegrationsAPPROVED

Quant Time: Jun 24 23:53:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :mohammad ahmed 06/29/2022

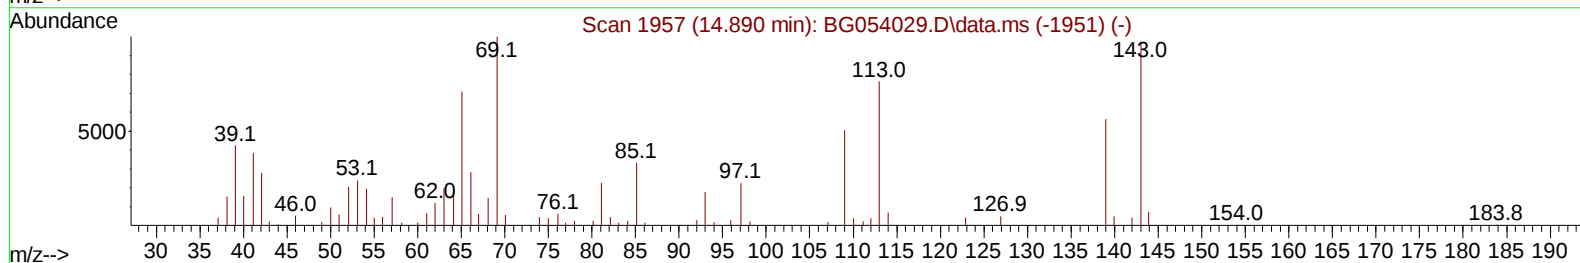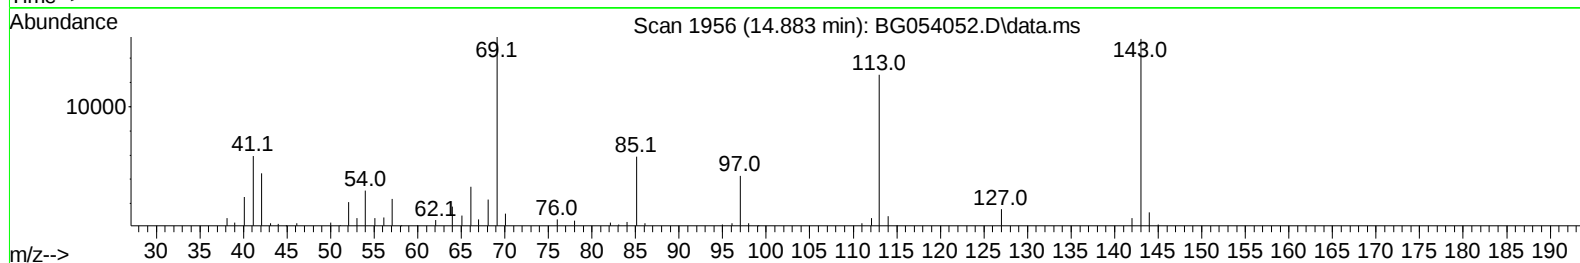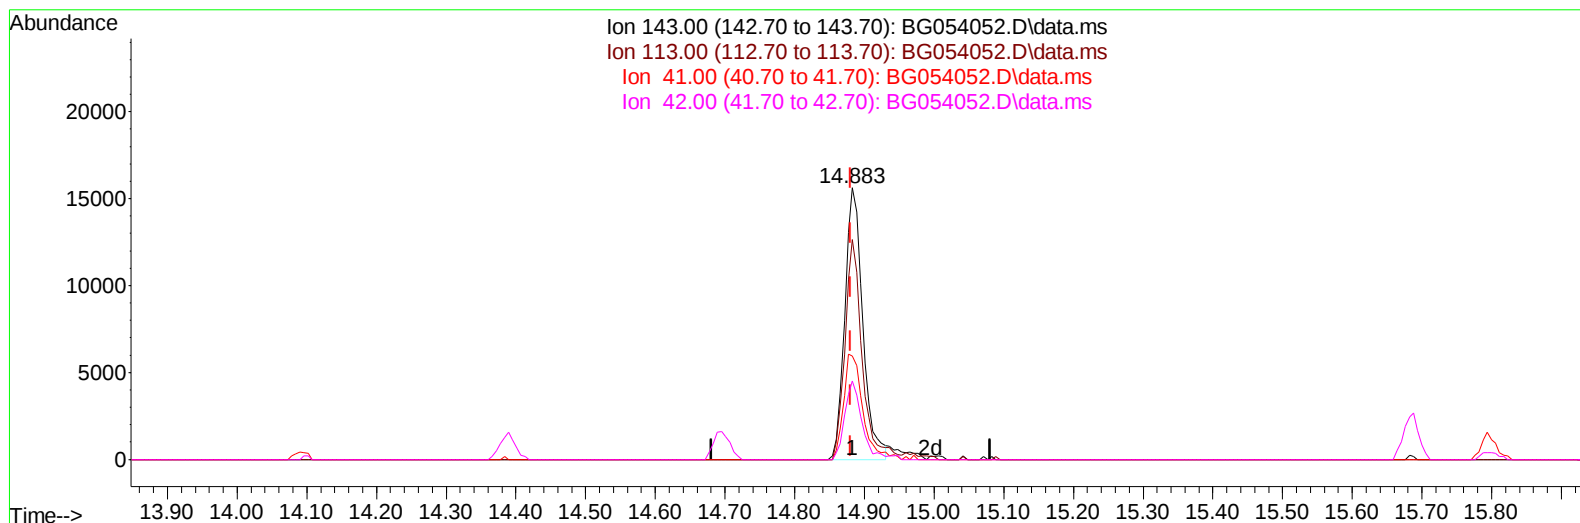

TIC: BG054052.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.883min (+ 0.002) 27.87 ng/ul m

response 28000

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	83.90	81.04
41.00	51.40	38.04#
42.00	37.10	28.86#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054052.D
 Acq On : 24 Jun 2022 17:47
 Operator : CG/JU
 Sample : PB145691BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK691

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :mohammad ahmed 06/29/2022

Quant Time: Jun 24 23:53:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.073	152	24298	20.000	ng/ul	0.00
20) Naphthalene-d8	10.882	136	115427	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.695	164	93275	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.439	188	239139	20.000	ng/ul	0.00
79) Chrysene-d12	21.710	240	262734	20.000	ng/ul	0.00
88) Perylene-d12	24.971	264	255401	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.491	96	2907	5.692	ng/uL	-0.02
4) Pyridine-d5	3.908	84	42419	30.539	ng/ul	0.00
7) Phenol-d5	7.227	99	57880	33.250	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.392	67	35370	33.684	ng/ul	0.00
11) 2-Chlorophenol-d4	7.603	132	45349	32.669	ng/ul	0.00
15) 4-Methylphenol-d8	8.773	113	51734	34.856	ng/ul	0.00
21) Nitrobenzene-d5	9.231	128	23596	27.541	ng/ul	0.00
24) 2-Nitrophenol-d4	9.954	143	27572	30.288	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.500	165	58092	28.843	ng/ul	0.00
31) 4-Chloroaniline-d4	11.011	131	76222	29.957	ng/ul	0.00
46) Dimethylphthalate-d6	14.096	166	216677	29.529	ng/ul	0.00
49) Acenaphthylene-d8	14.390	160	229838	28.805	ng/ul	0.00
54) 4-Nitrophenol-d4	14.883	143	28000m	27.868	ng/ul	0.00
60) Fluorene-d10	15.688	176	187006	28.372	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.794	200	33382	25.589	ng/ul	0.00
73) Anthracene-d10	17.539	188	319488	29.583	ng/ul	0.00
81) Pyrene-d10	19.824	212	409086	29.863	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.748	264	394702	30.616	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054052.D
Acq On : 24 Jun 2022 17:47
Operator : CG/JU
Sample : PB145691BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK691

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :mohammad ahmed 06/29/2022

Quant Time: Jun 24 23:53:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

