

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054025.D
 Acq On : 23 Jun 2022 22:50
 Operator : CG/JU
 Sample : N3400-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA3

Quant Time: Jun 23 23:49:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.076	152	19849	20.000	ng/ul	0.00
20) Naphthalene-d8	10.885	136	91058	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.698	164	73728	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.442	188	192483	20.000	ng/ul	0.00
79) Chrysene-d12	21.713	240	215336	20.000	ng/ul	0.00
88) Perylene-d12	24.968	264	213346	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.493	96	2102	5.039	ng/uL	-0.01
4) Pyridine-d5	3.910	84	14526	12.802	ng/ul	0.00
7) Phenol-d5	7.230	99	14789	10.400	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.395	67	32902	38.357	ng/ul	0.00
11) 2-Chlorophenol-d4	7.606	132	34933	30.806	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	29678	24.477	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	23424	34.657	ng/ul	0.00
24) 2-Nitrophenol-d4	9.956	143	26077	36.312	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.497	165	56824	35.764	ng/ul	0.00
31) 4-Chloroaniline-d4	11.008	131	60373	30.078	ng/ul	0.00
46) Dimethylphthalate-d6	14.099	166	223031	38.453	ng/ul	0.00
49) Acenaphthylene-d8	14.392	160	227060	36.001	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	8867	11.165	ng/ul	0.01
60) Fluorene-d10	15.685	176	192702	36.988	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.797	200	41964	39.965	ng/ul	0.00
73) Anthracene-d10	17.542	188	341129	39.243	ng/ul	0.00
81) Pyrene-d10	19.821	212	446607	39.778	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.751	264	437038	40.582	ng/ul	0.00
Target Compounds						
30) Naphthalene	10.932	128	14610	3.234	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054025.D
Acq On : 23 Jun 2022 22:50
Operator : CG/JU
Sample : N3400-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA3

Quant Time: Jun 23 23:49:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

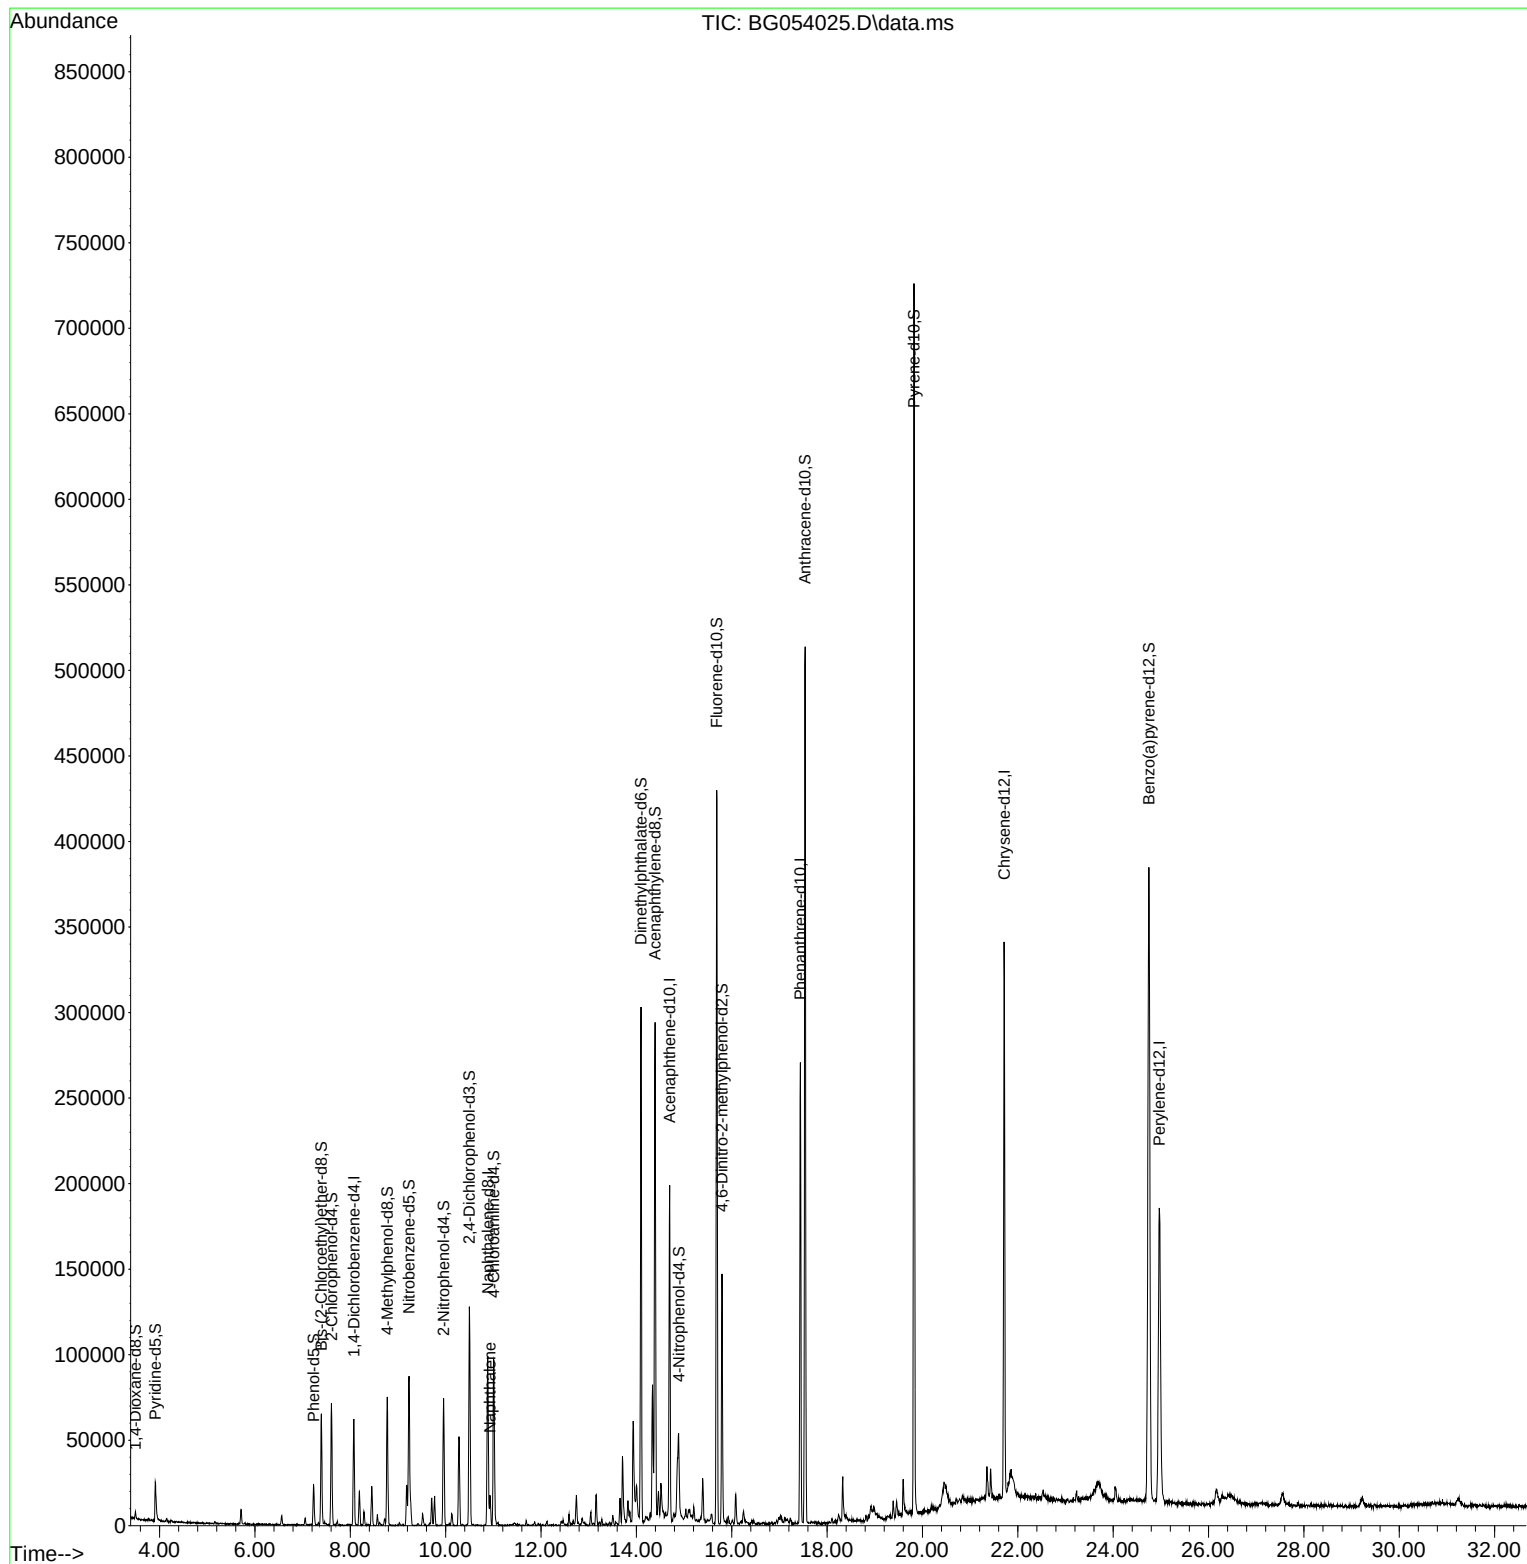

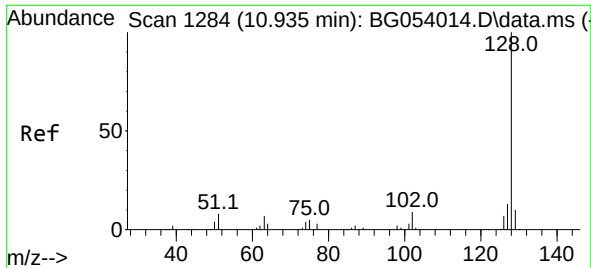

#30

Naphthalene

Concen: 3.234 ng/ul

RT: 10.932 min Scan# 1

Delta R.T. -0.007 min

Lab File: BG054025.D


Acq: 23 Jun 2022 22:50

Instrument :

BNA_G

ClientSampleId :

C0AA3

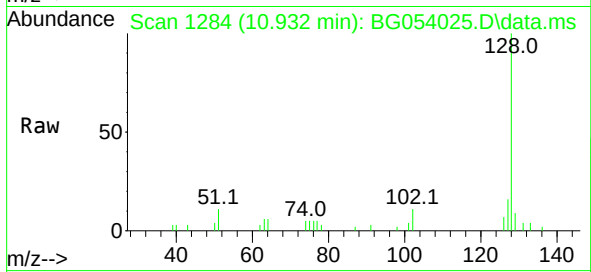

Tgt Ion:128 Resp: 14610

Ion Ratio Lower Upper

128 100

129 9.4 9.0 13.6

127 15.9 11.1 16.7

