

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
 Data File : BG054028.D
 Acq On : 24 Jun 2022 00:47
 Operator : CG/JU
 Sample : N3400-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AD9

Quant Time: Jun 24 01:27:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 20 15:29:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.072	152	21047	20.000	ng/ul	0.00
20) Naphthalene-d8	10.880	136	98823	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.699	164	79799	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.443	188	203644	20.000	ng/ul	0.00
79) Chrysene-d12	21.715	240	222799	20.000	ng/ul	0.00
88) Perylene-d12	24.975	264	224061	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.495	96	2058	4.652	ng/uL	-0.01
4) Pyridine-d5	3.912	84	17790	14.786	ng/ul	0.00
7) Phenol-d5	7.231	99	14674	9.732	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.390	67	36224	39.826	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.608	132	37563	31.240	ng/ul	0.00
15) 4-Methylphenol-d8	8.777	113	29322	22.807	ng/ul	0.00
21) Nitrobenzene-d5	9.235	128	25684	35.015	ng/ul	0.00
24) 2-Nitrophenol-d4	9.958	143	27858	35.744	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.498	165	59128	34.290	ng/ul	0.00
31) 4-Chloroaniline-d4	11.009	131	73783	33.870	ng/ul	0.00
46) Dimethylphthalate-d6	14.100	166	220680	35.153	ng/ul	0.00
49) Acenaphthylene-d8	14.394	160	251438	36.834	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	6943	8.077	ng/ul	0.00
60) Fluorene-d10	15.686	176	207878	36.865	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	38926	35.040	ng/ul	0.00
73) Anthracene-d10	17.537	188	357571	38.880	ng/ul	0.00
81) Pyrene-d10	19.823	212	459974	39.596	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.752	264	445864	39.422	ng/ul	0.00


Target Compounds					Qvalue	
8) Phenol	7.255	94	1974	1.255	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062322\
Data File : BG054028.D
Acq On : 24 Jun 2022 00:47
Operator : CG/JU
Sample : N3400-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AD9

Quant Time: Jun 24 01:27:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062022.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 20 15:29:13 2022
Response via : Initial Calibration

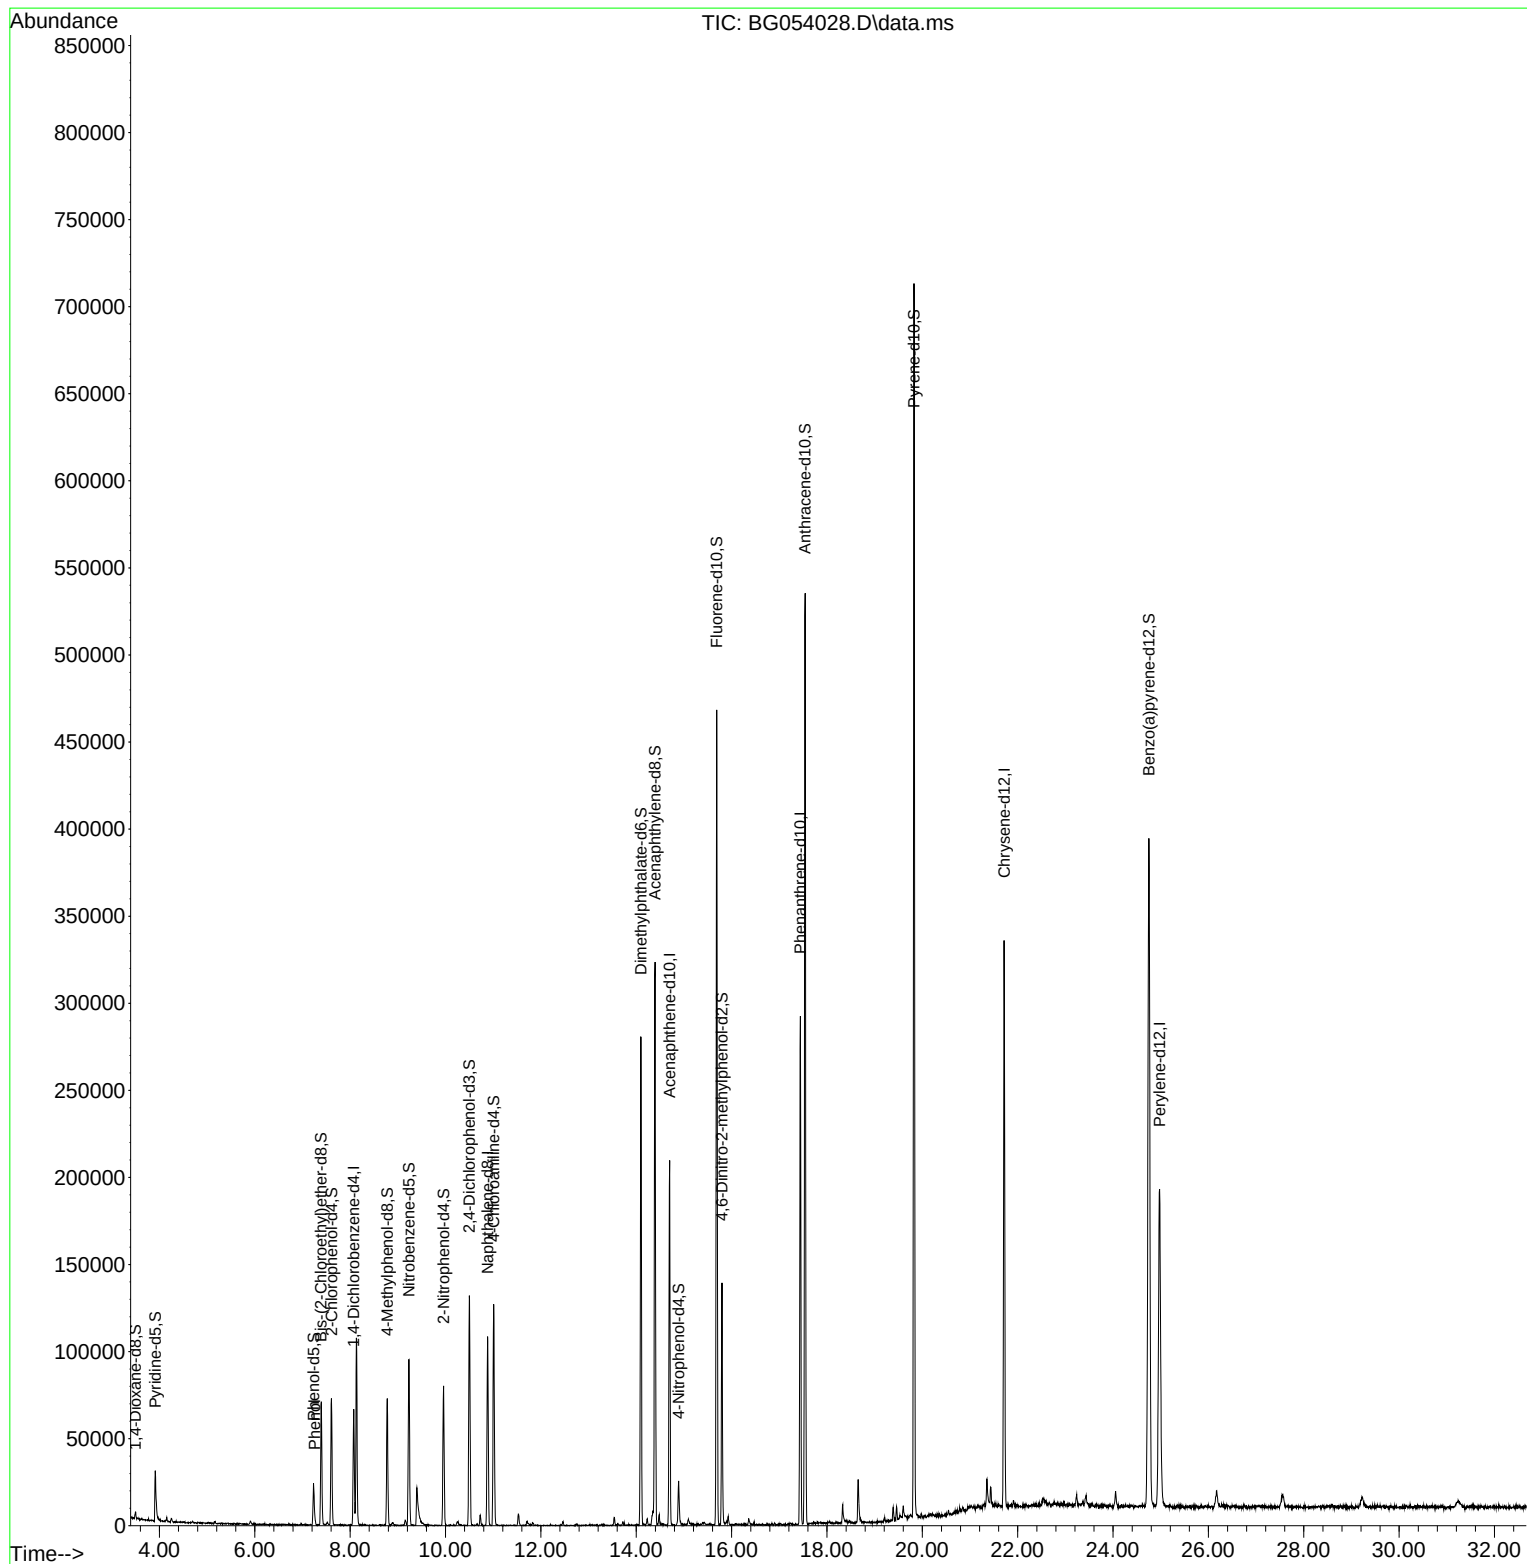

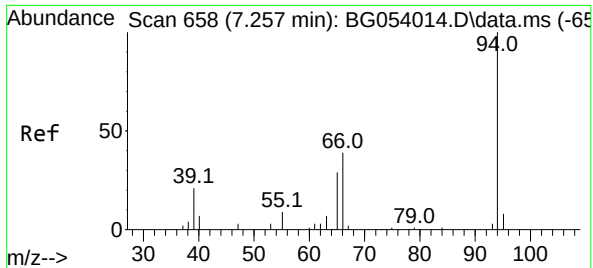

#8
Phenol
Concen: 1.255 ng/ul
RT: 7.255 min Scan# 61
Delta R.T. 0.001 min
Lab File: BG054028.D
Acq: 24 Jun 2022 00:47

Instrument :
BNA_G
ClientSampleId :
C0AD9

Tgt Ion: 94 Resp: 1974
Ion Ratio Lower Upper
94 100
65 46.4 24.1 36.1#
66 45.8 32.5 48.7

